

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050581.D
 Acq On : 01 Sep 2022 15:23
 Operator : SY/MD
 Sample : N4458-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050581.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	101	rBV	71635	87755	8.49%	1.167%
2	1.729	117	121	129	rVB2	7029	7845	0.76%	0.104%
3	1.906	168	176	189	rVB	67291	88569	8.56%	1.178%
4	2.221	273	274	275	rBV	300	109	0.01%	0.001%
5	2.562	369	380	398	rBV	160364	260387	25.18%	3.463%
6	2.706	419	425	428	rBV3	397	442	0.04%	0.006%
7	2.880	475	479	481	rBV	256	225	0.02%	0.003%
8	3.186	559	574	603	rBV	28519	68178	6.59%	0.907%
9	3.324	611	617	621	rVB	355	407	0.04%	0.005%
10	3.343	621	623	626	rVB	314	136	0.01%	0.002%
11	3.378	627	634	636	rBV2	338	393	0.04%	0.005%
12	3.411	642	644	647	rVB2	254	156	0.02%	0.002%
13	3.459	657	659	661	rBV2	222	126	0.01%	0.002%
14	3.700	731	734	736	rBV	333	259	0.03%	0.003%
15	3.813	759	769	772	rBV	332	631	0.06%	0.008%
16	3.877	786	789	791	rBV	305	201	0.02%	0.003%
17	3.909	795	799	804	rVB2	240	251	0.02%	0.003%
18	4.041	838	840	843	rBV	321	241	0.02%	0.003%
19	4.073	848	850	855	rVB	244	224	0.02%	0.003%
20	4.102	855	859	860	rBV	203	112	0.01%	0.001%
21	4.157	872	876	879	rBV2	205	215	0.02%	0.003%
22	4.218	890	895	897	rBV2	305	251	0.02%	0.003%
23	4.298	917	920	921	rBV2	213	144	0.01%	0.002%
24	4.356	934	938	940	rBV	238	172	0.02%	0.002%
25	4.385	944	947	950	rBV2	181	140	0.01%	0.002%
26	4.632	1010	1024	1067	rBV3	107493	347148	33.57%	4.617%
27	5.063	1139	1158	1180	rBV2	189950	429503	41.53%	5.712%
28	5.179	1192	1194	1199	rVB4	612	504	0.05%	0.007%
29	5.218	1203	1206	1208	rVV2	230	104	0.01%	0.001%
30	5.288	1220	1228	1233	rBV3	1075	1412	0.14%	0.019%
31	5.372	1249	1254	1255	rBV	323	320	0.03%	0.004%
32	5.423	1265	1270	1275	rBV2	317	426	0.04%	0.006%
33	5.468	1282	1284	1288	rBV2	233	157	0.02%	0.002%
34	5.513	1294	1298	1302	rVB2	245	206	0.02%	0.003%
35	5.542	1302	1307	1312	rBV2	213	310	0.03%	0.004%
36	5.568	1312	1315	1320	rVV2	243	240	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050581.D
 Acq On : 01 Sep 2022 15:23
 Operator : SY/MD
 Sample : N4458-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

37	5.591	1320	1322	1326	rVB	190	150	0.01%	0.002%
38	5.722	1343	1363	1388	rBV2	378726	1034088	100.00%	13.752%
39	6.009	1446	1452	1454	rBV2	333	403	0.04%	0.005%
40	6.060	1463	1468	1469	rBV	258	239	0.02%	0.003%
41	6.099	1478	1480	1483	rVB	230	115	0.01%	0.002%
42	6.115	1483	1485	1486	rBV	396	208	0.02%	0.003%
43	6.169	1498	1502	1505	rBV	182	170	0.02%	0.002%
44	6.250	1513	1527	1551	rBV	304097	589033	56.96%	7.834%
45	6.497	1601	1604	1607	rVV2	202	141	0.01%	0.002%
46	6.533	1607	1615	1622	rVB5	1357	1998	0.19%	0.027%
47	6.603	1633	1637	1640	rBV3	467	317	0.03%	0.004%
48	6.690	1650	1664	1688	rBV	247671	481957	46.61%	6.410%
49	6.835	1706	1709	1710	rBV	221	132	0.01%	0.002%
50	6.861	1713	1717	1721	rBV2	241	216	0.02%	0.003%
51	7.041	1770	1773	1775	rBV	191	141	0.01%	0.002%
52	7.089	1783	1788	1789	rBV	347	208	0.02%	0.003%
53	7.127	1798	1800	1804	rVB2	161	125	0.01%	0.002%
54	7.156	1804	1809	1814	rBV2	295	369	0.04%	0.005%
55	7.192	1816	1820	1828	rVB4	671	902	0.09%	0.012%
56	7.230	1828	1832	1834	rBV	404	212	0.02%	0.003%
57	7.565	1924	1936	1956	rBV2	118872	213111	20.61%	2.834%
58	7.793	2000	2007	2011	rBV4	654	839	0.08%	0.011%
59	7.899	2025	2040	2058	rBV	422982	740155	71.58%	9.843%
60	8.179	2116	2127	2146	rVV	81819	142675	13.80%	1.897%
61	8.404	2195	2197	2200	rBV2	412	272	0.03%	0.004%
62	8.523	2230	2234	2239	rVB3	489	408	0.04%	0.005%
63	8.549	2239	2242	2245	rBV	481	314	0.03%	0.004%
64	8.639	2255	2270	2280	rBV3	189236	420502	40.66%	5.592%
65	8.902	2345	2352	2354	rBV3	316	364	0.04%	0.005%
66	8.938	2360	2363	2368	rVB	298	199	0.02%	0.003%
67	9.041	2391	2395	2396	rBV	140	108	0.01%	0.001%
68	9.127	2418	2422	2424	rBV	159	119	0.01%	0.002%
69	9.143	2424	2427	2434	rVV	122	160	0.02%	0.002%
70	9.214	2446	2449	2453	rVB3	459	345	0.03%	0.005%
71	9.282	2466	2470	2473	rBV2	215	156	0.02%	0.002%
72	9.417	2499	2512	2530	rBV	428205	727095	70.31%	9.670%
73	9.555	2553	2555	2556	rBV	320	108	0.01%	0.001%
74	9.751	2614	2616	2620	rBV2	311	195	0.02%	0.003%
75	9.873	2651	2654	2656	rBV	358	215	0.02%	0.003%
76	10.015	2694	2698	2701	rBV2	396	263	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050581.D
 Acq On : 01 Sep 2022 15:23
 Operator : SY/MD
 Sample : N4458-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

77	10.066	2712	2714	2718	rVB	256	157	0.02%	0.002%
78	10.105	2722	2726	2727	rBV2	306	231	0.02%	0.003%
79	10.188	2751	2752	2756	rVB2	210	123	0.01%	0.002%
80	10.221	2757	2762	2767	rBV2	327	450	0.04%	0.006%
81	10.484	2842	2844	2846	rBV2	196	128	0.01%	0.002%
82	10.571	2869	2871	2874	rBV	201	108	0.01%	0.001%
83	10.754	2915	2928	2947	rBV	358316	593458	57.39%	7.892%
84	10.902	2971	2974	2978	rBV2	385	266	0.03%	0.004%
85	11.044	3014	3018	3019	rBV	253	170	0.02%	0.002%
86	11.159	3051	3054	3056	rBV	245	134	0.01%	0.002%
87	11.336	3107	3109	3112	rBV	242	166	0.02%	0.002%
88	11.430	3133	3138	3144	rBV2	343	391	0.04%	0.005%
89	11.639	3200	3203	3207	rBV2	349	331	0.03%	0.004%
90	11.725	3227	3230	3232	rBV	258	172	0.02%	0.002%
91	11.812	3244	3257	3277	rBV	329843	544841	52.69%	7.246%
92	12.063	3330	3335	3337	rBV2	2743	2541	0.25%	0.034%
93	12.192	3362	3375	3406	rBV	372881	662330	64.05%	8.808%
94	12.336	3417	3420	3426	rBV3	684	458	0.04%	0.006%
95	12.629	3509	3511	3517	rBV2	430	318	0.03%	0.004%
96	12.812	3564	3568	3569	rBV	353	199	0.02%	0.003%
97	12.976	3616	3619	3621	rBV	280	185	0.02%	0.002%
98	13.217	3686	3694	3703	rBV6	2339	4132	0.40%	0.055%
99	13.841	3880	3888	3902	rVB	19200	29520	2.85%	0.393%
100	14.333	4033	4041	4057	rVB5	12873	21866	2.11%	0.291%




Sum of corrected areas: 7519301

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050581.D
Acq On : 01 Sep 2022 15:23
Operator : SY/MD
Sample : N4458-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

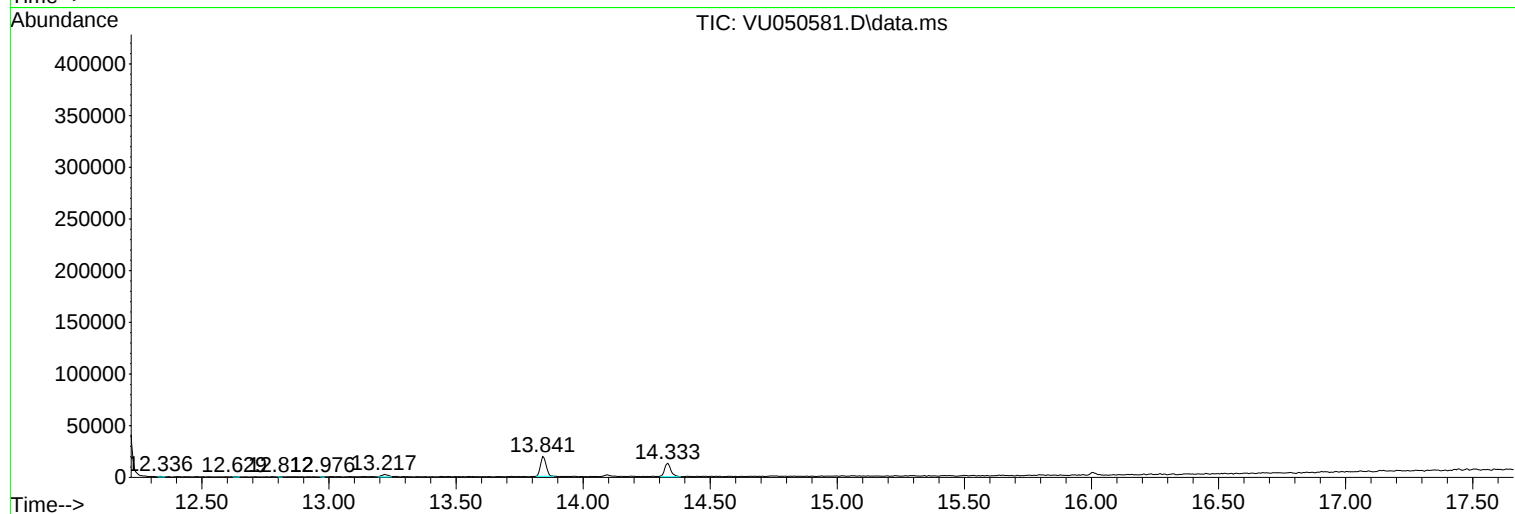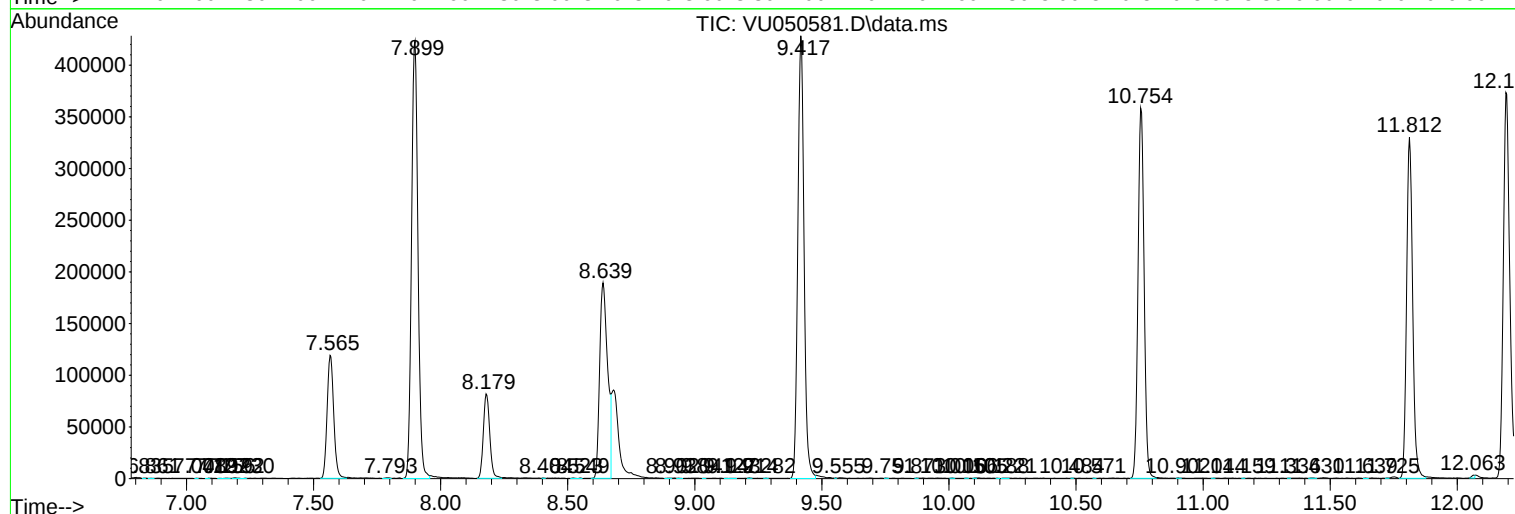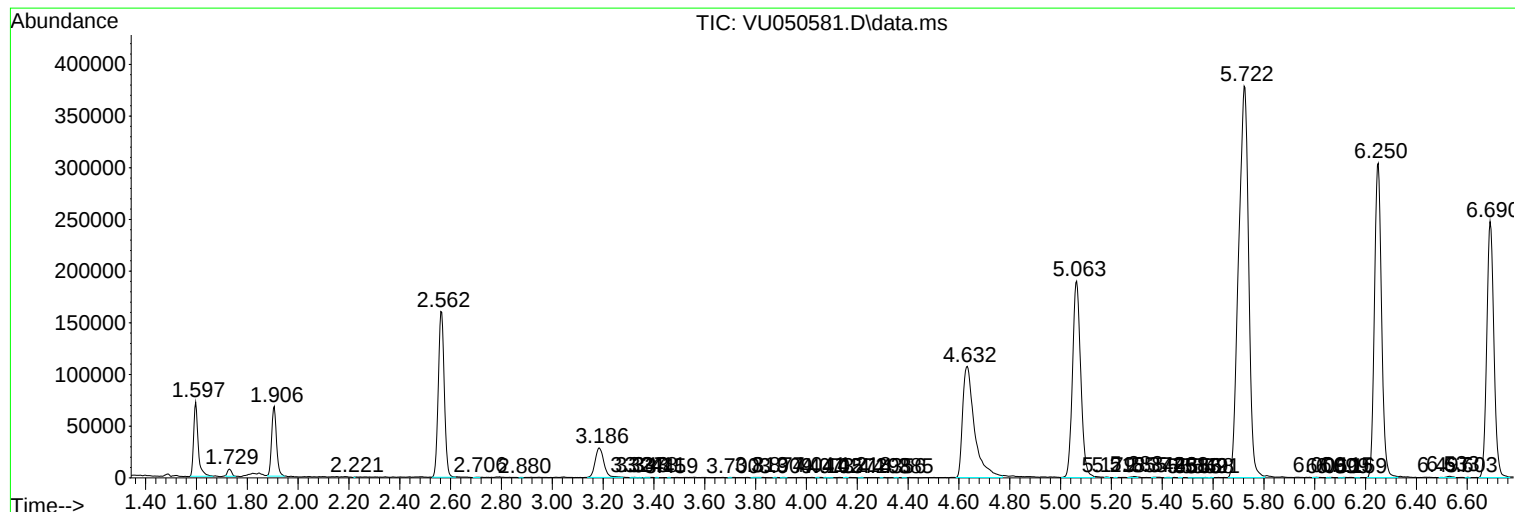

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050581.D
Acq On : 01 Sep 2022 15:23
Operator : SY/MD
Sample : N4458-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050581.D
Acq On : 01 Sep 2022 15:23
Operator : SY/MD
Sample : N4458-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc