

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050582.D
 Acq On : 01 Sep 2022 15:46
 Operator : SY/MD
 Sample : N4458-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050582.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	50	rVB3	1892	1715	0.14%	0.021%
2	1.597	72	80	101	rBV	104181	133717	11.16%	1.642%
3	1.903	167	175	194	rVB	89641	119137	9.95%	1.463%
4	2.324	304	306	311	rBV2	536	310	0.03%	0.004%
5	2.562	366	380	395	rBV	210262	343823	28.70%	4.223%
6	2.636	399	403	414	rVB	3834	5524	0.46%	0.068%
7	2.742	427	436	439	rBV2	385	549	0.05%	0.007%
8	2.797	445	453	459	rBV3	701	978	0.08%	0.012%
9	2.967	502	506	507	rBV2	230	199	0.02%	0.002%
10	3.044	524	530	532	rBV4	603	621	0.05%	0.008%
11	3.173	567	570	572	rBV2	393	261	0.02%	0.003%
12	3.243	589	592	597	rVB2	255	230	0.02%	0.003%
13	3.272	597	601	604	rBV	258	257	0.02%	0.003%
14	3.321	612	616	620	rBV2	216	229	0.02%	0.003%
15	3.777	754	758	762	rBV2	305	258	0.02%	0.003%
16	3.829	770	774	778	rVB2	249	226	0.02%	0.003%
17	3.890	788	793	797	rVV	254	247	0.02%	0.003%
18	3.925	799	804	810	rVB2	281	362	0.03%	0.004%
19	4.086	851	854	860	rBV2	221	319	0.03%	0.004%
20	4.276	911	913	917	rVB	436	250	0.02%	0.003%
21	4.298	917	920	925	rBV2	238	233	0.02%	0.003%
22	4.333	926	931	934	rBV2	193	189	0.02%	0.002%
23	4.629	1009	1023	1067	rBV	101097	309619	25.85%	3.803%
24	5.063	1142	1158	1179	rBV	212557	473347	39.51%	5.814%
25	5.205	1199	1202	1204	rBV	283	230	0.02%	0.003%
26	5.285	1221	1227	1237	rVB3	963	1966	0.16%	0.024%
27	5.440	1272	1275	1282	rVB2	224	226	0.02%	0.003%
28	5.722	1341	1363	1397	rBV2	441345	1197901	100.00%	14.714%
29	5.841	1398	1400	1412	rVV3	902	1352	0.11%	0.017%
30	5.890	1412	1415	1419	rVV2	421	300	0.03%	0.004%
31	6.092	1474	1478	1483	rVV2	251	347	0.03%	0.004%
32	6.157	1490	1498	1501	rBV2	205	290	0.02%	0.004%
33	6.250	1513	1527	1549	rBV	307183	584234	48.77%	7.176%
34	6.433	1580	1584	1588	rBV2	315	193	0.02%	0.002%
35	6.485	1596	1600	1603	rBV2	191	206	0.02%	0.003%
36	6.533	1610	1615	1617	rBV3	1035	953	0.08%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050582.D
 Acq On : 01 Sep 2022 15:46
 Operator : SY/MD
 Sample : N4458-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

37	6.587	1624	1632	1637	rBV3	675	884	0.07%	0.011%
38	6.690	1649	1664	1689	rBV	279544	545486	45.54%	6.700%
39	6.806	1695	1700	1705	rVB4	943	885	0.07%	0.011%
40	7.086	1781	1787	1789	rBV	381	356	0.03%	0.004%
41	7.192	1810	1820	1823	rBV5	698	1202	0.10%	0.015%
42	7.433	1893	1895	1901	rVB2	271	198	0.02%	0.002%
43	7.468	1901	1906	1909	rBV	252	214	0.02%	0.003%
44	7.491	1909	1913	1916	rBV	255	251	0.02%	0.003%
45	7.565	1923	1936	1958	rBV	139114	247537	20.66%	3.041%
46	7.899	2023	2040	2065	rBV	489503	862087	71.97%	10.589%
47	8.066	2089	2092	2095	rBV2	341	253	0.02%	0.003%
48	8.179	2115	2127	2147	rBV2	93820	161429	13.48%	1.983%
49	8.317	2166	2170	2177	rBV5	322	312	0.03%	0.004%
50	8.488	2220	2223	2227	rBV2	247	207	0.02%	0.003%
51	8.549	2240	2242	2248	rVB2	612	481	0.04%	0.006%
52	8.584	2250	2253	2257	rBV2	215	207	0.02%	0.003%
53	8.639	2257	2270	2280	rBV3	216895	474074	39.58%	5.823%
54	8.851	2330	2336	2338	rBV2	362	419	0.03%	0.005%
55	8.967	2370	2372	2376	rBV	221	196	0.02%	0.002%
56	9.417	2496	2512	2538	rBV	426657	724861	60.51%	8.904%
57	9.607	2568	2571	2574	rBV	219	195	0.02%	0.002%
58	9.819	2633	2637	2639	rBV	306	212	0.02%	0.003%
59	9.883	2653	2657	2662	rBV2	342	397	0.03%	0.005%
60	10.118	2728	2730	2733	rBV2	336	233	0.02%	0.003%
61	10.150	2738	2740	2746	rBV2	218	223	0.02%	0.003%
62	10.574	2865	2872	2876	rBV2	478	628	0.05%	0.008%
63	10.635	2888	2891	2896	rVB2	302	233	0.02%	0.003%
64	10.754	2915	2928	2955	rBV	407255	657968	54.93%	8.082%
65	10.880	2965	2967	2970	rVB2	507	302	0.03%	0.004%
66	10.896	2970	2972	2978	rBV2	404	391	0.03%	0.005%
67	11.037	3012	3016	3019	rBB2	295	222	0.02%	0.003%
68	11.086	3029	3031	3034	rBV	302	259	0.02%	0.003%
69	11.356	3112	3115	3121	rBV2	310	269	0.02%	0.003%
70	11.594	3185	3189	3193	rBV2	306	305	0.03%	0.004%
71	11.619	3193	3197	3200	rVB2	257	217	0.02%	0.003%
72	11.745	3233	3236	3241	rBV2	666	653	0.05%	0.008%
73	11.812	3245	3257	3279	rBV	332996	540640	45.13%	6.641%
74	11.986	3307	3311	3313	rVB	448	339	0.03%	0.004%
75	12.005	3313	3317	3320	rBV2	326	292	0.02%	0.004%
76	12.063	3326	3335	3351	rBV4	6357	11652	0.97%	0.143%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050582.D
 Acq On : 01 Sep 2022 15:46
 Operator : SY/MD
 Sample : N4458-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

77	12.192	3363	3375	3398	rBV	425277	699727	58.41%	8.595%
78	12.404	3438	3441	3443	rBV	361	245	0.02%	0.003%
79	12.587	3496	3498	3502	rBV	337	306	0.03%	0.004%
80	12.696	3530	3532	3537	rVB	295	197	0.02%	0.002%
81	12.767	3549	3554	3555	rBV2	453	363	0.03%	0.004%
82	12.822	3568	3571	3575	rBV2	433	306	0.03%	0.004%
83	12.860	3580	3583	3585	rBV2	259	189	0.02%	0.002%
84	12.979	3616	3620	3623	rBV2	379	359	0.03%	0.004%
85	13.063	3643	3646	3651	rVB2	351	277	0.02%	0.003%
86	13.188	3682	3685	3686	rBV2	311	196	0.02%	0.002%
87	13.278	3710	3713	3716	rVB	404	260	0.02%	0.003%
88	13.307	3716	3722	3727	rBV2	531	705	0.06%	0.009%
89	13.475	3771	3774	3778	rBV	384	302	0.03%	0.004%
90	13.523	3786	3789	3794	rVB3	417	421	0.04%	0.005%
91	13.555	3794	3799	3801	rBV3	341	333	0.03%	0.004%
92	13.713	3846	3848	3850	rBV	325	204	0.02%	0.003%
93	13.774	3863	3867	3871	rBV3	347	357	0.03%	0.004%
94	13.844	3881	3889	3898	rBV6	5893	8903	0.74%	0.109%
95	14.050	3950	3953	3956	rBV3	329	198	0.02%	0.002%
96	14.076	3956	3961	3963	rBV2	554	485	0.04%	0.006%
97	14.098	3963	3968	3971	rVV3	1317	1302	0.11%	0.016%
98	14.192	3994	3997	3999	rBV	474	254	0.02%	0.003%
99	14.330	4033	4040	4051	rBV5	4347	7045	0.59%	0.087%
100	14.500	4091	4093	4098	rBV2	365	218	0.02%	0.003%




Sum of corrected areas: 8141119

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050582.D
Acq On : 01 Sep 2022 15:46
Operator : SY/MD
Sample : N4458-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

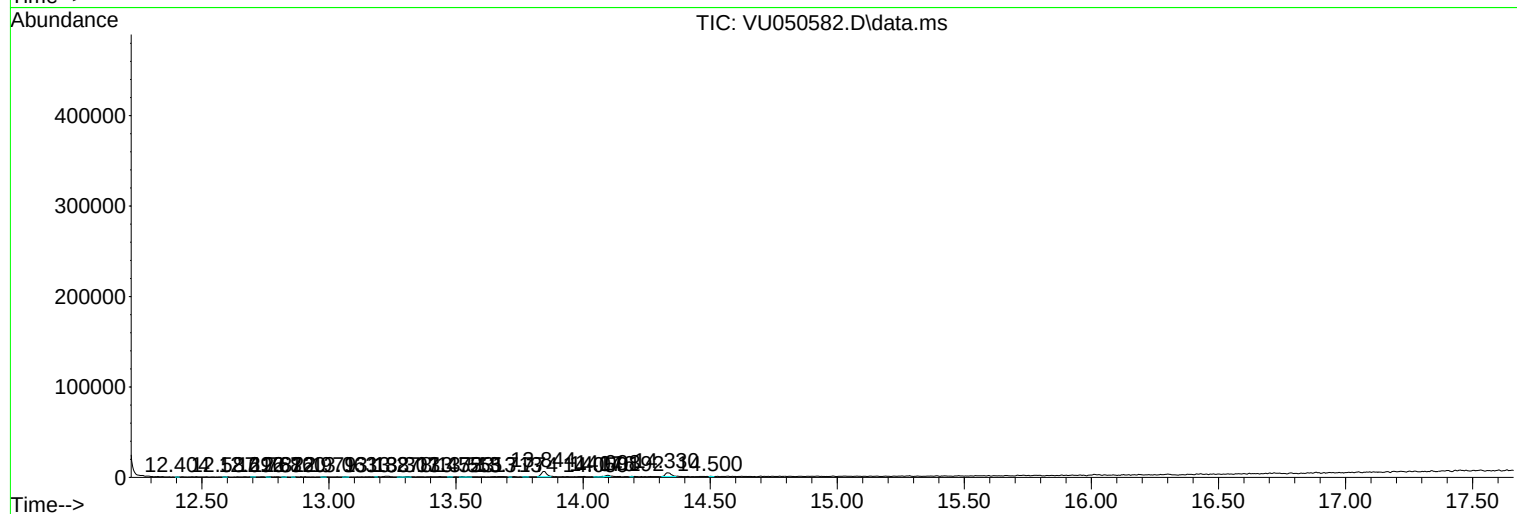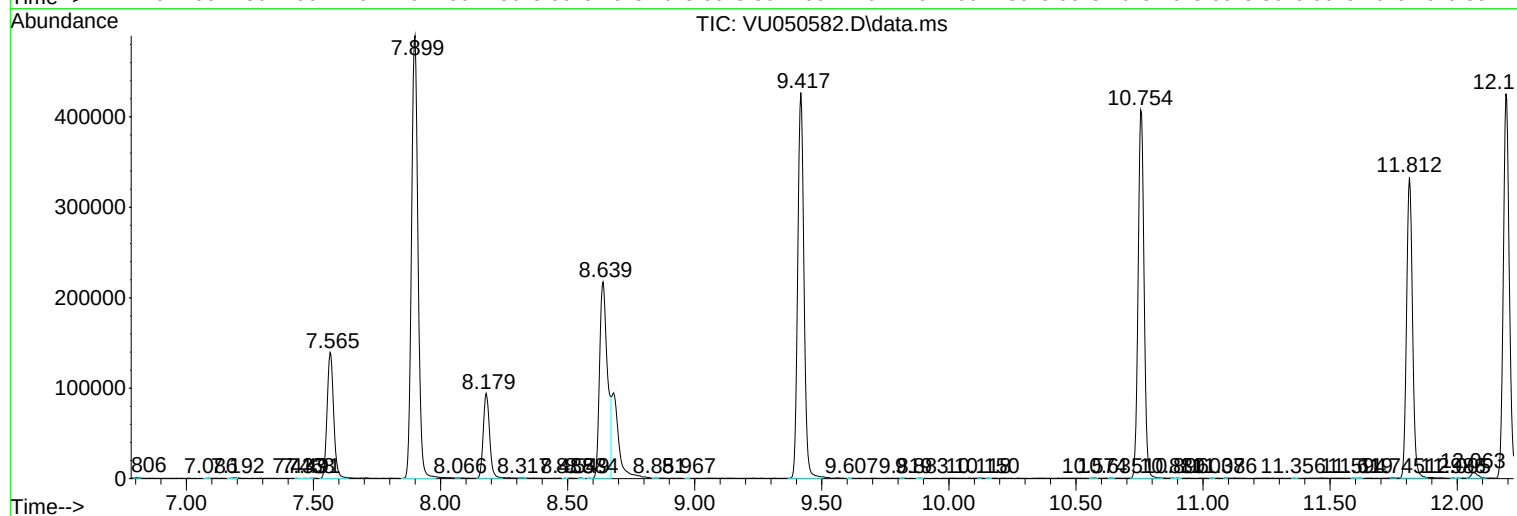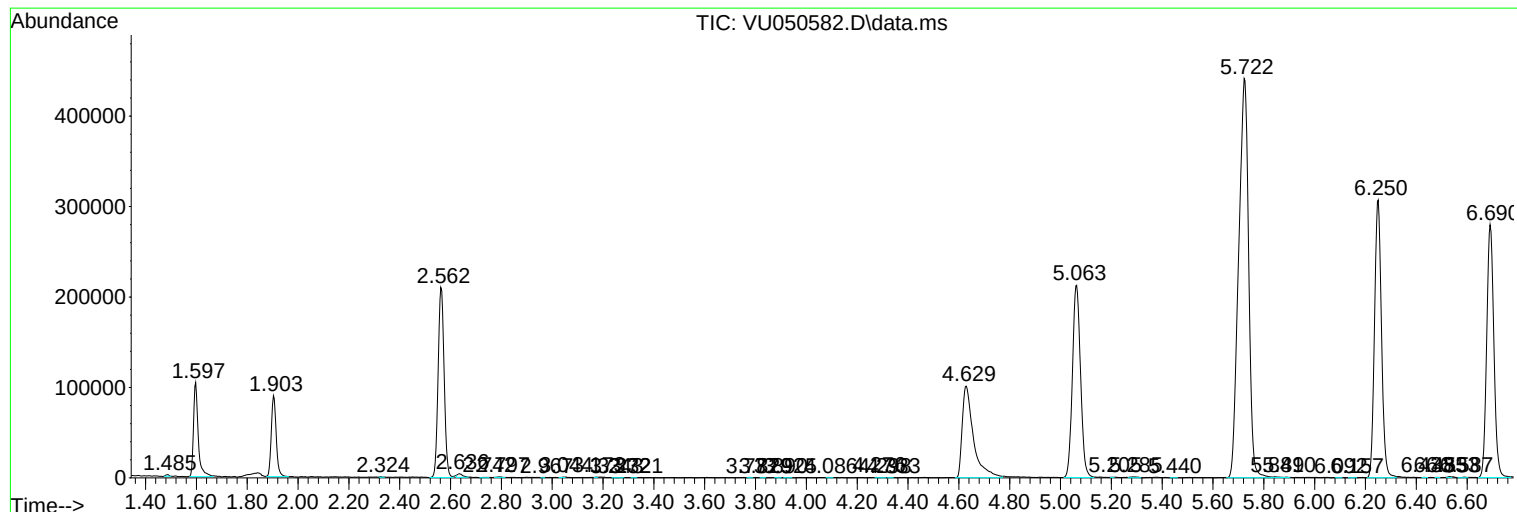

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050582.D
Acq On : 01 Sep 2022 15:46
Operator : SY/MD
Sample : N4458-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050582.D
Acq On : 01 Sep 2022 15:46
Operator : SY/MD
Sample : N4458-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc