

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050583.D
 Acq On : 01 Sep 2022 16:10
 Operator : SY/MD
 Sample : N4362-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050583.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	104	rBV	107502	133673	10.90%	1.620%
2	1.903	168	175	192	rVB	90230	122197	9.97%	1.481%
3	2.231	275	277	279	rBV	439	212	0.02%	0.003%
4	2.504	359	362	365	rBV	362	296	0.02%	0.004%
5	2.562	369	380	396	rVV	216767	353197	28.81%	4.281%
6	2.787	444	450	454	rBV4	823	1284	0.10%	0.016%
7	2.996	512	515	517	rBV	270	161	0.01%	0.002%
8	3.031	523	526	528	rBV2	407	242	0.02%	0.003%
9	3.189	565	575	580	rBV2	1367	2424	0.20%	0.029%
10	3.382	631	635	636	rBV	221	171	0.01%	0.002%
11	3.665	715	723	726	rBV2	235	326	0.03%	0.004%
12	3.710	734	737	741	rBV2	165	140	0.01%	0.002%
13	3.829	770	774	776	rBV	252	223	0.02%	0.003%
14	3.874	783	788	792	rBV2	229	244	0.02%	0.003%
15	3.990	819	824	828	rVB2	275	293	0.02%	0.004%
16	4.009	828	830	832	rBV	185	119	0.01%	0.001%
17	4.044	838	841	845	rBV2	241	209	0.02%	0.003%
18	4.147	870	873	879	rBV	254	300	0.02%	0.004%
19	4.324	925	928	930	rBV2	213	153	0.01%	0.002%
20	4.375	942	944	947	rVB2	190	124	0.01%	0.002%
21	4.404	950	953	955	rBV	221	171	0.01%	0.002%
22	4.465	967	972	975	rBV2	349	452	0.04%	0.005%
23	4.629	1009	1023	1069	rBV2	104385	322696	26.32%	3.911%
24	5.063	1140	1158	1186	rBV	220215	490487	40.01%	5.944%
25	5.266	1217	1221	1224	rBV2	463	432	0.04%	0.005%
26	5.366	1247	1252	1260	rBV3	643	1164	0.09%	0.014%
27	5.433	1270	1273	1276	rBV2	232	210	0.02%	0.003%
28	5.475	1282	1286	1291	rBV	247	313	0.03%	0.004%
29	5.530	1300	1303	1307	rVB2	176	145	0.01%	0.002%
30	5.575	1313	1317	1321	rVB	408	379	0.03%	0.005%
31	5.594	1321	1323	1328	rBV	211	180	0.01%	0.002%
32	5.633	1328	1335	1339	rBV	266	246	0.02%	0.003%
33	5.723	1339	1363	1392	rBV2	446441	1226000	100.00%	14.859%
34	6.044	1461	1463	1466	rVB2	402	204	0.02%	0.002%
35	6.118	1482	1486	1488	rBV2	238	213	0.02%	0.003%
36	6.170	1499	1502	1507	rVB2	212	196	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050583.D
 Acq On : 01 Sep 2022 16:10
 Operator : SY/MD
 Sample : N4362-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

37	6.250	1511	1527	1548	rBV	306525	588938	48.04%	7.138%
38	6.366	1559	1563	1565	rBV3	730	516	0.04%	0.006%
39	6.514	1605	1609	1611	rBV2	588	423	0.03%	0.005%
40	6.533	1611	1615	1617	rBV4	838	694	0.06%	0.008%
41	6.604	1633	1637	1640	rVB2	516	414	0.03%	0.005%
42	6.642	1641	1649	1650	rBV	264	271	0.02%	0.003%
43	6.690	1650	1664	1690	rVV	287182	563674	45.98%	6.831%
44	6.964	1746	1749	1752	rBV2	192	158	0.01%	0.002%
45	7.034	1763	1771	1775	rBV2	277	351	0.03%	0.004%
46	7.054	1775	1777	1779	rBV	217	135	0.01%	0.002%
47	7.131	1798	1801	1804	rBV	158	120	0.01%	0.001%
48	7.186	1816	1818	1819	rBV	580	305	0.02%	0.004%
49	7.375	1872	1877	1880	rBV	270	206	0.02%	0.002%
50	7.401	1880	1885	1888	rVV	119	124	0.01%	0.002%
51	7.420	1888	1891	1893	rVV2	205	141	0.01%	0.002%
52	7.478	1905	1909	1916	rBV	287	352	0.03%	0.004%
53	7.565	1924	1936	1956	rBV	139511	252475	20.59%	3.060%
54	7.681	1971	1972	1974	rBV	421	191	0.02%	0.002%
55	7.735	1987	1989	1991	rBV2	315	193	0.02%	0.002%
56	7.758	1994	1996	1999	rVB	249	124	0.01%	0.002%
57	7.800	2005	2009	2012	rBV2	353	333	0.03%	0.004%
58	7.841	2019	2022	2025	rVB	219	122	0.01%	0.001%
59	7.899	2025	2040	2067	rBV	502654	883209	72.04%	10.704%
60	8.179	2115	2127	2144	rBV	94656	165041	13.46%	2.000%
61	8.436	2203	2207	2210	rVB2	288	235	0.02%	0.003%
62	8.462	2210	2215	2216	rBV	417	260	0.02%	0.003%
63	8.539	2236	2239	2241	rBV2	182	126	0.01%	0.002%
64	8.639	2258	2270	2280	rBV4	224065	482702	39.37%	5.850%
65	8.893	2345	2349	2351	rBV3	479	287	0.02%	0.003%
66	8.948	2362	2366	2371	rBV2	334	416	0.03%	0.005%
67	9.086	2405	2409	2410	rBV	280	219	0.02%	0.003%
68	9.198	2441	2444	2446	rBV	291	221	0.02%	0.003%
69	9.227	2450	2453	2458	rBV2	284	284	0.02%	0.003%
70	9.353	2488	2492	2494	rBV	278	203	0.02%	0.002%
71	9.417	2499	2512	2533	rBV	431615	732168	59.72%	8.874%
72	9.639	2576	2581	2584	rBV2	337	284	0.02%	0.003%
73	9.658	2584	2587	2592	rVB2	349	282	0.02%	0.003%
74	9.687	2594	2596	2600	rVB	364	232	0.02%	0.003%
75	9.726	2606	2608	2611	rBV2	193	153	0.01%	0.002%
76	9.838	2641	2643	2646	rBV	190	124	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050583.D
 Acq On : 01 Sep 2022 16:10
 Operator : SY/MD
 Sample : N4362-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

77	10.063	2711	2713	2719	rVB2	254	172	0.01%	0.002%
78	10.247	2764	2770	2771	rBV2	786	684	0.06%	0.008%
79	10.394	2813	2816	2818	rBV2	299	192	0.02%	0.002%
80	10.423	2818	2825	2832	rVV2	535	860	0.07%	0.010%
81	10.668	2897	2901	2903	rBV2	209	166	0.01%	0.002%
82	10.755	2915	2928	2950	rBV	414435	675613	55.11%	8.188%
83	10.938	2982	2985	2988	rBV	331	271	0.02%	0.003%
84	11.134	3043	3046	3047	rBV2	245	170	0.01%	0.002%
85	11.256	3079	3084	3088	rBV2	424	513	0.04%	0.006%
86	11.359	3114	3116	3119	rBV	294	167	0.01%	0.002%
87	11.587	3183	3187	3188	rBV	390	236	0.02%	0.003%
88	11.648	3201	3206	3211	rBV2	433	461	0.04%	0.006%
89	11.812	3244	3257	3276	rBV	331304	529186	43.16%	6.414%
90	11.973	3303	3307	3309	rBV2	453	418	0.03%	0.005%
91	12.066	3327	3336	3350	rBV6	4680	9432	0.77%	0.114%
92	12.192	3362	3375	3395	rBV	420748	687606	56.09%	8.333%
93	12.713	3534	3537	3540	rBV	341	304	0.02%	0.004%
94	12.751	3547	3549	3555	rBV3	377	443	0.04%	0.005%
95	12.816	3566	3569	3571	rBV2	332	240	0.02%	0.003%
96	12.873	3584	3587	3589	rBV	426	311	0.03%	0.004%
97	13.488	3775	3778	3782	rBV2	352	237	0.02%	0.003%
98	13.661	3830	3832	3836	rBV3	606	477	0.04%	0.006%
99	13.848	3885	3890	3898	rVB5	2465	3223	0.26%	0.039%
100	14.333	4035	4041	4051	rVB5	2456	3546	0.29%	0.043%




Sum of corrected areas: 8251110

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050583.D
Acq On : 01 Sep 2022 16:10
Operator : SY/MD
Sample : N4362-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

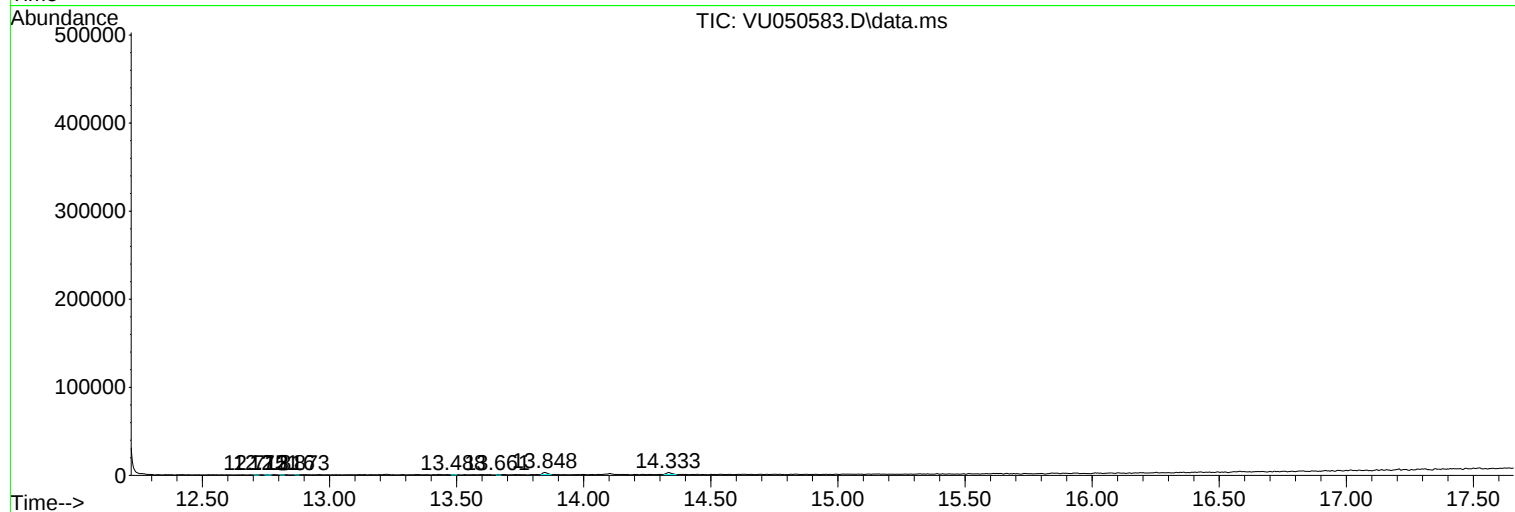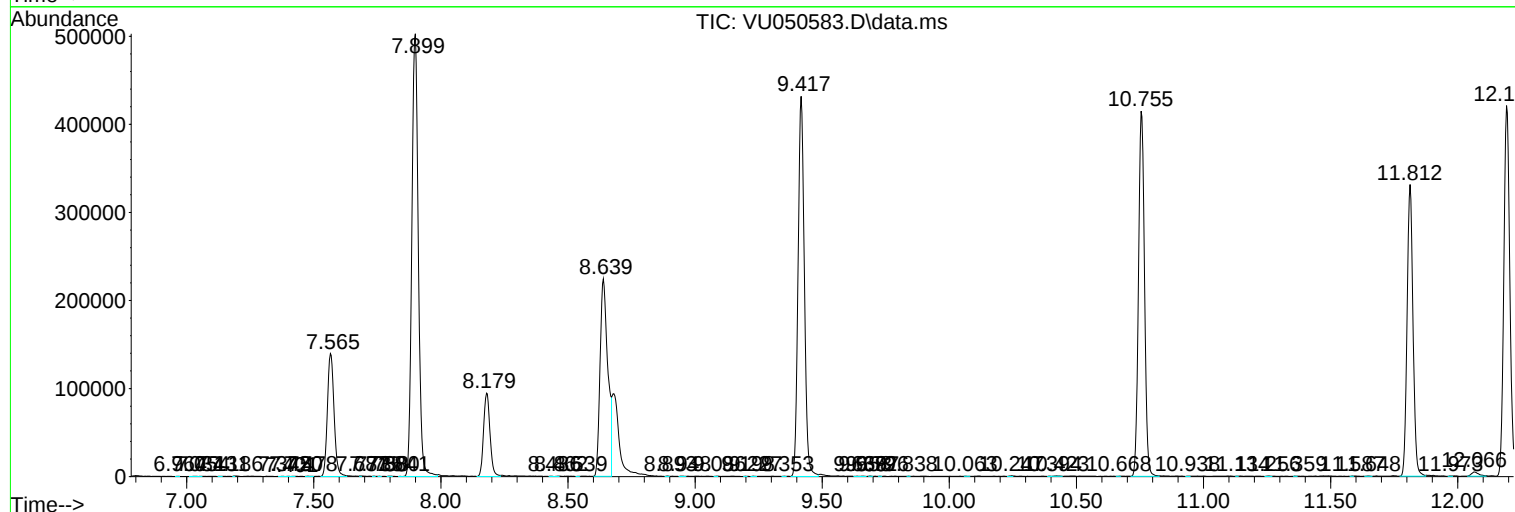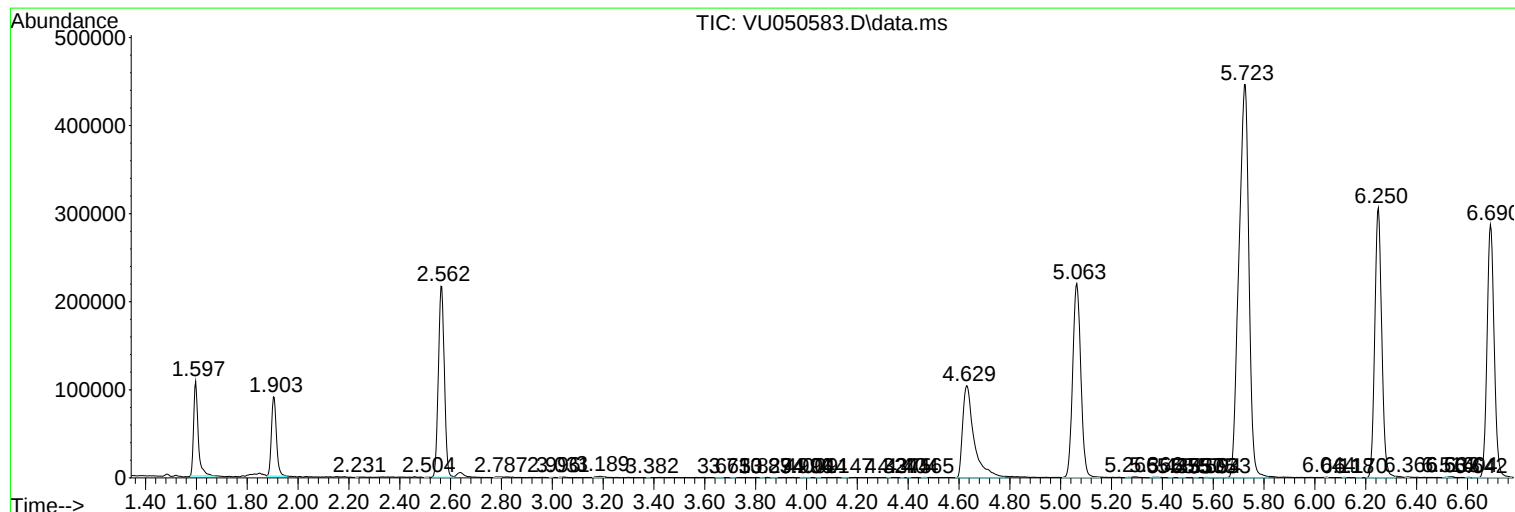

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050583.D
Acq On : 01 Sep 2022 16:10
Operator : SY/MD
Sample : N4362-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050583.D
Acq On : 01 Sep 2022 16:10
Operator : SY/MD
Sample : N4362-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc