

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050586.D
 Acq On : 01 Sep 2022 17:21
 Operator : SY/MD
 Sample : N4458-02DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M

Title : VOC Analysis

Signal : TIC: VU050586.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	51	rBV3	4946	6287	0.26%	0.037%
2	1.597	72	80	104	rBV	318278	400041	16.79%	2.344%
3	1.906	168	176	200	rVB	240753	324622	13.63%	1.902%
4	2.562	366	380	400	rBV	514189	838171	35.19%	4.912%
5	2.784	444	449	454	rBV4	1102	1367	0.06%	0.008%
6	3.019	517	522	523	rBV3	354	275	0.01%	0.002%
7	3.047	523	531	540	rVB4	2076	3548	0.15%	0.021%
8	3.109	547	550	553	rBV2	464	285	0.01%	0.002%
9	3.179	566	572	586	rVB2	2777	5498	0.23%	0.032%
10	3.302	607	610	617	rBV3	493	518	0.02%	0.003%
11	3.350	621	625	629	rBV3	299	290	0.01%	0.002%
12	3.433	648	651	654	rBV2	314	242	0.01%	0.001%
13	3.462	657	660	666	rVV3	431	355	0.01%	0.002%
14	3.504	670	673	679	rVB3	279	280	0.01%	0.002%
15	3.668	716	724	728	rBV3	418	606	0.03%	0.004%
16	3.941	805	809	814	rVB2	327	310	0.01%	0.002%
17	3.993	821	825	830	rVB	383	306	0.01%	0.002%
18	4.182	877	884	886	rBV2	403	458	0.02%	0.003%
19	4.321	920	927	929	rVV2	504	399	0.02%	0.002%
20	4.629	1007	1023	1063	rBV	216829	627795	26.35%	3.679%
21	4.961	1123	1126	1130	rVB3	562	434	0.02%	0.003%
22	4.993	1134	1136	1141	rVB3	369	241	0.01%	0.001%
23	5.063	1141	1158	1186	rBV	405767	906766	38.07%	5.314%
24	5.285	1221	1227	1228	rBV	1374	1063	0.04%	0.006%
25	5.369	1249	1253	1256	rBV3	1090	992	0.04%	0.006%
26	5.385	1256	1258	1266	rVB3	697	635	0.03%	0.004%
27	5.427	1267	1271	1273	rBV2	465	269	0.01%	0.002%
28	5.488	1284	1290	1294	rBV2	421	426	0.02%	0.002%
29	5.517	1294	1299	1300	rBV3	468	414	0.02%	0.002%
30	5.726	1342	1364	1377	rBV2	871220	2382113	100.00%	13.961%
31	5.938	1427	1430	1433	rBV	512	332	0.01%	0.002%
32	5.980	1441	1443	1446	rVB3	592	260	0.01%	0.002%
33	6.015	1451	1454	1457	rBV	419	431	0.02%	0.003%
34	6.035	1457	1460	1462	rBV3	697	409	0.02%	0.002%
35	6.076	1470	1473	1475	rBV	357	263	0.01%	0.002%
36	6.182	1501	1506	1508	rBV2	295	239	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050586.D
 Acq On : 01 Sep 2022 17:21
 Operator : SY/MD
 Sample : N4458-02DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

37	6.250	1512	1527	1553	rBV	572242	1094455	45.94%	6.414%
38	6.469	1593	1595	1597	rBV2	432	234	0.01%	0.001%
39	6.533	1606	1615	1622	rVB3	3035	4688	0.20%	0.027%
40	6.600	1631	1636	1639	rBV3	488	387	0.02%	0.002%
41	6.690	1647	1664	1685	rBV	522033	1040470	43.68%	6.098%
42	6.880	1720	1723	1725	rVB2	358	242	0.01%	0.001%
43	6.909	1730	1732	1736	rVB2	365	273	0.01%	0.002%
44	6.970	1747	1751	1756	rVB3	378	348	0.01%	0.002%
45	7.128	1796	1800	1802	rBV	334	243	0.01%	0.001%
46	7.189	1810	1819	1821	rBV5	1012	1026	0.04%	0.006%
47	7.388	1876	1881	1884	rBV4	361	360	0.02%	0.002%
48	7.485	1908	1911	1917	rVB3	350	336	0.01%	0.002%
49	7.565	1923	1936	1956	rBV	246757	441366	18.53%	2.587%
50	7.848	2020	2024	2026	rBV3	409	267	0.01%	0.002%
51	7.899	2026	2040	2068	rBV	968227	1722686	72.32%	10.096%
52	8.073	2091	2094	2097	rBV4	519	355	0.01%	0.002%
53	8.179	2115	2127	2145	rBV	164605	282412	11.86%	1.655%
54	8.369	2182	2186	2189	rBV2	287	288	0.01%	0.002%
55	8.488	2218	2223	2225	rBV3	381	362	0.02%	0.002%
56	8.546	2236	2241	2242	rBV2	525	356	0.01%	0.002%
57	8.639	2256	2270	2327	rBV5	476513	1234286	51.81%	7.234%
58	8.854	2335	2337	2342	rVB	1012	602	0.03%	0.004%
59	8.877	2342	2344	2350	rVB2	655	493	0.02%	0.003%
60	9.050	2392	2398	2402	rVB5	301	303	0.01%	0.002%
61	9.079	2402	2407	2409	rBV2	333	287	0.01%	0.002%
62	9.166	2432	2434	2438	rVB	477	284	0.01%	0.002%
63	9.227	2449	2453	2455	rBV	342	267	0.01%	0.002%
64	9.330	2481	2485	2492	rVB3	340	314	0.01%	0.002%
65	9.417	2498	2512	2517	rBV	821528	1389268	58.32%	8.142%
66	9.796	2625	2630	2635	rVB3	506	523	0.02%	0.003%
67	9.906	2661	2664	2670	rBV3	334	298	0.01%	0.002%
68	10.063	2709	2713	2717	rVB2	610	510	0.02%	0.003%
69	10.086	2717	2720	2722	rBV	321	249	0.01%	0.001%
70	10.102	2722	2725	2733	rVB4	741	851	0.04%	0.005%
71	10.314	2786	2791	2801	rBV2	367	406	0.02%	0.002%
72	10.366	2801	2807	2808	rBV2	493	425	0.02%	0.002%
73	10.417	2815	2823	2826	rBV2	282	347	0.01%	0.002%
74	10.481	2841	2843	2848	rVB2	329	240	0.01%	0.001%
75	10.513	2850	2853	2858	rVB2	488	386	0.02%	0.002%
76	10.581	2870	2874	2880	rBV2	312	243	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050586.D
 Acq On : 01 Sep 2022 17:21
 Operator : SY/MD
 Sample : N4458-02DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

77	10.639	2889	2892	2897	rBV	558	405	0.02%	0.002%
78	10.668	2897	2901	2903	rBV2	289	245	0.01%	0.001%
79	10.758	2913	2929	2949	rBV	601478	1012935	42.52%	5.936%
80	11.044	3010	3018	3020	rBV	1182	1172	0.05%	0.007%
81	11.115	3035	3040	3048	rBV4	1041	1152	0.05%	0.007%
82	11.346	3110	3112	3114	rBV	392	237	0.01%	0.001%
83	11.597	3187	3190	3194	rVV2	410	324	0.01%	0.002%
84	11.748	3225	3237	3246	rBV	33449	52935	2.22%	0.310%
85	11.812	3246	3257	3289	rVB2	582225	1326832	55.70%	7.776%
86	12.002	3312	3316	3319	rBV	394	308	0.01%	0.002%
87	12.128	3351	3355	3357	rBV2	593	443	0.02%	0.003%
88	12.195	3360	3376	3400	rBV3	857708	1846084	77.50%	10.819%
89	12.500	3464	3471	3472	rBV3	412	371	0.02%	0.002%
90	12.616	3502	3507	3512	rBV3	552	646	0.03%	0.004%
91	12.677	3521	3526	3527	rBV2	264	239	0.01%	0.001%
92	12.748	3543	3548	3549	rBV2	443	363	0.02%	0.002%
93	13.063	3639	3646	3649	rBV3	613	905	0.04%	0.005%
94	13.234	3697	3699	3703	rVB2	484	234	0.01%	0.001%
95	13.275	3709	3712	3715	rBV2	356	265	0.01%	0.002%
96	13.844	3878	3889	3906	rBV2	40625	69306	2.91%	0.406%
97	14.333	4033	4041	4053	rBV5	9646	16954	0.71%	0.099%
98	15.028	4255	4257	4261	rBV3	685	438	0.02%	0.003%
99	15.134	4288	4290	4294	rBV5	659	401	0.02%	0.002%
100	16.131	4597	4600	4603	rBV3	1455	1205	0.05%	0.007%




Sum of corrected areas: 17063075

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050586.D
Acq On : 01 Sep 2022 17:21
Operator : SY/MD
Sample : N4458-02DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

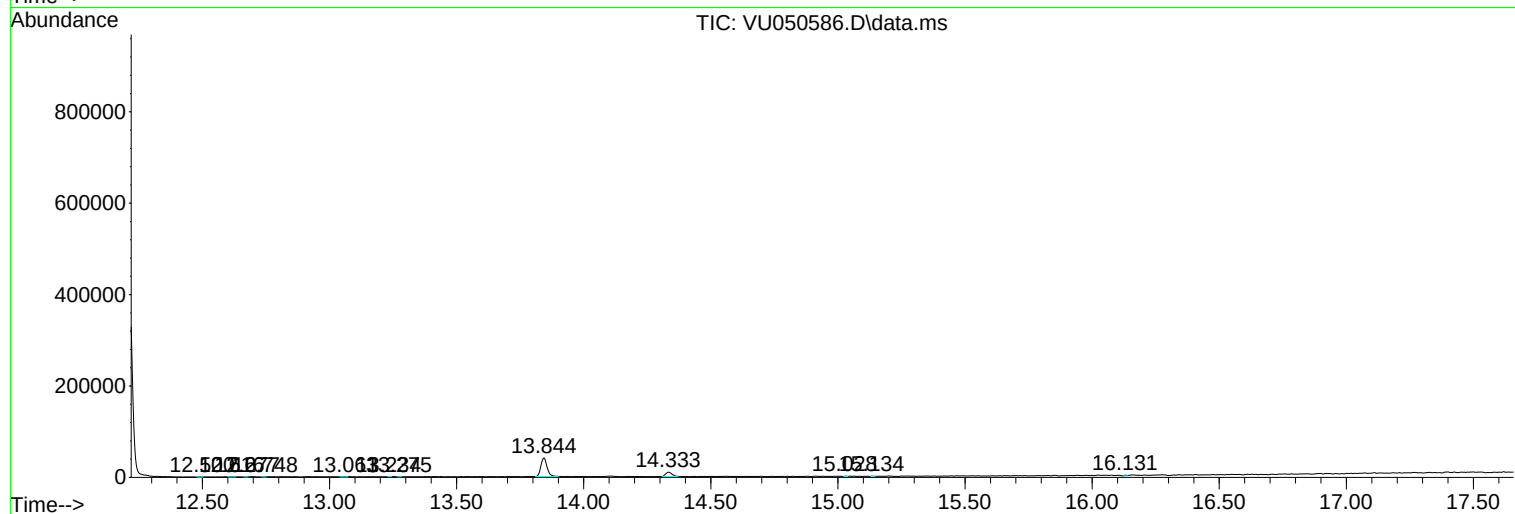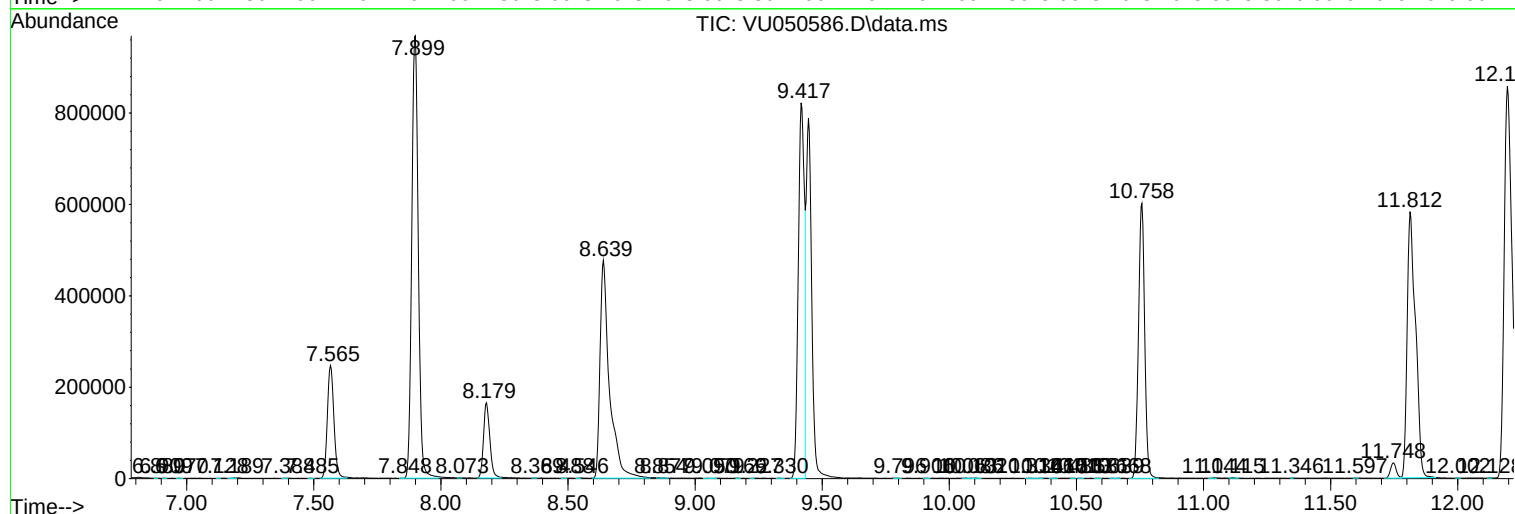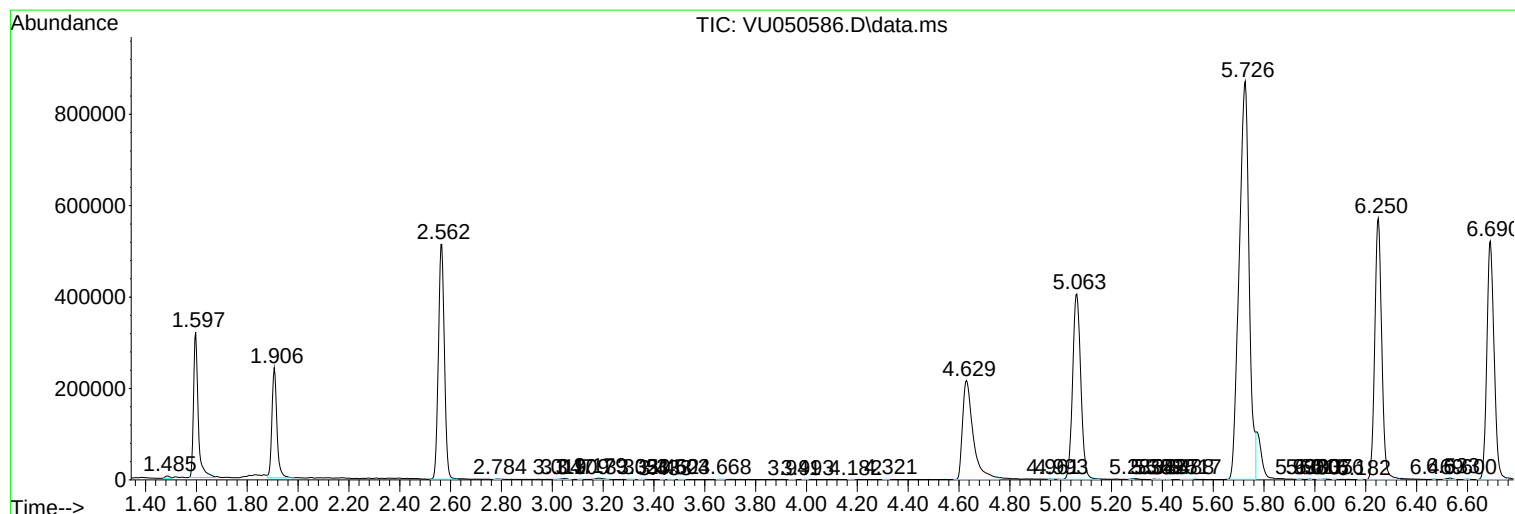

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050586.D
Acq On : 01 Sep 2022 17:21
Operator : SY/MD
Sample : N4458-02DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050586.D
Acq On : 01 Sep 2022 17:21
Operator : SY/MD
Sample : N4458-02DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------