

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050587.D
 Acq On : 01 Sep 2022 17:45
 Operator : SY/MD
 Sample : N4458-02 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M

Title : VOC Analysis

Signal : TIC: VU050587.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	51	rBV3	3380	3422	0.05%	0.012%
2	1.598	72	80	106	rBV	305234	397961	5.53%	1.387%
3	1.903	166	175	194	rVB	253142	342771	4.77%	1.194%
4	2.562	368	380	397	rBV	502911	809798	11.26%	2.822%
5	2.784	444	449	451	rBV2	782	748	0.01%	0.003%
6	2.839	464	466	470	rBV	312	213	0.00%	0.001%
7	2.861	470	473	477	rVB	372	283	0.00%	0.001%
8	2.967	502	506	507	rBV2	429	311	0.00%	0.001%
9	3.045	521	530	540	rVB6	1990	3009	0.04%	0.010%
10	3.115	548	552	553	rBV	393	292	0.00%	0.001%
11	3.183	560	573	594	rVB2	10058	23992	0.33%	0.084%
12	3.305	608	611	615	rBV	318	227	0.00%	0.001%
13	3.340	618	622	625	rBV3	267	243	0.00%	0.001%
14	3.546	681	686	687	rBV	342	232	0.00%	0.001%
15	3.688	727	730	733	rBV2	349	247	0.00%	0.001%
16	3.710	733	737	743	rVB2	439	416	0.01%	0.001%
17	3.832	771	775	778	rVB3	295	266	0.00%	0.001%
18	3.848	778	780	784	rBV2	239	216	0.00%	0.001%
19	3.887	789	792	796	rVB	343	235	0.00%	0.001%
20	4.041	833	840	844	rBV	446	518	0.01%	0.002%
21	4.173	878	881	887	rVB2	325	358	0.00%	0.001%
22	4.273	903	912	914	rBV2	380	542	0.01%	0.002%
23	4.527	987	991	1002	rVB4	1432	2246	0.03%	0.008%
24	4.627	1009	1022	1069	rBV	217736	623972	8.67%	2.174%
25	4.990	1130	1135	1141	rBV2	814	1074	0.01%	0.004%
26	5.061	1141	1157	1181	rVV	416826	918951	12.78%	3.202%
27	5.208	1200	1203	1205	rBV2	510	307	0.00%	0.001%
28	5.295	1219	1230	1240	rVB5	2344	4850	0.07%	0.017%
29	5.376	1252	1255	1257	rBV3	711	405	0.01%	0.001%
30	5.517	1291	1299	1313	rVB6	2772	5805	0.08%	0.020%
31	5.578	1314	1318	1321	rBV2	301	221	0.00%	0.001%
32	5.610	1326	1328	1332	rVB2	332	239	0.00%	0.001%
33	5.723	1342	1363	1372	rBV2	874606	2339103	32.52%	8.151%
34	5.983	1439	1444	1445	rBV4	721	656	0.01%	0.002%
35	6.048	1462	1464	1467	rVB4	517	243	0.00%	0.001%
36	6.099	1477	1480	1482	rBV2	440	259	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050587.D
 Acq On : 01 Sep 2022 17:45
 Operator : SY/MD
 Sample : N4458-02 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

37	6.144	1491	1494	1501	rVB4	354	327	0.00%	0.001%
38	6.247	1511	1526	1550	rBV	616905	1180941	16.42%	4.115%
39	6.520	1604	1611	1613	rBV6	1612	1683	0.02%	0.006%
40	6.607	1636	1638	1643	rVB	389	251	0.00%	0.001%
41	6.691	1649	1664	1686	rBV	540197	1060708	14.75%	3.696%
42	6.842	1709	1711	1715	rVB3	447	289	0.00%	0.001%
43	6.868	1715	1719	1722	rVB3	493	341	0.00%	0.001%
44	7.070	1780	1782	1788	rVB	281	221	0.00%	0.001%
45	7.109	1788	1794	1798	rBV2	388	371	0.01%	0.001%
46	7.186	1807	1818	1820	rBV3	936	1104	0.02%	0.004%
47	7.430	1890	1894	1899	rVB2	326	343	0.00%	0.001%
48	7.466	1899	1905	1906	rBV	401	342	0.00%	0.001%
49	7.514	1915	1920	1924	rBV2	285	278	0.00%	0.001%
50	7.565	1924	1936	1960	rBV	229432	406133	5.65%	1.415%
51	7.758	1994	1996	2002	rVB4	248	246	0.00%	0.001%
52	7.790	2002	2006	2009	rBV4	467	432	0.01%	0.002%
53	7.896	2024	2039	2060	rBV	900558	1567739	21.80%	5.463%
54	8.073	2091	2094	2102	rVV5	782	990	0.01%	0.003%
55	8.179	2115	2127	2143	rBV	128485	215211	2.99%	0.750%
56	8.372	2185	2187	2192	rVB3	409	212	0.00%	0.001%
57	8.401	2194	2196	2199	rBV	339	254	0.00%	0.001%
58	8.488	2221	2223	2227	rVB	395	279	0.00%	0.001%
59	8.549	2235	2242	2246	rBV6	763	1047	0.01%	0.004%
60	8.639	2255	2270	2319	rBV5	422868	1159176	16.12%	4.039%
61	8.964	2367	2371	2375	rVB3	295	264	0.00%	0.001%
62	9.019	2386	2388	2392	rBV2	349	248	0.00%	0.001%
63	9.305	2471	2477	2478	rBV2	281	299	0.00%	0.001%
64	9.446	2494	2521	2565	rBV2	3638100	7192870	100.00%	25.063%
65	9.662	2586	2588	2592	rBV3	505	389	0.01%	0.001%
66	9.697	2596	2599	2607	rVB5	1140	1189	0.02%	0.004%
67	9.797	2627	2630	2635	rBV	559	430	0.01%	0.001%
68	9.903	2659	2663	2665	rBV2	629	464	0.01%	0.002%
69	10.099	2719	2724	2725	rBV3	431	317	0.00%	0.001%
70	10.121	2725	2731	2733	rVV3	527	601	0.01%	0.002%
71	10.163	2742	2744	2748	rVV	403	324	0.00%	0.001%
72	10.382	2807	2812	2815	rBV	378	352	0.00%	0.001%
73	10.520	2851	2855	2858	rBV2	325	256	0.00%	0.001%
74	10.588	2874	2876	2881	rVB	320	232	0.00%	0.001%
75	10.636	2888	2891	2894	rVB	396	270	0.00%	0.001%
76	10.755	2915	2928	2948	rBV	700499	1114198	15.49%	3.882%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050587.D
 Acq On : 01 Sep 2022 17:45
 Operator : SY/MD
 Sample : N4458-02 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

77	11.096	3031	3034	3036	rVV3	473	346	0.00%	0.001%
78	11.112	3036	3039	3042	rVV2	787	617	0.01%	0.002%
79	11.160	3050	3054	3058	rVB3	373	271	0.00%	0.001%
80	11.202	3063	3067	3070	rBB	423	246	0.00%	0.001%
81	11.244	3076	3080	3082	rBV2	282	213	0.00%	0.001%
82	11.260	3082	3085	3090	rBV3	261	213	0.00%	0.001%
83	11.321	3099	3104	3110	rBV2	317	341	0.00%	0.001%
84	11.363	3110	3117	3120	rVV2	497	512	0.01%	0.002%
85	11.453	3141	3145	3147	rBV2	423	321	0.00%	0.001%
86	11.530	3163	3169	3172	rVV3	393	498	0.01%	0.002%
87	11.610	3191	3194	3197	rBV3	339	214	0.00%	0.001%
88	11.745	3225	3236	3246	rBV	180815	290330	4.04%	1.012%
89	11.835	3246	3264	3289	rVB2	1587406	3542928	49.26%	12.345%
90	12.041	3325	3328	3336	rBV6	648	877	0.01%	0.003%
91	12.208	3362	3380	3409	rBV2	2322818	4858677	67.55%	16.930%
92	12.826	3570	3572	3574	rBV2	707	397	0.01%	0.001%
93	12.977	3616	3619	3626	rVB5	2418	2645	0.04%	0.009%
94	13.227	3692	3697	3703	rBV6	1401	1662	0.02%	0.006%
95	13.337	3724	3731	3739	rBV7	1643	2445	0.03%	0.009%
96	13.752	3857	3860	3863	rBV2	552	380	0.01%	0.001%
97	13.842	3876	3888	3904	rBV	296164	482156	6.70%	1.680%
98	14.067	3956	3958	3961	rBV3	587	349	0.00%	0.001%
99	14.330	4030	4040	4055	rBV	69586	114913	1.60%	0.400%
100	15.366	4358	4362	4365	rBV3	905	826	0.01%	0.003%




Sum of corrected areas: 28698629

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050587.D
Acq On : 01 Sep 2022 17:45
Operator : SY/MD
Sample : N4458-02 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

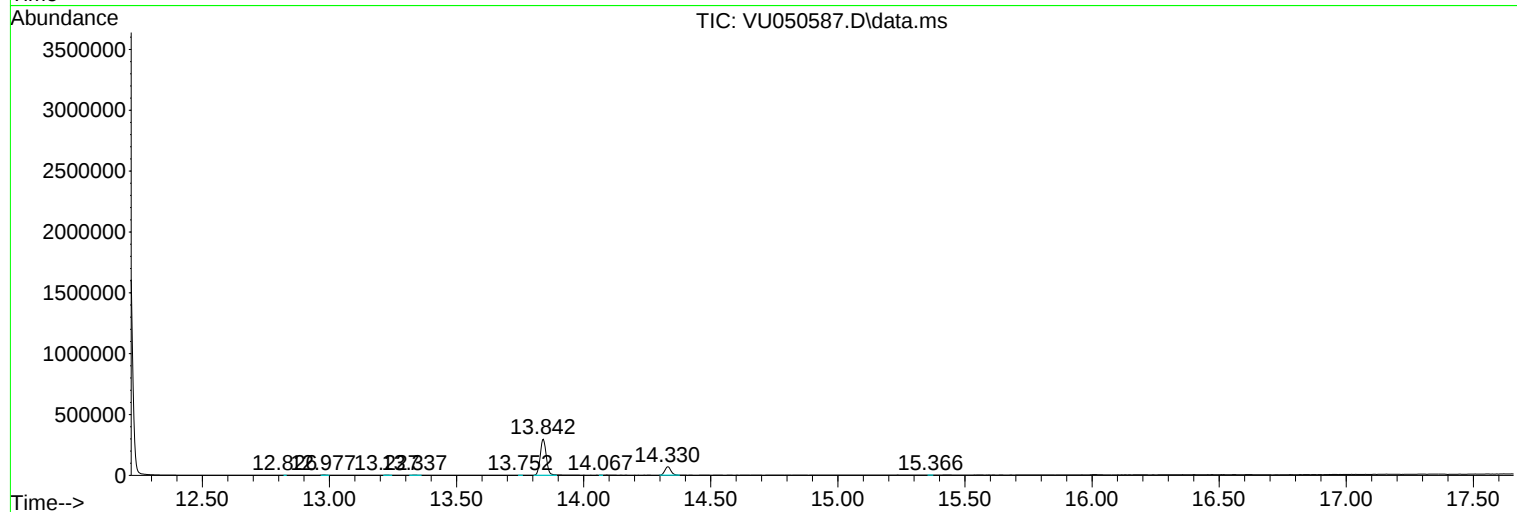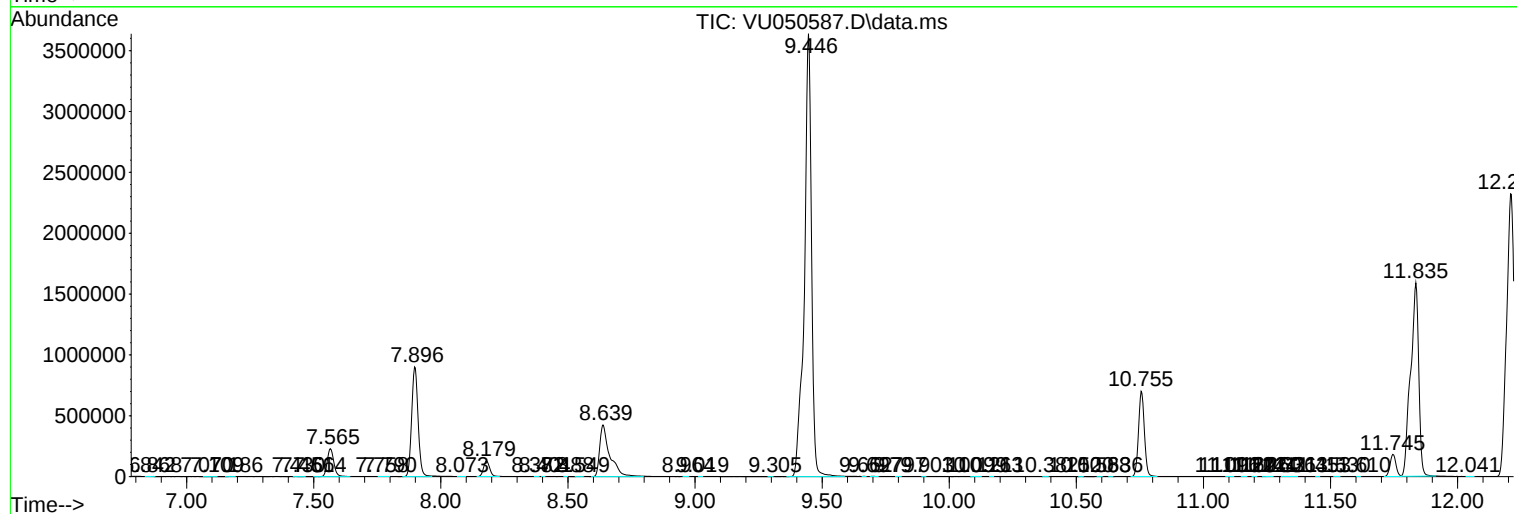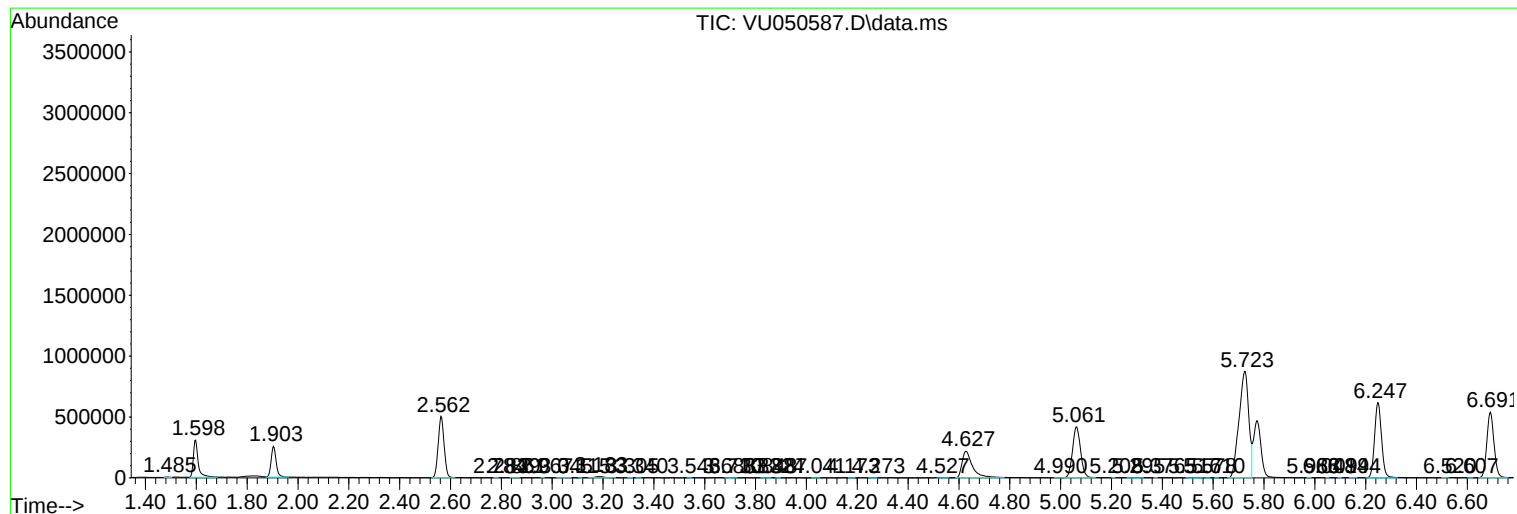

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050587.D
Acq On : 01 Sep 2022 17:45
Operator : SY/MD
Sample : N4458-02 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050587.D
Acq On : 01 Sep 2022 17:45
Operator : SY/MD
Sample : N4458-02 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc