

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050593.D
 Acq On : 01 Sep 2022 20:06
 Operator : SY/MD
 Sample : VIBLK130
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK130

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050593.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	39	44	49	rBV2	5639	6208	0.15%	0.023%
2	1.594	71	79	114	rBV	296062	508208	12.50%	1.882%
3	1.890	165	171	193	rBV	185304	270359	6.65%	1.001%
4	2.549	363	376	397	rBV	761506	1229360	30.23%	4.552%
5	2.829	461	463	468	rVB3	462	321	0.01%	0.001%
6	2.906	482	487	488	rBV4	481	401	0.01%	0.001%
7	3.038	518	528	540	rBV	5967	10712	0.26%	0.040%
8	3.183	561	573	585	rBV2	6707	14983	0.37%	0.055%
9	3.379	631	634	637	rVV2	465	313	0.01%	0.001%
10	3.549	682	687	690	rBV3	253	291	0.01%	0.001%
11	3.732	739	744	746	rBV2	273	248	0.01%	0.001%
12	3.793	760	763	767	rVV2	261	240	0.01%	0.001%
13	3.848	775	780	785	rBV3	310	337	0.01%	0.001%
14	4.134	866	869	873	rVB	339	245	0.01%	0.001%
15	4.166	873	879	884	rBV3	1254	1381	0.03%	0.005%
16	4.411	950	955	958	rVB2	359	283	0.01%	0.001%
17	4.633	1008	1024	1090	rBV	348101	1142714	28.10%	4.231%
18	4.996	1134	1137	1139	rBV3	418	288	0.01%	0.001%
19	5.060	1139	1157	1188	rVV	728127	1598528	39.31%	5.919%
20	5.292	1220	1229	1237	rVB6	1864	3726	0.09%	0.014%
21	5.327	1237	1240	1243	rVB2	465	309	0.01%	0.001%
22	5.359	1243	1250	1253	rBV3	864	943	0.02%	0.003%
23	5.375	1253	1255	1261	rVB5	757	612	0.02%	0.002%
24	5.430	1270	1272	1276	rBV2	481	419	0.01%	0.002%
25	5.514	1295	1298	1300	rBV2	511	352	0.01%	0.001%
26	5.526	1300	1302	1307	rVB5	583	414	0.01%	0.002%
27	5.568	1311	1315	1318	rBB2	295	263	0.01%	0.001%
28	5.597	1321	1324	1327	rBV2	380	311	0.01%	0.001%
29	5.719	1340	1362	1400	rBV2	1542989	4066829	100.00%	15.057%
30	5.977	1432	1442	1453	rBV4	5976	12617	0.31%	0.047%
31	6.115	1483	1485	1490	rVB2	773	523	0.01%	0.002%
32	6.186	1505	1507	1511	rVB3	511	326	0.01%	0.001%
33	6.247	1511	1526	1562	rBV	908039	1753388	43.11%	6.492%
34	6.481	1595	1599	1601	rBV2	504	370	0.01%	0.001%
35	6.526	1604	1613	1624	rVB8	6761	13063	0.32%	0.048%
36	6.604	1624	1637	1647	rBV8	2577	5976	0.15%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050593.D
 Acq On : 01 Sep 2022 20:06
 Operator : SY/MD
 Sample : VIBLK130
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK130

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

37	6.687	1648	1663	1692	rBV	944624	1871443	46.02%	6.929%
38	6.800	1695	1698	1700	rBV4	1565	1086	0.03%	0.004%
39	7.028	1764	1769	1771	rBV	311	259	0.01%	0.001%
40	7.047	1771	1775	1781	rVB3	283	284	0.01%	0.001%
41	7.192	1812	1820	1822	rBV3	2785	3468	0.09%	0.013%
42	7.288	1847	1850	1852	rBV	385	308	0.01%	0.001%
43	7.314	1856	1858	1861	rVB2	522	249	0.01%	0.001%
44	7.420	1887	1891	1895	rBV2	345	328	0.01%	0.001%
45	7.565	1920	1936	1957	rBV	443591	792584	19.49%	2.935%
46	7.896	2023	2039	2059	rBV	1670075	2943540	72.38%	10.898%
47	8.124	2108	2110	2114	rVB3	745	492	0.01%	0.002%
48	8.179	2114	2127	2146	rBV	291522	511066	12.57%	1.892%
49	8.472	2214	2218	2220	rVB3	430	268	0.01%	0.001%
50	8.501	2224	2227	2231	rBV3	437	240	0.01%	0.001%
51	8.552	2231	2243	2256	rVB2	40104	68304	1.68%	0.253%
52	8.645	2256	2272	2305	rBV2	1046767	2332363	57.35%	8.636%
53	8.915	2351	2356	2360	rVB4	602	580	0.01%	0.002%
54	8.948	2360	2366	2369	rBV3	435	428	0.01%	0.002%
55	9.034	2389	2393	2399	rVB3	394	493	0.01%	0.002%
56	9.070	2399	2404	2407	rBV3	463	455	0.01%	0.002%
57	9.124	2418	2421	2429	rBV3	489	483	0.01%	0.002%
58	9.224	2445	2452	2456	rVB3	371	460	0.01%	0.002%
59	9.279	2459	2469	2475	rBV2	449	839	0.02%	0.003%
60	9.417	2498	2512	2537	rBV	1165533	1953342	48.03%	7.232%
61	9.600	2567	2569	2574	rVB2	1044	537	0.01%	0.002%
62	9.687	2592	2596	2597	rBV2	453	297	0.01%	0.001%
63	9.735	2605	2611	2613	rBV2	487	577	0.01%	0.002%
64	9.883	2654	2657	2664	rBV2	409	434	0.01%	0.002%
65	9.983	2683	2688	2692	rBV2	334	362	0.01%	0.001%
66	10.060	2708	2712	2718	rVB2	535	524	0.01%	0.002%
67	10.105	2719	2726	2729	rBV2	887	1051	0.03%	0.004%
68	10.237	2764	2767	2769	rBV2	426	255	0.01%	0.001%
69	10.369	2804	2808	2811	rBV2	261	241	0.01%	0.001%
70	10.391	2812	2815	2818	rVB3	423	316	0.01%	0.001%
71	10.491	2844	2846	2852	rVB3	508	417	0.01%	0.002%
72	10.591	2873	2877	2883	rBV3	382	450	0.01%	0.002%
73	10.703	2910	2912	2916	rBV3	315	271	0.01%	0.001%
74	10.758	2916	2929	2953	rVV	1325520	2139876	52.62%	7.923%
75	11.118	3037	3041	3046	rVV2	1083	827	0.02%	0.003%
76	11.140	3046	3048	3055	rVB2	326	277	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050593.D
 Acq On : 01 Sep 2022 20:06
 Operator : SY/MD
 Sample : VIBLK130
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK130

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis

77	11.410	3128	3132	3138	rVB4	1206	1221	0.03%	0.005%
78	11.468	3144	3150	3154	rBV3	736	957	0.02%	0.004%
79	11.510	3159	3163	3165	rVB2	567	450	0.01%	0.002%
80	11.529	3166	3169	3174	rBV2	387	478	0.01%	0.002%
81	11.587	3183	3187	3191	rVB	414	360	0.01%	0.001%
82	11.616	3191	3196	3198	rBV	409	352	0.01%	0.001%
83	11.722	3226	3229	3233	rVB3	515	389	0.01%	0.001%
84	11.748	3233	3237	3244	rBV3	948	926	0.02%	0.003%
85	11.812	3244	3257	3277	rBV	952522	1471093	36.17%	5.447%
86	12.195	3362	3376	3402	rBV	1407883	2251099	55.35%	8.335%
87	12.465	3457	3460	3463	rBV3	582	443	0.01%	0.002%
88	12.562	3487	3490	3494	rBV3	373	304	0.01%	0.001%
89	12.783	3556	3559	3563	rBV4	393	375	0.01%	0.001%
90	13.124	3663	3665	3669	rBV3	338	243	0.01%	0.001%
91	13.189	3681	3685	3688	rBV	291	284	0.01%	0.001%
92	13.311	3720	3723	3726	rBV2	968	873	0.02%	0.003%
93	13.844	3886	3889	3890	rBV	689	359	0.01%	0.001%
94	13.947	3918	3921	3923	rBV2	470	297	0.01%	0.001%
95	14.217	4003	4005	4008	rBV	648	399	0.01%	0.001%
96	14.269	4019	4021	4024	rBV	516	415	0.01%	0.002%
97	14.478	4084	4086	4088	rBV	687	375	0.01%	0.001%
98	14.758	4170	4173	4176	rVB2	628	410	0.01%	0.002%
99	14.931	4225	4227	4230	rBV3	489	271	0.01%	0.001%
100	15.079	4268	4273	4275	rBV3	734	631	0.02%	0.002%




Sum of corrected areas: 27008939

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050593.D
Acq On : 01 Sep 2022 20:06
Operator : SY/MD
Sample : VIBLK130
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK130

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

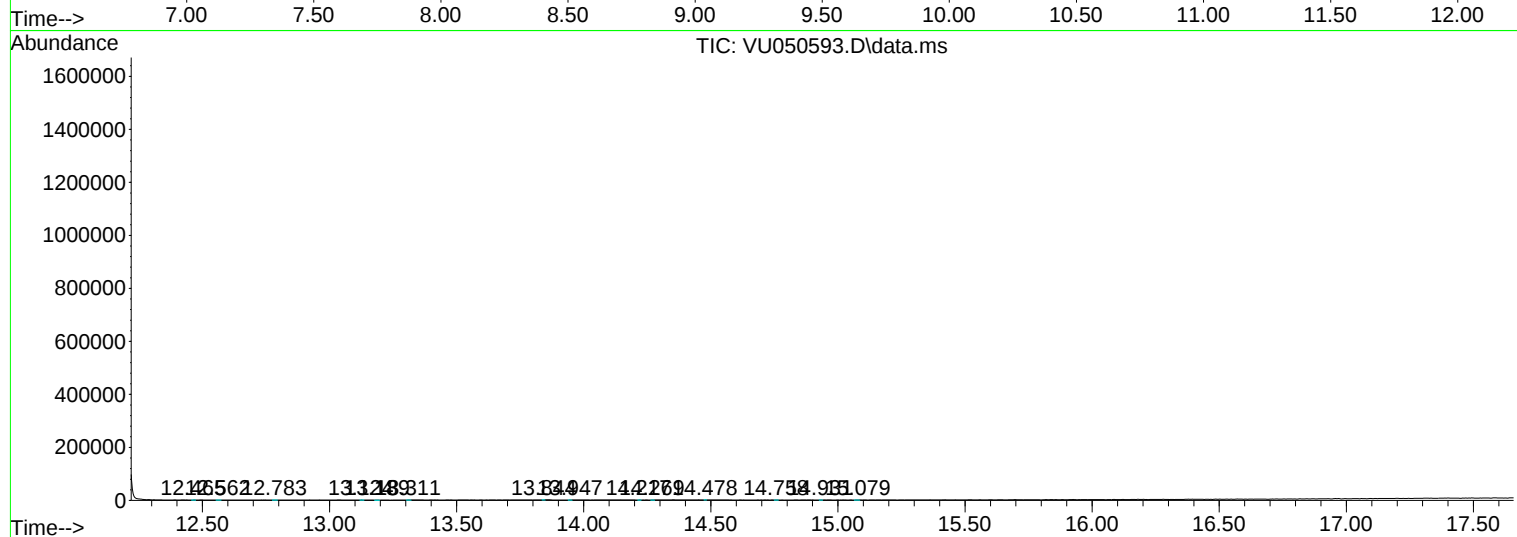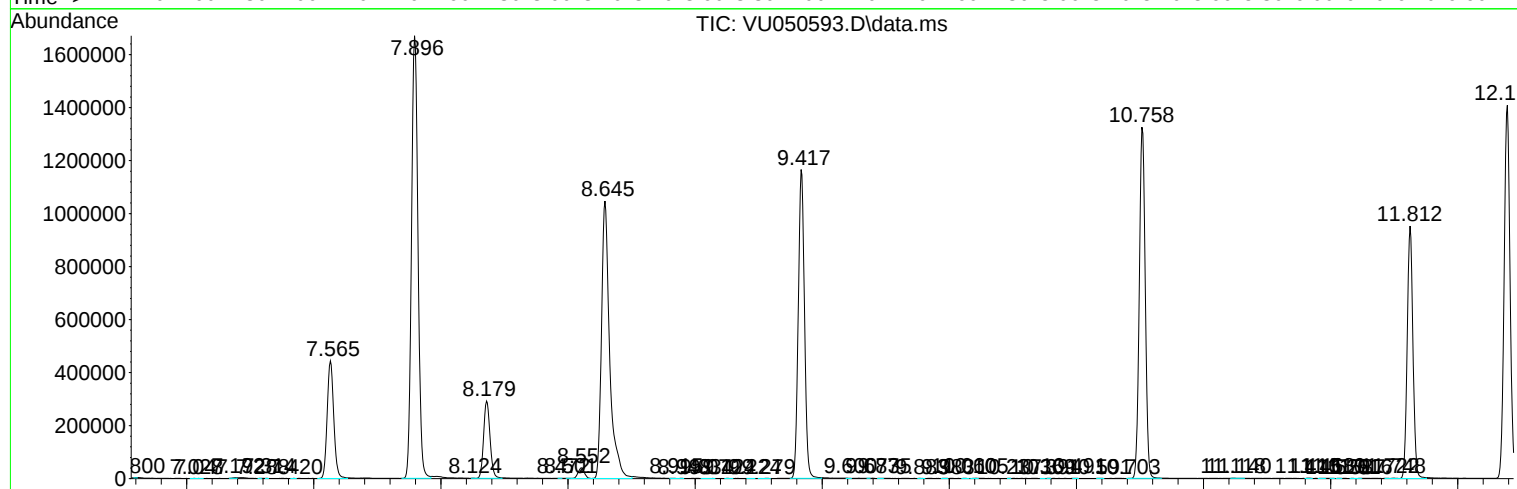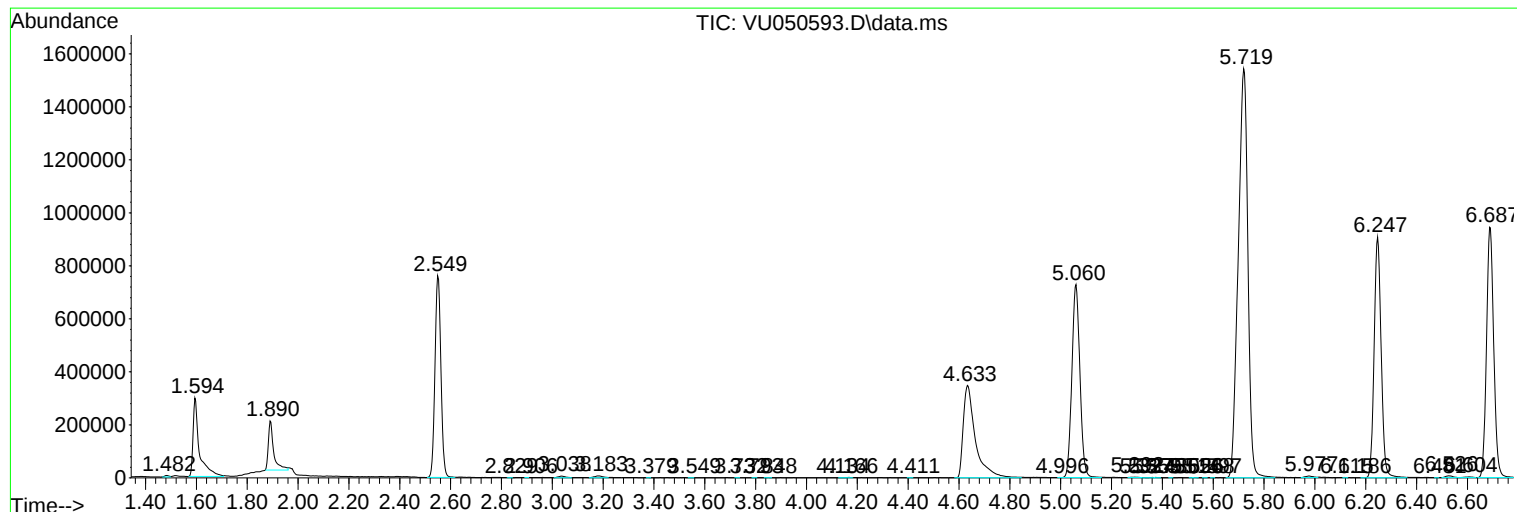

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050593.D
Acq On : 01 Sep 2022 20:06
Operator : SY/MD
Sample : VIBLK130
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK130

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
Data File : VU050593.D
Acq On : 01 Sep 2022 20:06
Operator : SY/MD
Sample : VIBLK130
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK130

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------