


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090122\
 Data File : VU050574.D
 Acq On : 01 Sep 2022 09:47
 Operator : SY/MD
 Sample : BFB117
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB117

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Title : VOC Analysis
 Last Update : Fri Sep 02 02:07:32 2022

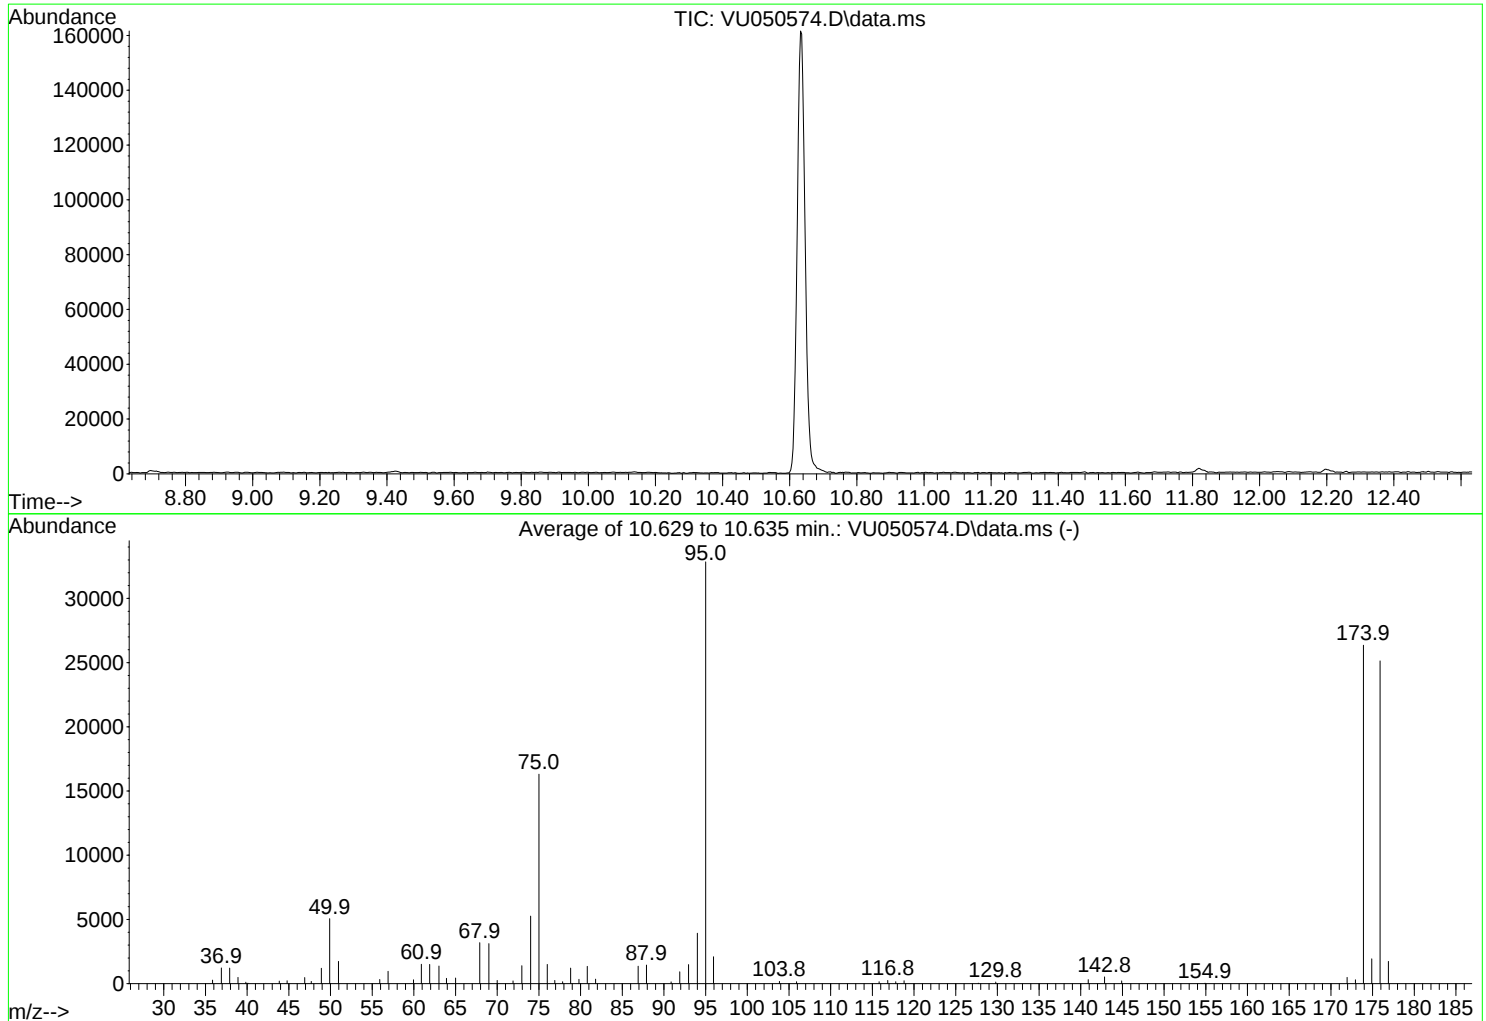

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	5056	PASS
75	95	30	80	49.7	16317	PASS
95	95	100	100	100.0	32848	PASS
96	95	5	9	6.4	2097	PASS
173	174	0.00	2	1.2	304	PASS
174	95	50	120	80.2	26349	PASS
175	174	5	9	7.3	1929	PASS
176	174	95	101	95.4	25128	PASS
177	176	5	9	6.9	1731	PASS

m/z	Abundance
43.80	330.0

Instrument :
MSVOA_U
ClientSampleId :
BFB117

m/z	Abundance
35.90	240.0
36.90	1212.0
37.90	1154.0
38.90	511.0
39.90	104.0
43.90	533.0
44.80	264.0
46.90	518.0
47.70	164.0
48.90	1182.0
49.90	4962.0
51.00	1735.0
55.90	327.0
56.90	907.0
59.90	357.0
60.90	1482.0
61.90	1506.0
63.00	1341.0
63.90	420.0
65.00	487.0
67.90	3008.0
69.00	2891.0
70.00	245.0
71.90	199.0
72.90	1316.0
74.00	5186.0
75.00	15754.0
76.00	1522.0
76.90	217.0
77.90	151.0
78.80	1166.0
79.80	309.0
80.80	1237.0
81.80	315.0
86.90	1334.0
87.90	1305.0
90.80	116.0
91.90	885.0
93.00	1375.0
94.00	3711.0
95.00	31080.0
95.90	2039.0
103.90	137.0
105.90	144.0
115.80	120.0
116.90	245.0
117.80	122.0
118.80	159.0
129.80	137.0
140.90	270.0
142.80	491.0
144.90	262.0
171.90	481.0
172.90	249.0
173.90	24256.0
174.90	1823.0
175.90	23424.0
176.90	1696.0

Instrument :
MSVOA_U
ClientSampleId :
BFB117

m/z	Abundance
35.90	280.0
36.90	1230.0
37.90	1254.0
38.90	499.0
39.90	108.0
43.90	556.0
44.80	234.0
46.90	503.0
47.70	181.0
48.90	1222.0
49.90	5237.0
51.00	1772.0
55.90	346.0
56.90	1000.0
59.90	304.0
60.90	1525.0
61.90	1523.0
63.00	1397.0
63.90	434.0
65.00	441.0
67.90	3348.0
69.00	3193.0
70.00	254.0
71.90	241.0
72.90	1442.0
74.00	5361.0
75.00	16912.0
76.00	1544.0
76.90	250.0
77.80	140.0
78.80	1244.0
79.80	336.0
80.80	1416.0
81.80	368.0
86.90	1401.0
87.90	1475.0
90.90	138.0
91.90	932.0
93.00	1505.0
94.00	3997.0
95.00	33824.0
95.90	2148.0
103.80	194.0
105.90	138.0
115.80	147.0
116.80	256.0
117.80	163.0
118.80	234.0
129.80	125.0
140.90	321.0
142.80	553.0
144.90	212.0
171.90	478.0
173.00	291.0
173.90	27304.0
174.90	1963.0
175.90	25896.0
176.90	1789.0

Instrument :
MSVOA_U
ClientSampleId :
BFB117

m/z	Abundance
35.80	296.0
36.90	1229.0
37.90	1232.0
38.90	457.0
39.80	112.0
40.10	124.0
43.90	484.0
44.80	180.0
46.90	420.0
47.70	190.0
48.90	1189.0
49.90	4970.0
50.90	1689.0
55.90	317.0
56.90	993.0
60.00	251.0
60.90	1510.0
61.90	1446.0
63.00	1390.0
63.90	363.0
65.00	396.0
67.90	3205.0
69.00	3280.0
70.00	252.0
71.90	202.0
73.00	1426.0
74.00	5244.0
75.00	16284.0
76.00	1414.0
76.90	274.0
77.80	155.0
78.80	1223.0
79.80	358.0
80.80	1398.0
81.80	381.0
86.90	1348.0
87.90	1559.0
90.90	146.0
91.90	950.0
92.90	1585.0
94.00	4072.0
95.00	33640.0
96.00	2103.0
103.80	209.0
105.90	151.0
115.80	171.0
116.80	256.0
117.80	148.0
118.80	274.0
127.70	112.0
129.80	130.0
140.90	332.0
142.90	517.0
144.90	183.0
154.90	105.0
172.00	491.0
173.00	372.0
173.90	27488.0
174.90	2000.0
175.90	26064.0
176.90	1709.0

Instrument :
MSVOA_U
ClientSampleId :
BFB117