

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090123\
 Data File : VU055045.D
 Acq On : 01 Sep 2023 17:15
 Operator : MD/SY
 Sample : 04153-04DL 1000X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH461DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU055045.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	109	rBV	63773	73475	6.17%	0.954%
2	1.907	185	192	207	rVB	73103	94792	7.96%	1.230%
3	2.563	384	396	413	rBV	137209	226564	19.02%	2.941%
4	3.039	532	544	560	rBV3	30020	59304	4.98%	0.770%
5	4.660	1028	1048	1078	rBV2	234504	742596	62.33%	9.638%
6	5.062	1156	1173	1198	rBV	129880	301214	25.28%	3.909%
7	5.724	1356	1379	1399	rBV2	268003	692799	58.15%	8.992%
8	6.245	1528	1541	1569	rBV	252395	487776	40.94%	6.331%
9	6.541	1618	1633	1664	rBV	612501	1191383	100.00%	15.463%
10	6.689	1666	1679	1695	rVB	168446	327768	27.51%	4.254%
11	7.563	1941	1951	1978	rBV	64289	121823	10.23%	1.581%
12	7.898	2041	2055	2091	rBV	320224	585749	49.17%	7.602%
13	8.181	2132	2143	2162	rBV3	35940	65568	5.50%	0.851%
14	8.634	2273	2284	2318	rBV2	297273	676153	56.75%	8.776%
15	9.415	2515	2527	2552	rBV	364372	630391	52.91%	8.182%
16	10.753	2931	2943	2959	rBV	118889	197414	16.57%	2.562%
17	11.811	3260	3272	3295	rBV	401183	663258	55.67%	8.608%
18	12.193	3376	3391	3409	rBV	311495	518894	43.55%	6.735%
19	13.843	3895	3904	3916	rBV4	14913	22390	1.88%	0.291%
20	14.097	3974	3983	3994	rBV3	6980	12614	1.06%	0.164%
21	14.331	4048	4056	4070	rBV5	8392	12906	1.08%	0.168%




Sum of corrected areas: 7704831

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090123\
Data File : VU055045.D
Acq On : 01 Sep 2023 17:15
Operator : MD/SY
Sample : 04153-04DL 1000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH461DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

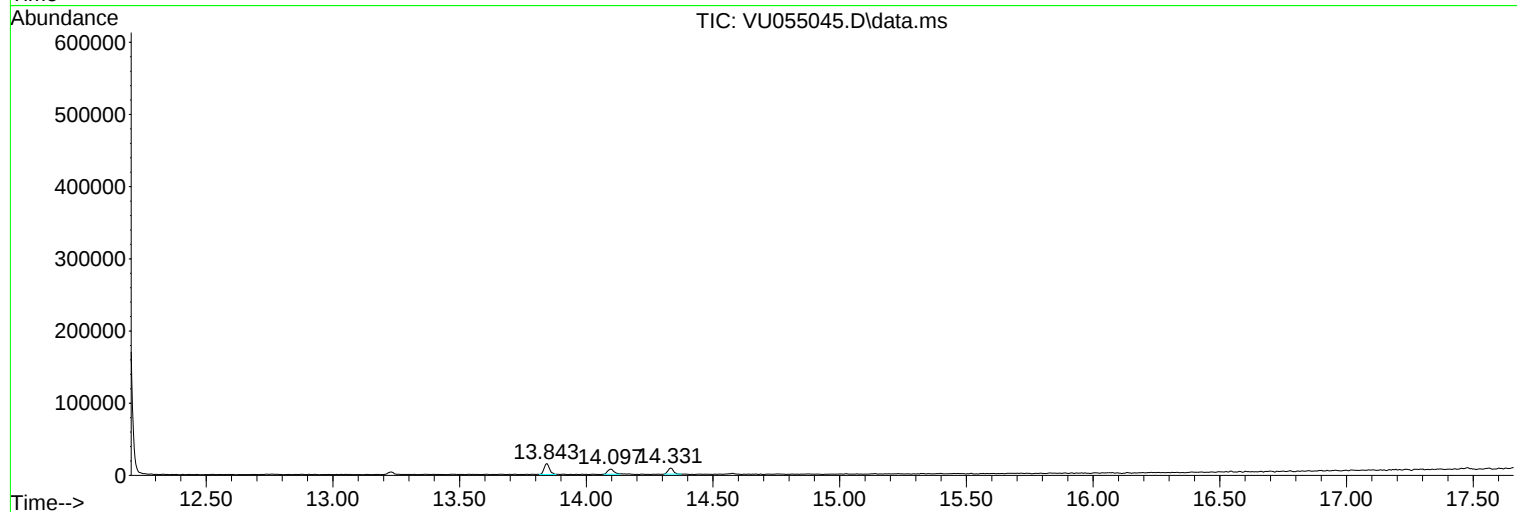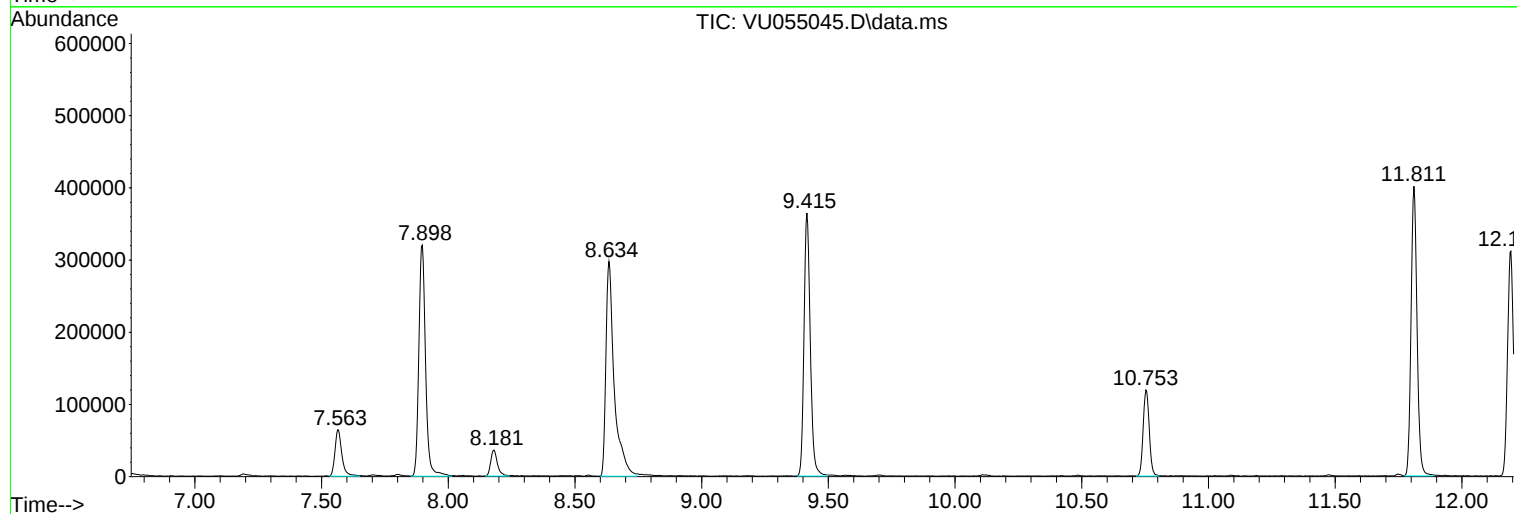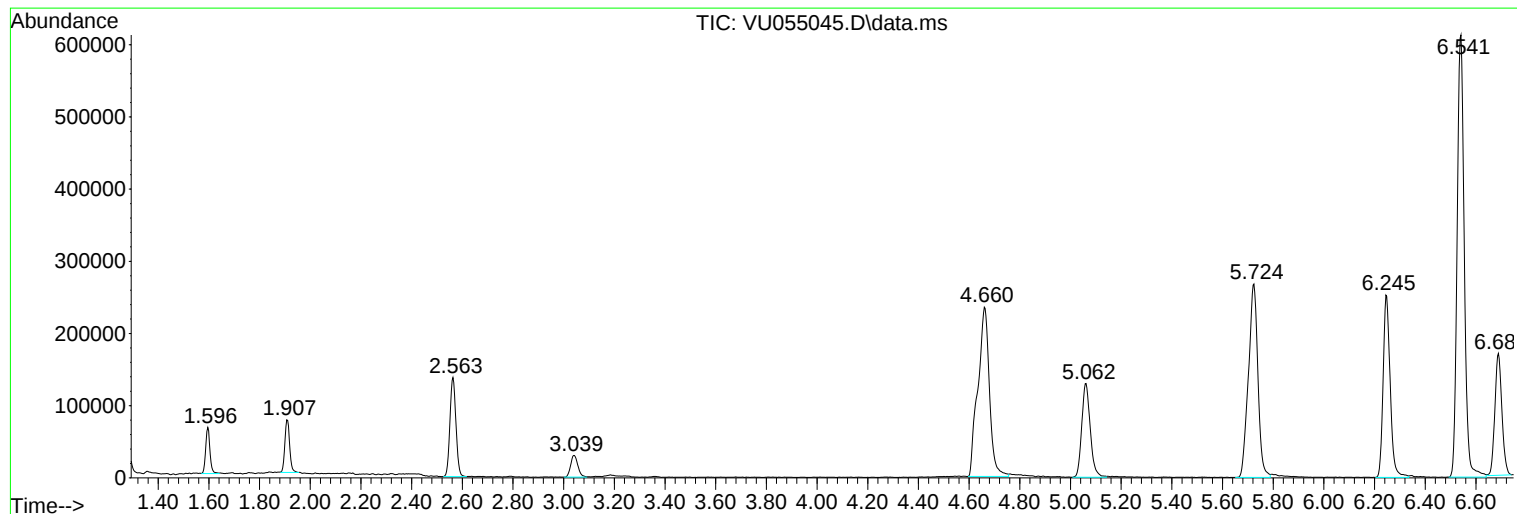

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090123\
Data File : VU055045.D
Acq On : 01 Sep 2023 17:15
Operator : MD/SY
Sample : 04153-04DL 1000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH461DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090123\
Data File : VU055045.D
Acq On : 01 Sep 2023 17:15
Operator : MD/SY
Sample : 04153-04DL 1000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH461DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc