

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090123\
 Data File : VU055076.D
 Acq On : 02 Sep 2023 05:56
 Operator : MD/SY
 Sample : 04250-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4C0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU055076.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	65	95	107	rBV2	83028	204795	8.77%	2.420%
2	1.911	186	193	205	rVB	72391	91613	3.92%	1.083%
3	2.567	384	397	416	rBV2	146109	268676	11.50%	3.175%
4	4.631	1027	1039	1069	rBV	75048	264869	11.34%	3.130%
5	5.058	1157	1172	1198	rBV	124967	297458	12.73%	3.515%
6	5.721	1359	1378	1403	rBV2	253892	669467	28.66%	7.912%
7	6.248	1525	1542	1565	rBV	241035	475586	20.36%	5.620%
8	6.541	1617	1633	1654	rBV2	125722	247299	10.59%	2.923%
9	6.689	1665	1679	1696	rBV	160314	313770	13.43%	3.708%
10	7.566	1940	1952	1970	rBV2	54199	100482	4.30%	1.188%
11	7.894	2040	2054	2073	rBV	304082	543304	23.26%	6.421%
12	8.181	2131	2143	2155	rBV2	31089	54726	2.34%	0.647%
13	8.550	2244	2258	2274	rBV	1354052	2335898	100.00%	27.606%
14	8.634	2274	2284	2321	rVB3	258481	610121	26.12%	7.210%
15	9.415	2515	2527	2549	rBV	361324	639493	27.38%	7.558%
16	10.753	2931	2943	2961	rBV	109434	178488	7.64%	2.109%
17	11.811	3260	3272	3293	rBV	396392	656680	28.11%	7.761%
18	12.065	3341	3351	3365	rBV5	14833	28795	1.23%	0.340%
19	12.190	3379	3390	3415	rVB	288339	480118	20.55%	5.674%




Sum of corrected areas: 8461638

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090123\
Data File : VU055076.D
Acq On : 02 Sep 2023 05:56
Operator : MD/SY
Sample : 04250-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4C0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

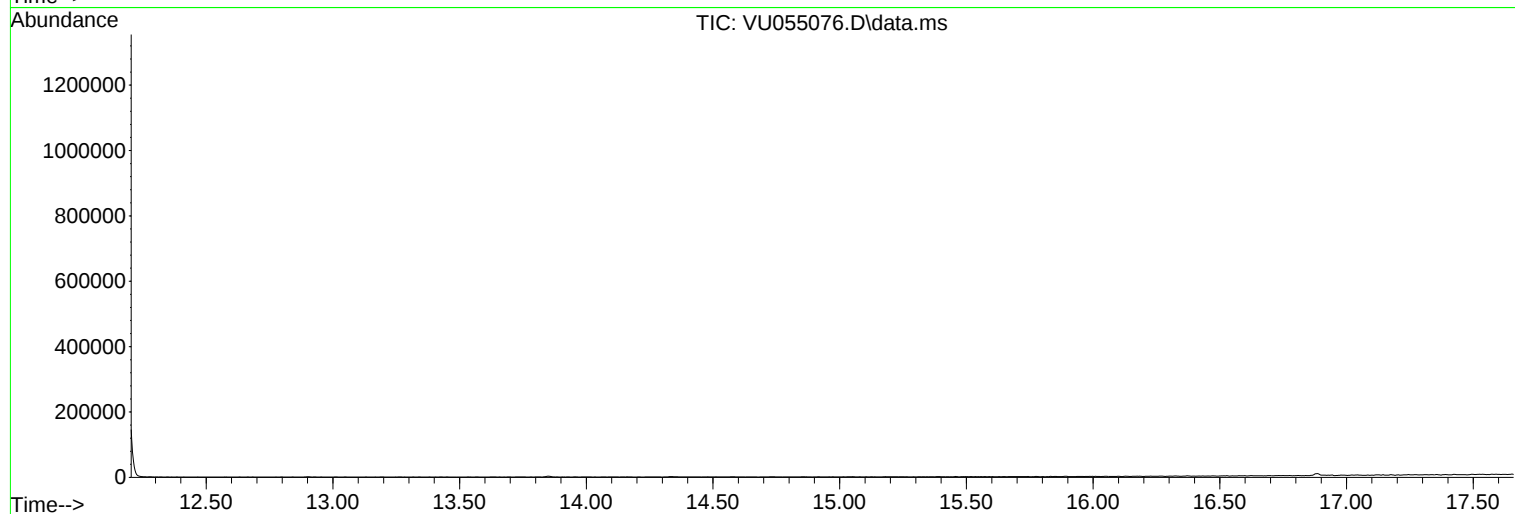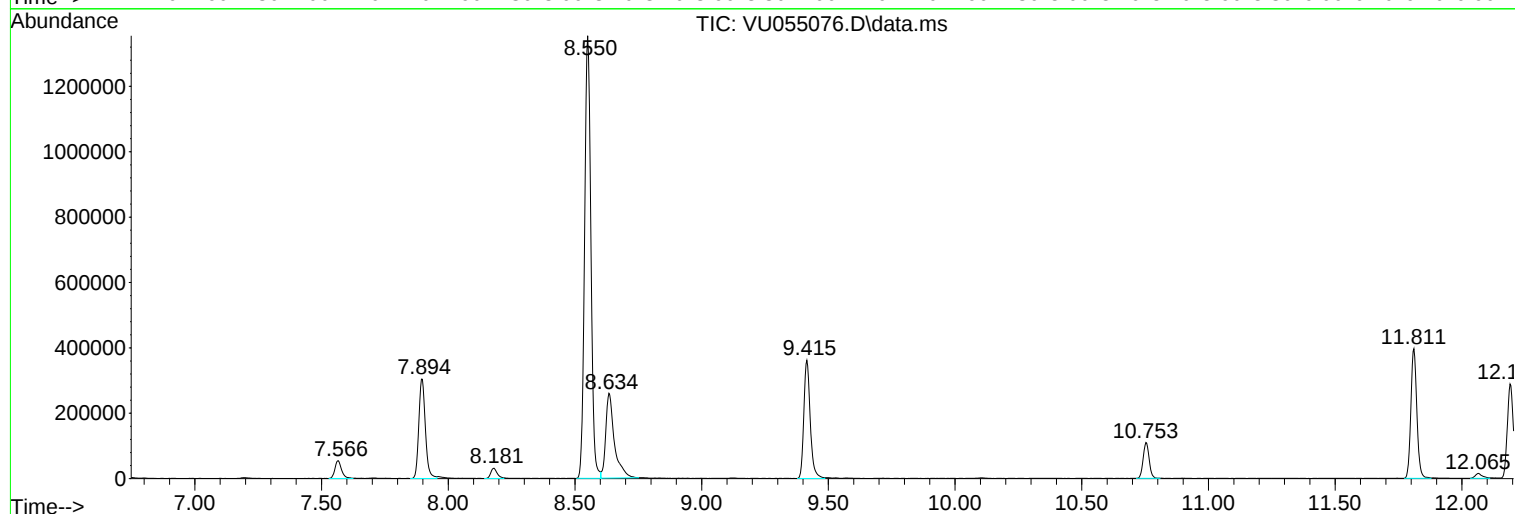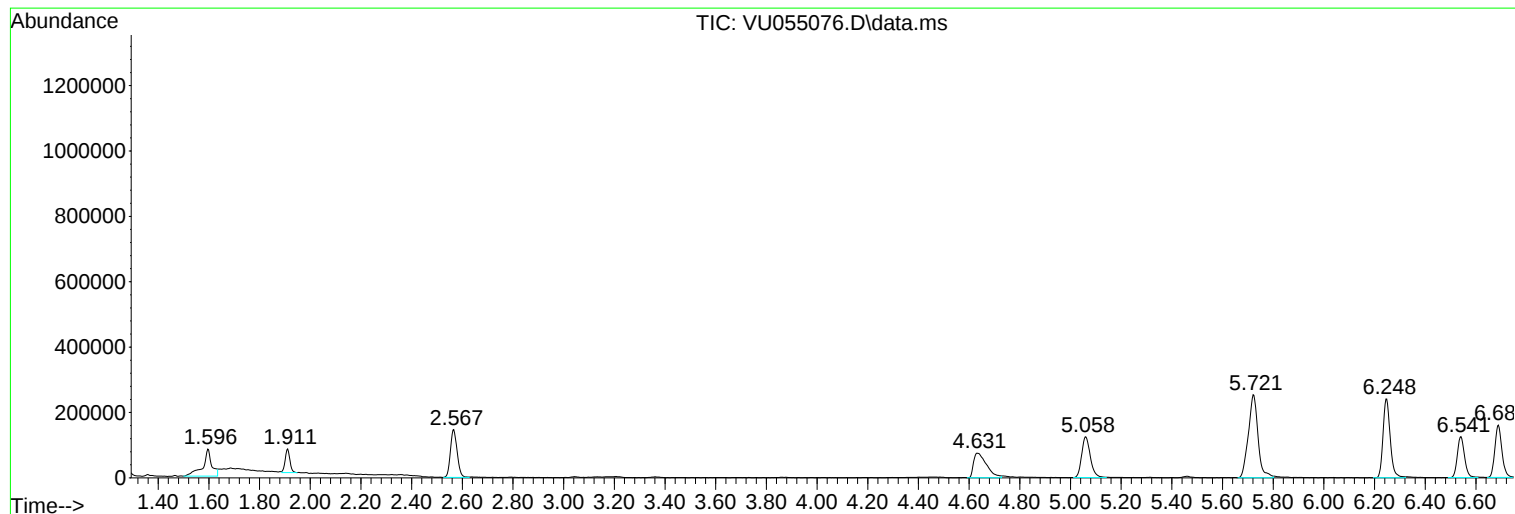

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090123\
Data File : VU055076.D
Acq On : 02 Sep 2023 05:56
Operator : MD/SY
Sample : 04250-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4C0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090123\
Data File : VU055076.D
Acq On : 02 Sep 2023 05:56
Operator : MD/SY
Sample : 04250-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4C0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------