


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090123\
Data File : VU055034.D
Acq On : 01 Sep 2023 11:42
Operator : MD/SY
Sample : BFB038
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB038

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Sep 06 05:03:37 2023

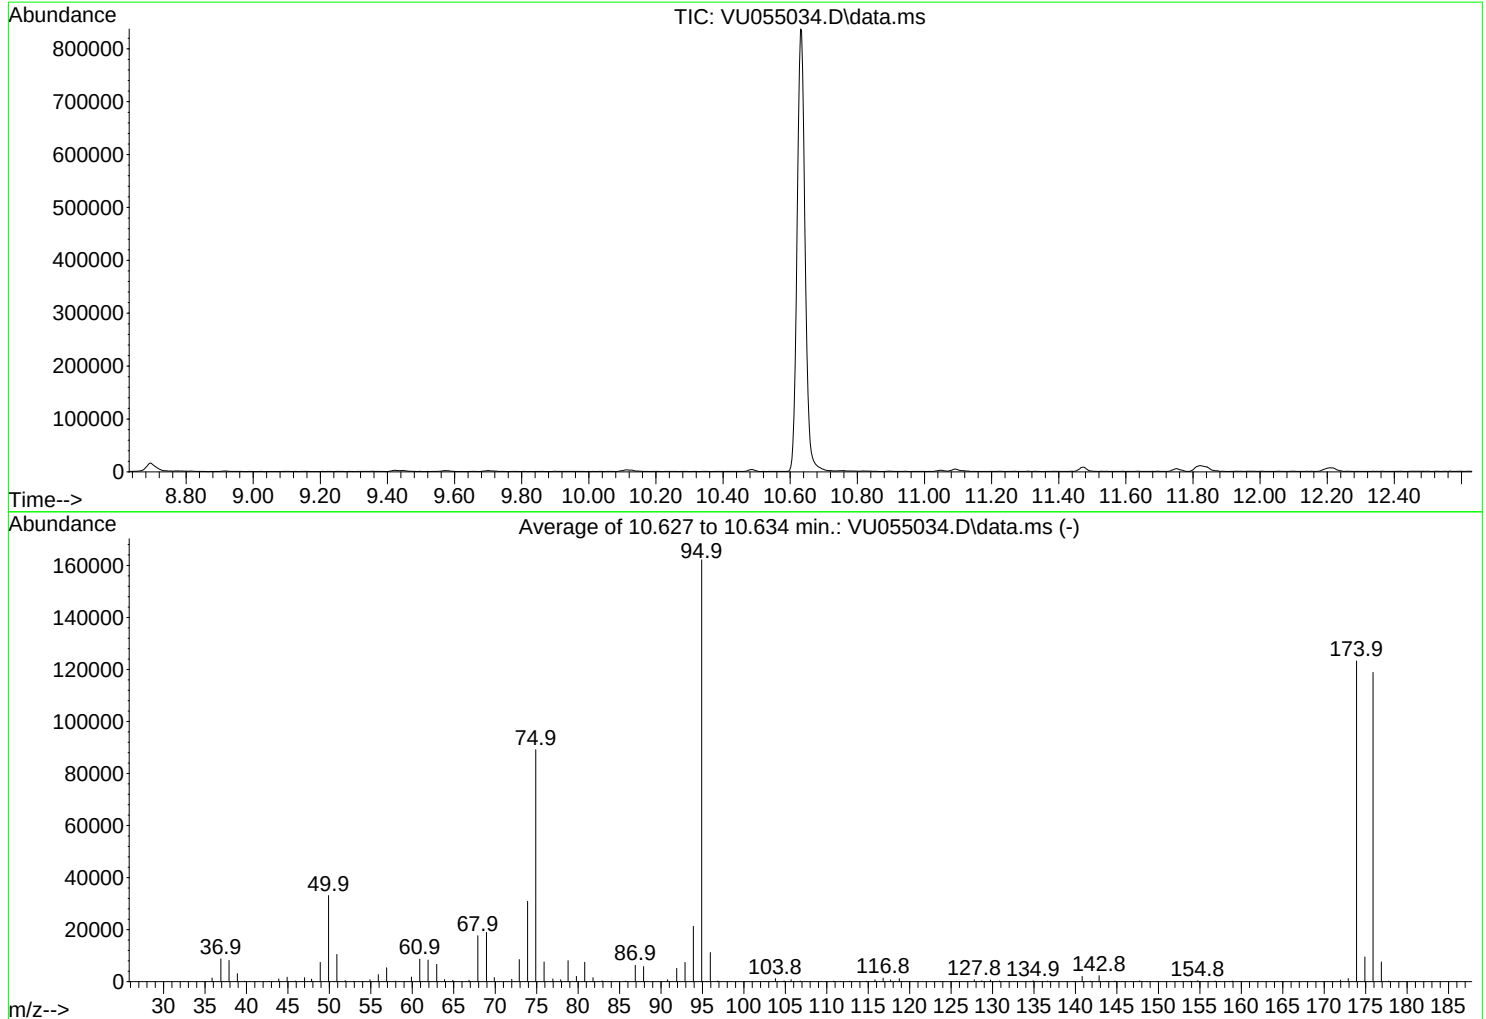

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	33099	PASS
75	95	30	80	55.0	89208	PASS
95	95	100	100	100.0	162133	PASS
96	95	5	9	6.9	11171	PASS
173	174	0.00	2	1.0	1200	PASS
174	95	50	120	76.0	123267	PASS
175	174	5	9	7.7	9489	PASS
176	174	95	101	96.5	118909	PASS
177	176	5	9	6.4	7562	PASS

Scan 2891 (10.586 min): VU055034.D\data.ms
BFB038

m/z	Abundance
39.90	190.0
44.00	777.0

Instrument :
MSVOA_U
ClientSampleId :
BFB038

m/z	Abundance
35.90	1573.0
36.90	8539.0
37.90	8202.0
38.90	3049.0
39.80	317.0
42.90	110.0
43.90	1648.0
44.90	1485.0
45.90	304.0
47.00	1516.0
47.90	927.0
48.90	6962.0
49.90	31768.0
50.90	10110.0
51.90	402.0
52.90	100.0
54.90	679.0
55.90	2604.0
56.90	4978.0
58.00	193.0
59.90	1899.0
60.90	8335.0
61.90	8182.0
62.90	6382.0
63.90	715.0
64.90	616.0
66.90	449.0
67.90	16198.0
69.00	18032.0
69.90	1558.0
72.00	794.0
72.90	7692.0
73.90	29480.0
74.90	85704.0
75.90	7389.0
76.90	970.0
77.90	754.0
78.80	7939.0
79.80	2000.0
80.80	7074.0
81.80	1548.0
82.90	294.0
85.70	226.0
86.90	6021.0
87.90	5317.0
90.80	778.0
91.90	4804.0
92.90	6576.0
93.90	20752.0
94.90	152960.0
96.00	10705.0
96.90	203.0
102.70	152.0
103.80	1026.0
104.80	330.0
105.70	722.0
106.80	197.0
110.90	211.0
111.60	118.0
112.80	143.0
114.70	178.0
115.80	686.0
116.80	1271.0
117.70	571.0
118.80	1027.0
123.70	122.0
127.80	792.0
128.70	439.0
129.70	570.0
130.90	250.0
134.90	352.0
136.60	228.0
139.70	136.0
140.80	1935.0
141.80	166.0
142.90	2106.0
143.70	135.0
144.80	231.0
145.60	242.0
146.80	120.0
147.80	455.0
148.70	122.0
150.00	135.0
153.90	142.0
154.80	390.0
156.80	319.0
158.90	270.0
161.00	140.0
170.90	125.0
171.90	594.0
172.90	1080.0
173.90	113256.0

Instrument :
MSVOA_U
ClientSampleId :
BFB038

174.90	8601.0
175.90	109680.0
176.90	6701.0
177.80	290.0

Instrument :
MSVOA_U
ClientSampleId :
BFB038

m/z	Abundance
35.80	1448.0
36.90	9278.0
37.90	8440.0
38.90	3191.0
39.80	348.0
42.70	132.0
43.90	1865.0
44.90	1785.0
45.90	298.0
47.00	1560.0
47.90	976.0
48.90	7496.0
49.90	34088.0
50.90	10792.0
51.90	418.0
52.90	116.0
54.90	826.0
55.90	2816.0
56.90	5564.0
58.00	254.0
59.90	1867.0
60.90	9055.0
61.90	8607.0
62.90	6832.0
63.90	826.0
64.90	599.0
66.80	571.0
67.90	18176.0
69.00	19512.0
69.90	1554.0
72.00	910.0
72.90	8800.0
73.90	31832.0
74.90	91936.0
75.90	7803.0
76.90	1049.0
77.90	765.0
78.80	8417.0
79.80	2140.0
80.80	7602.0
81.80	1624.0
82.90	319.0
83.70	127.0
85.80	266.0
86.90	6376.0
87.90	5946.0
90.80	798.0
91.90	5235.0
92.90	7538.0
93.90	21872.0
94.90	166912.0
95.90	11493.0
96.80	282.0
102.60	138.0
103.80	1248.0
104.90	330.0
105.70	824.0
106.80	276.0
110.90	248.0
111.70	154.0
112.70	175.0
114.80	218.0
115.80	826.0
116.80	1404.0
117.70	734.0
118.80	1218.0
123.70	106.0
125.70	104.0
127.80	752.0
128.70	411.0
129.70	660.0
130.90	309.0
134.90	367.0
136.70	279.0
139.70	149.0
140.80	2145.0
141.80	208.0
142.90	2334.0
143.70	150.0
144.70	256.0
145.60	217.0
146.80	164.0
147.80	390.0
149.90	180.0
152.90	156.0
153.90	159.0
154.80	484.0
156.90	261.0
158.90	255.0
161.10	144.0
170.90	158.0
172.00	605.0

Instrument :
MSVOA_U
ClientSampleId :
BFB038

172.90	1260.0
173.90	127040.0
174.90	9841.0
175.90	122552.0
176.90	7845.0
177.80	292.0

Instrument :
MSVOA_U
ClientSampleId :
BFB038

m/z	Abundance
35.80	1273.0
36.90	8651.0
37.90	7895.0
38.90	3091.0
39.80	395.0
42.70	165.0
43.90	1923.0
44.90	1884.0
45.90	231.0
47.00	1532.0
47.80	1002.0
48.90	7653.0
49.90	33440.0
50.90	10444.0
51.90	404.0
52.90	114.0
54.90	821.0
55.90	2730.0
56.90	5480.0
57.90	265.0
59.90	1687.0
60.90	8693.0
61.90	8179.0
63.00	6668.0
63.90	810.0
64.90	521.0
66.80	576.0
67.90	18648.0
68.90	19280.0
69.90	1448.0
72.00	1098.0
72.90	8965.0
73.90	31400.0
74.90	89984.0
75.90	7517.0
77.00	1129.0
77.90	715.0
78.80	7888.0
79.80	2047.0
80.80	7744.0
81.80	1537.0
82.90	287.0
83.70	112.0
85.80	248.0
86.90	6520.0
87.90	6038.0
90.80	724.0
91.90	5227.0
92.90	7952.0
93.90	21232.0
94.90	166528.0
95.90	11315.0
96.80	366.0
103.80	1214.0
104.80	348.0
105.70	853.0
106.80	263.0
110.80	268.0
111.70	138.0
112.70	236.0
114.90	202.0
115.80	802.0
116.80	1342.0
117.70	789.0
118.70	1263.0
125.60	118.0
127.80	621.0
128.70	337.0
129.80	648.0
130.80	356.0
134.90	319.0
136.70	308.0
139.80	133.0
140.80	2074.0
141.80	221.0
142.80	2460.0
143.80	179.0
144.70	269.0
145.80	176.0
146.80	166.0
147.70	361.0
149.90	212.0
152.90	170.0
153.90	183.0
154.70	495.0
156.90	235.0
158.60	166.0
159.00	167.0
161.00	148.0
170.70	160.0
172.00	602.0
172.90	1259.0

Instrument :
MSVOA_U
ClientSampleId :
BFB038

173.90	129504.0
174.90	10024.0
175.90	124496.0
176.90	8141.0
177.80	252.0

Instrument :
MSVOA_U
ClientSampleId :
BFB038