

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090219\
 Data File : VU034142.D
 Acq On : 31 Aug 2019 23:50
 Operator : JC/SP
 Sample : K4526-23
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 T9-12-13-D-(0)

Quant Time: Sep 01 05:38:30 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 29 04:11:12 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.96	168	448028	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.87	114	716972	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.07	117	714428	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.47	152	348709	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.29	65	284495	49.56	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.12%	
35) Dibromofluoromethane	4.86	113	235124	47.28	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.56%	
50) Toluene-d8	7.55	98	931939	50.05	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.10%	
62) 4-Bromofluorobenzene	10.29	95	325977	45.01	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.02%	
Target Compounds						
20) Methylene Chloride	2.69	84	10902	1.966	ug/l	96
43) Isopropyl Acetate	5.53	43	73394	6.353	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU090219\
Data File : VU034142.D
Acq On : 31 Aug 2019 23:50
Operator : JC/SP
Sample : K4526-23
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
T9-12-13-D-(0)

Quant Time: Sep 01 05:38:30 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 29 04:11:12 2019
Response via : Initial Calibration

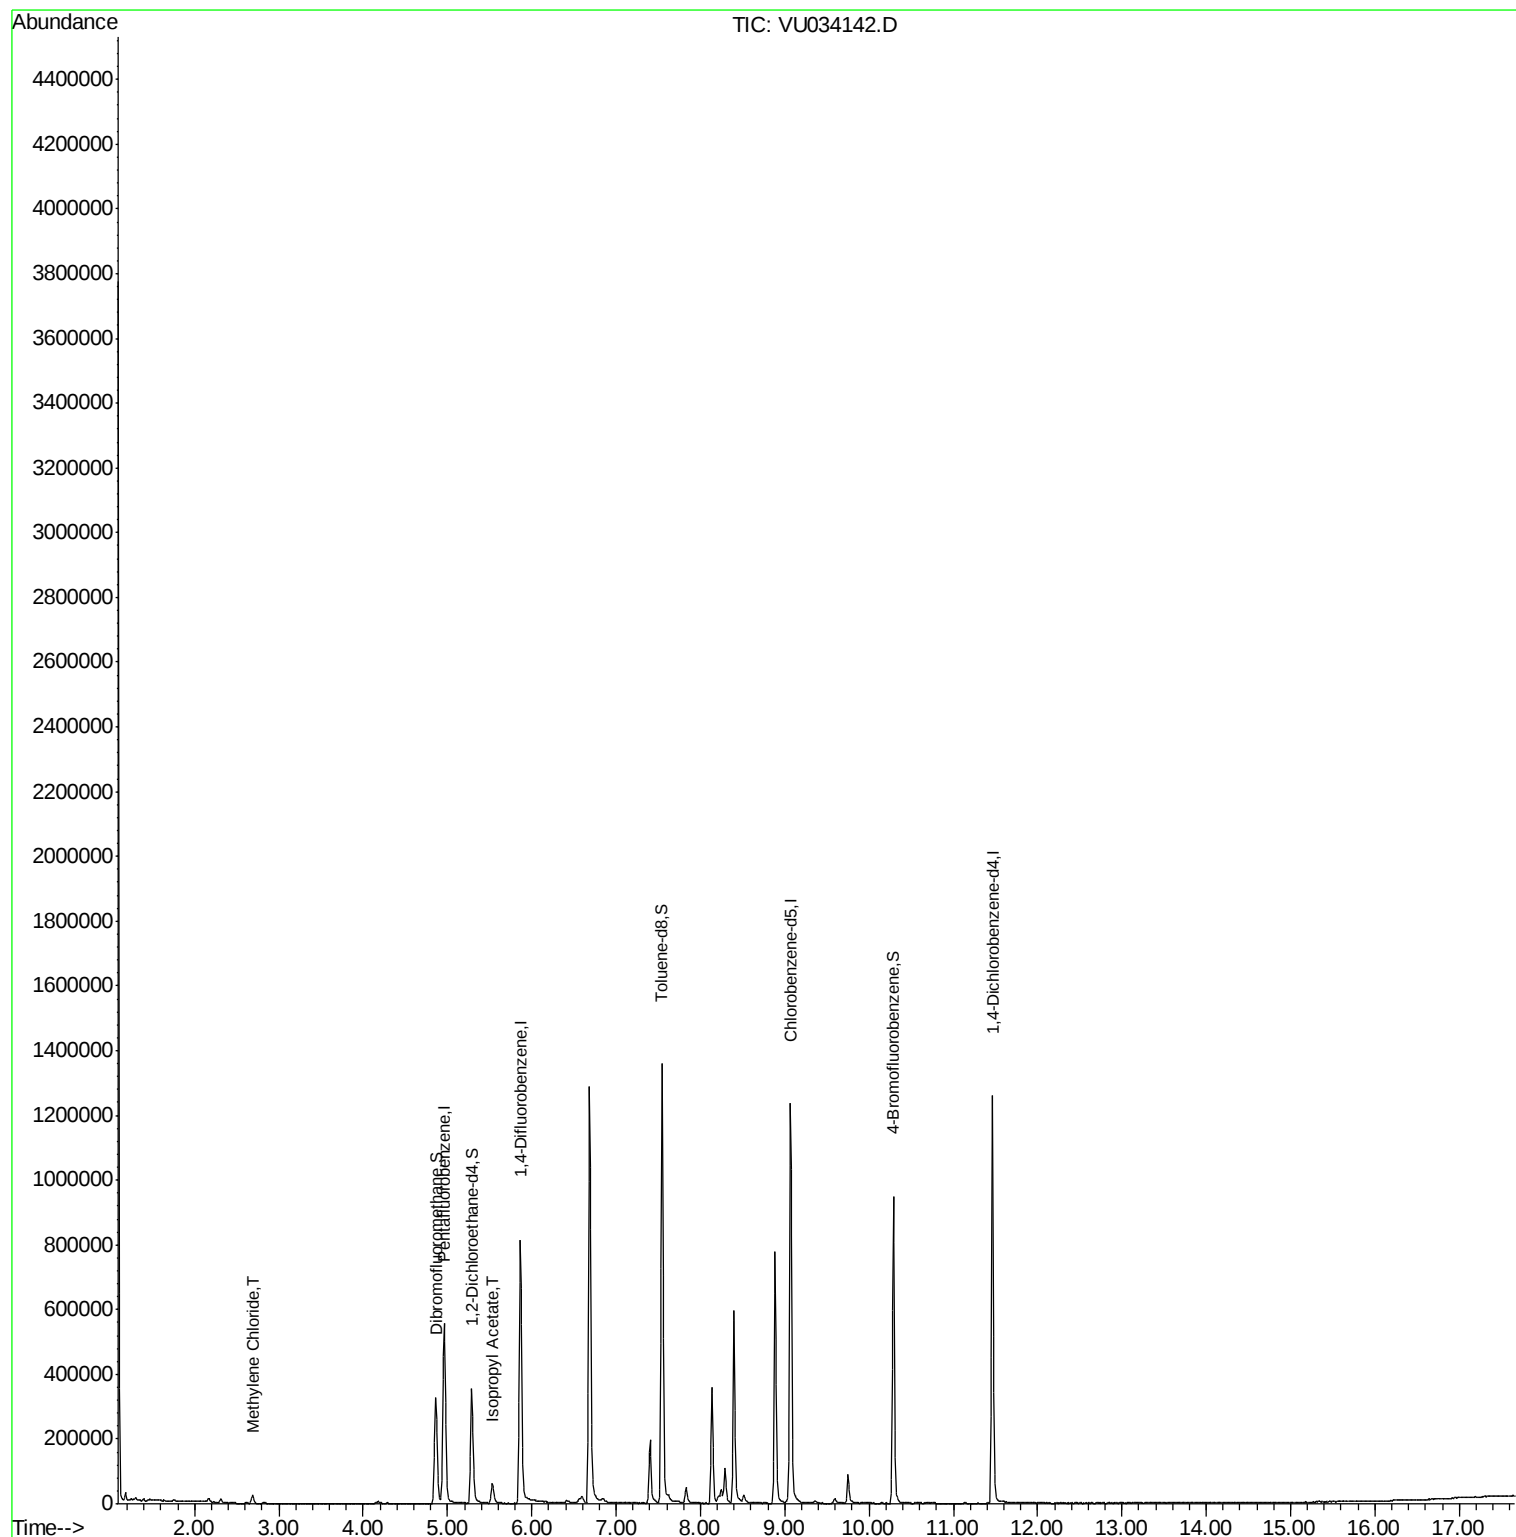



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.96 min Scan# 1204

Delta R.T. 0.00 min

Lab File: VU034142.D

Acq: 31 Aug 2019 23:50

Instrument :

MSVOA_U

ClientSampleId :


T9-12-13-D-(0)

Tot Ion:168 Resp: 448028

Ion Ratio Lower Upper

168 100

99 52.7 42.3 63.5

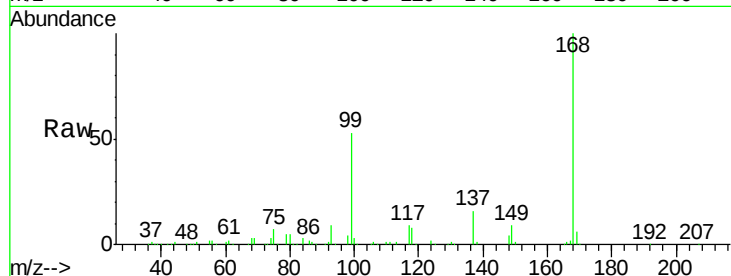

Abundance Ion 167.90 (167.60 to 168.60): VU034142.D (-1110) (-)

Ion 98.90 (98.60 to 99.60): VU034142.D (-1110) (-)

4.96

200000

150000



100000

50000

0

4.90 5.00

Time-->

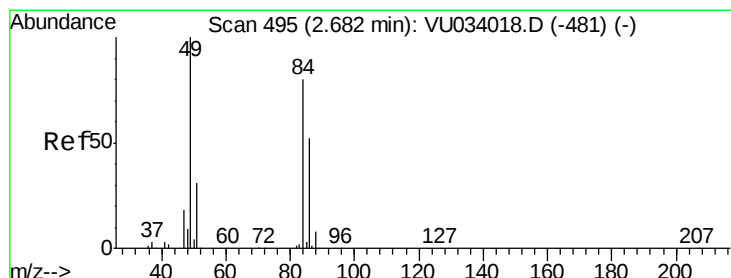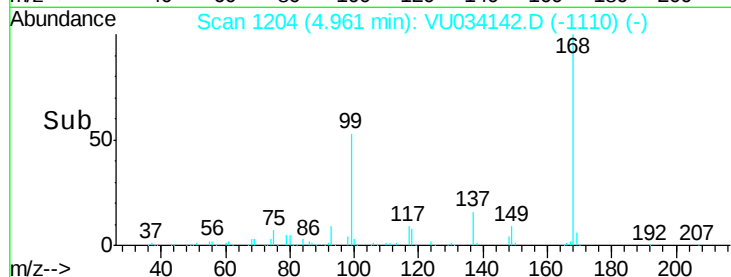

#20

Methylene Chloride

Concen: 1.966 ug/l

RT: 2.69 min Scan# 497

Delta R.T. 0.01 min

Lab File: VU034142.D

Acq: 31 Aug 2019 23:50

Tgt Ion: 84 Resp: 10902


Ion Ratio Lower Upper

84 100

49 123.9 100.2 150.4

51 37.3 30.8 46.2

86 58.4 52.5 78.7

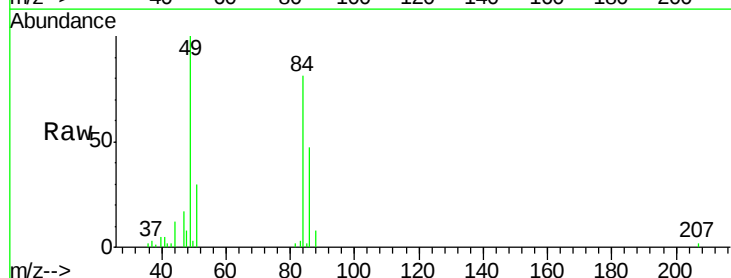

Abundance Ion 83.90 (83.60 to 84.60): VU034142.D (-402) (-)

Ion 48.90 (48.60 to 49.60): VU034142.D (-402) (-)

Ion 50.90 (50.60 to 51.60): VU034142.D (-402) (-)

Ion 85.90 (85.60 to 86.60): VU034142.D (-402) (-)

2.69

12000

10000

8000

6000


4000


2000

0

2.65 2.70 2.75

Time-->




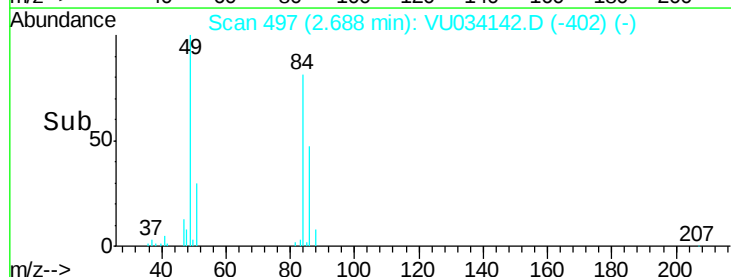


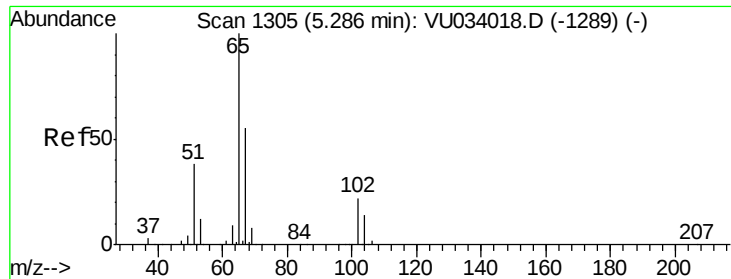

#33
 1,2-Dichloroethane-d4
 Concen: 49.557 ug/l
 RT: 5.29 min Scan# 1306
 Delta R.T. 0.00 min
 Lab File: VU034142.D
 Acq: 31 Aug 2019 23:50




Instrument :
 MSVOA_U
 ClientSampleId :
 T9-12-13-D-(0)


Tot Ion: 65 Resp: 284495
 Ion Ratio Lower Upper
 65 100
 67 54.1 0.0 110.6

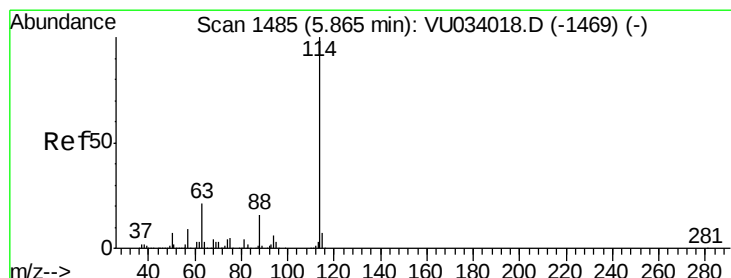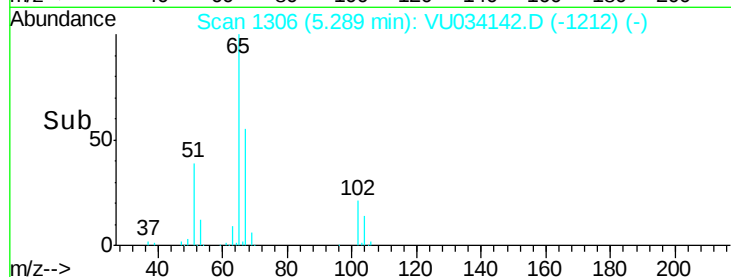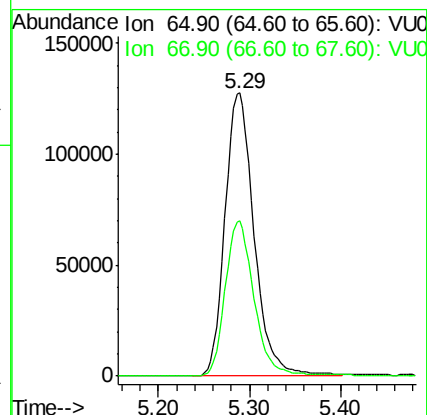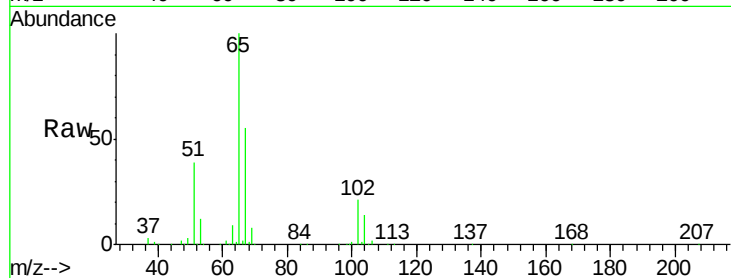

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 5.87 min Scan# 1486
 Delta R.T. 0.00 min
 Lab File: VU034142.D
 Acq: 31 Aug 2019 23:50

Tgt Ion: 114 Resp: 716972
 Ion Ratio Lower Upper
 114 100
 63 20.9 0.0 42.0
 88 16.2 0.0 32.0


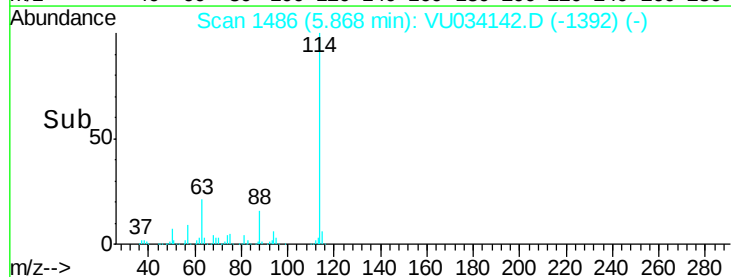
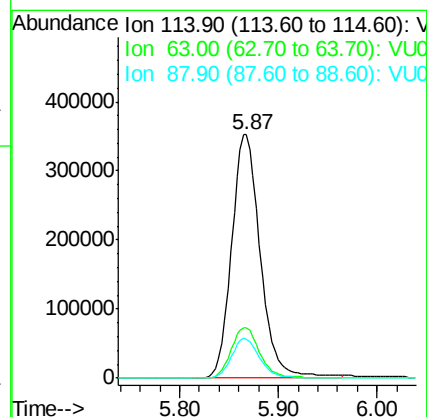
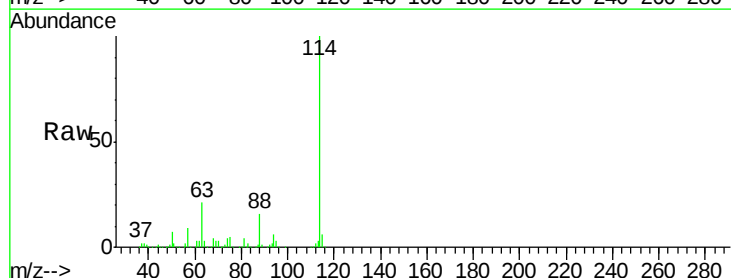


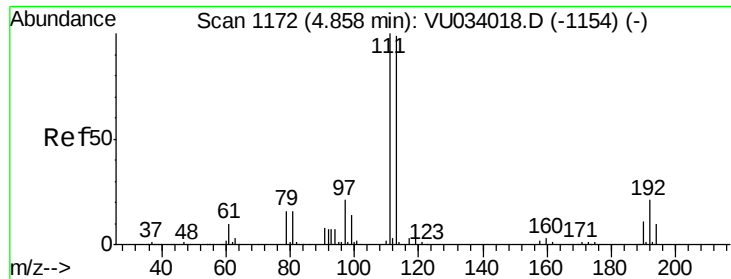

#35
 Dibromofluoromethane
 Concen: 47.282 ug/l
 RT: 4.86 min Scan# 1173
 Delta R.T. 0.00 min
 Lab File: VU034142.D
 Acq: 31 Aug 2019 23:50




Instrument :
 MSVOA_U
 ClientSampleId :
 T9-12-13-D-(0)


Tot Ion	Ratio	Lower	Upper
113	100		
111	104.1	81.7	122.5
192	21.2	17.1	25.7

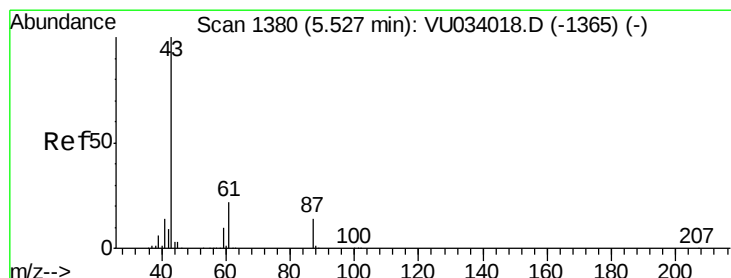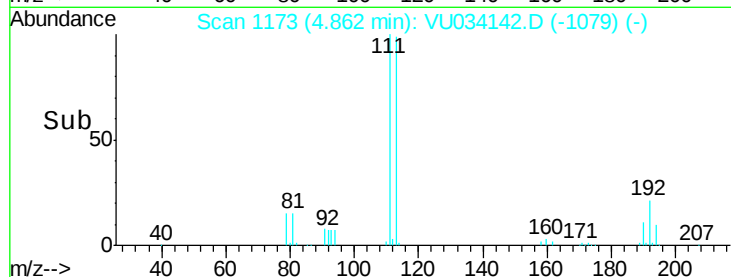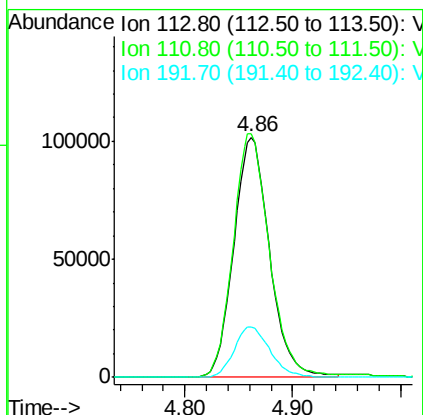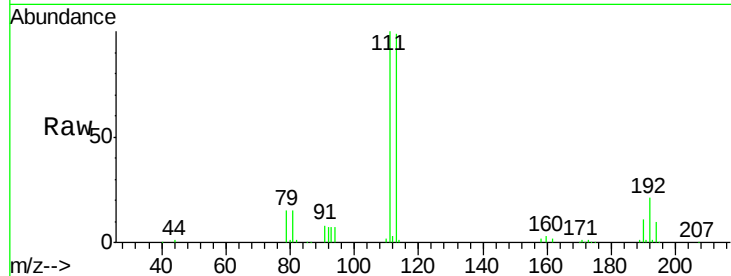

#43
 Isopropyl Acetate
 Concen: 6.353 ug/l
 RT: 5.53 min Scan# 1382
 Delta R.T. 0.01 min
 Lab File: VU034142.D
 Acq: 31 Aug 2019 23:50

Tgt Ion	Ratio	Lower	Upper
43	100		
61	20.8	17.2	25.8
87	13.3	10.8	16.2

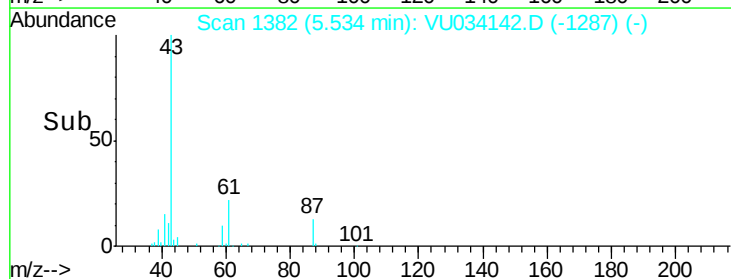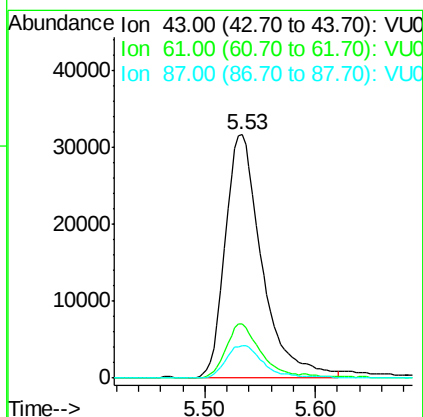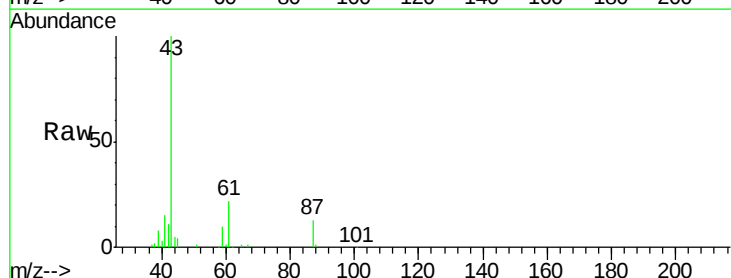

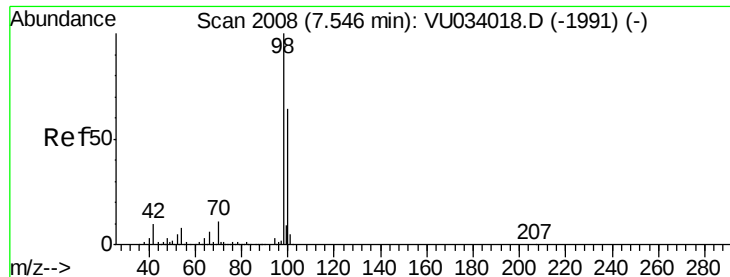

#50

Toluene-d8

Concen: 50.050 ug/l

RT: 7.55 min Scan# 2008

Delta R.T. -0.00 min

Lab File: VU034142.D

Acq: 31 Aug 2019 23:50

Instrument :

MSVOA_U

ClientSampleId :





T9-12-13-D-(0)

Tot Ion: 98 Resp: 931939

Ion Ratio Lower Upper

98 100

100 63.8 50.3 75.5

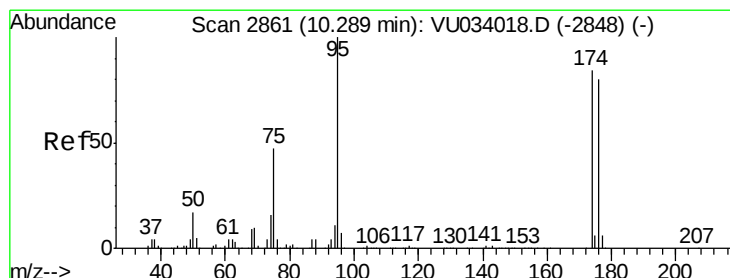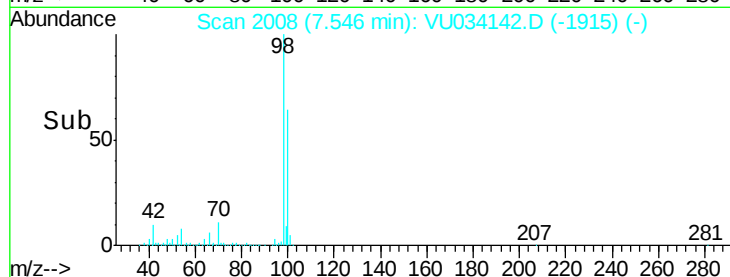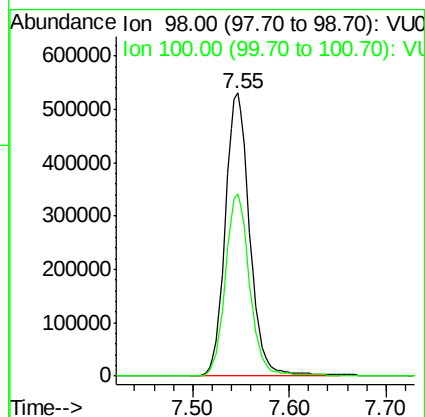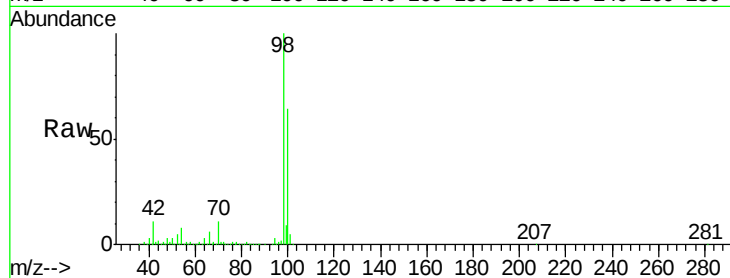

#62

4-Bromofluorobenzene

Concen: 45.005 ug/l

RT: 10.29 min Scan# 2861

Delta R.T. -0.00 min

Lab File: VU034142.D

Acq: 31 Aug 2019 23:50




Tgt Ion: 95 Resp: 325977


Ion Ratio Lower Upper

95 100

174 84.6 0.0 168.8

176 81.5 0.0 161.8

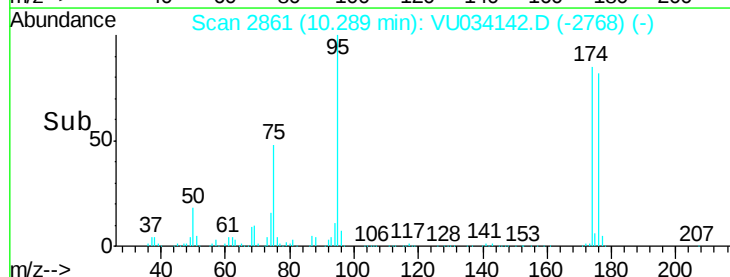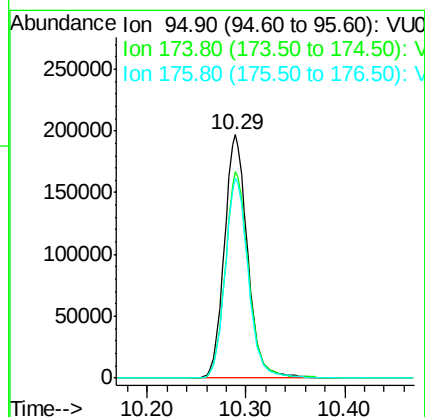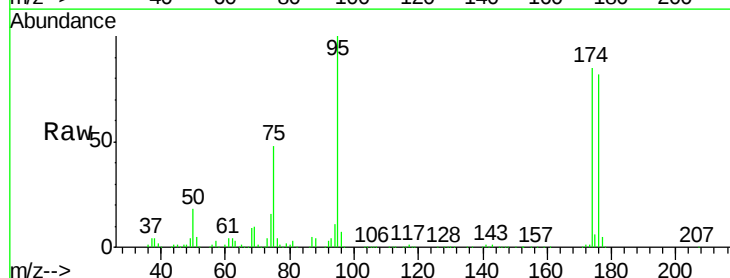


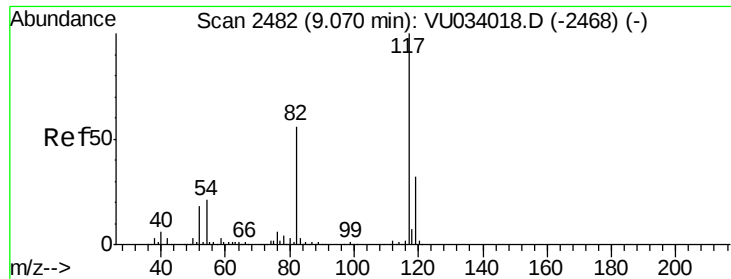




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.07 min Scan# 2482
Delta R.T. -0.00 min
Lab File: VU034142.D
Acq: 31 Aug 2019 23:50

Instrument :
MSVOA_U
ClientSampleId :
T9-12-13-D-(0)

Tot Ion:117 Resp: 714428
Ion Ratio Lower Upper
117 100
82 56.5 45.1 67.7
119 32.2 25.4 38.0

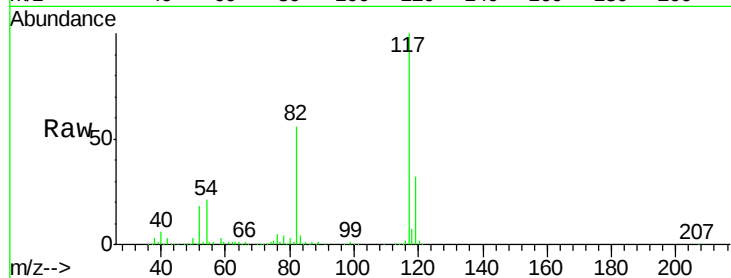


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VU0
Ion 118.90 (118.60 to 119.60): V

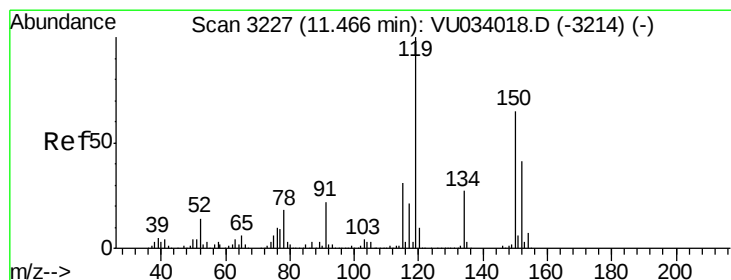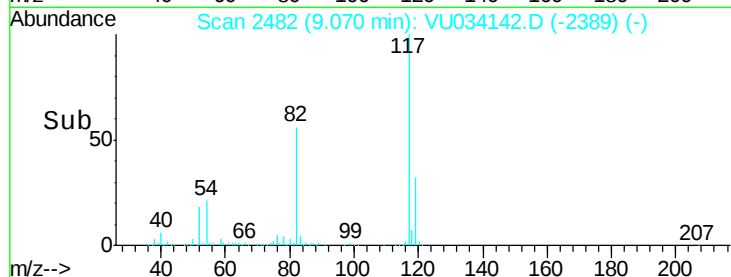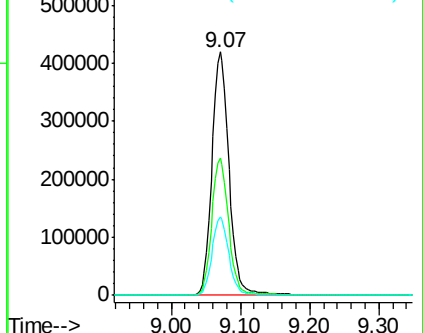

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.47 min Scan# 3227
Delta R.T. -0.00 min
Lab File: VU034142.D
Acq: 31 Aug 2019 23:50

Tgt Ion:152 Resp: 348709
Ion Ratio Lower Upper
152 100
115 56.3 41.1 123.3
150 156.4 0.0 348.8

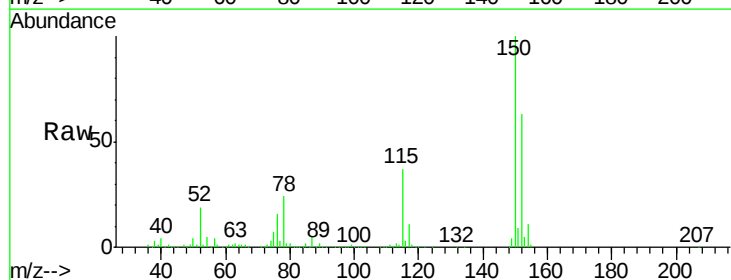

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

