

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090219\
 Data File : VU034156.D
 Acq On : 01 Sep 2019 05:15
 Operator : JC/SP
 Sample : K4526-40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 T9-12-13-L-(0)

Quant Time: Sep 01 06:09:39 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 29 04:11:12 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.96	168	432701	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.87	114	703162	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.07	117	707028	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.46	152	349978	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.29	65	276587	49.89	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.78%	
35) Dibromofluoromethane	4.86	113	230401	47.24	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.48%	
50) Toluene-d8	7.55	98	913642	50.03	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.06%	
62) 4-Bromofluorobenzene	10.29	95	324443	45.67	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.34%	
Target Compounds						
16) Acetone	2.31	43	17276	6.107	ug/l	96
20) Methylene Chloride	2.69	84	15549	2.903	ug/l	97
43) Isopropyl Acetate	5.53	43	49149	4.338	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU090219\
Data File : VU034156.D
Acq On : 01 Sep 2019 05:15
Operator : JC/SP
Sample : K4526-40
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
T9-12-13-L-(0)

Quant Time: Sep 01 06:09:39 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 29 04:11:12 2019
Response via : Initial Calibration

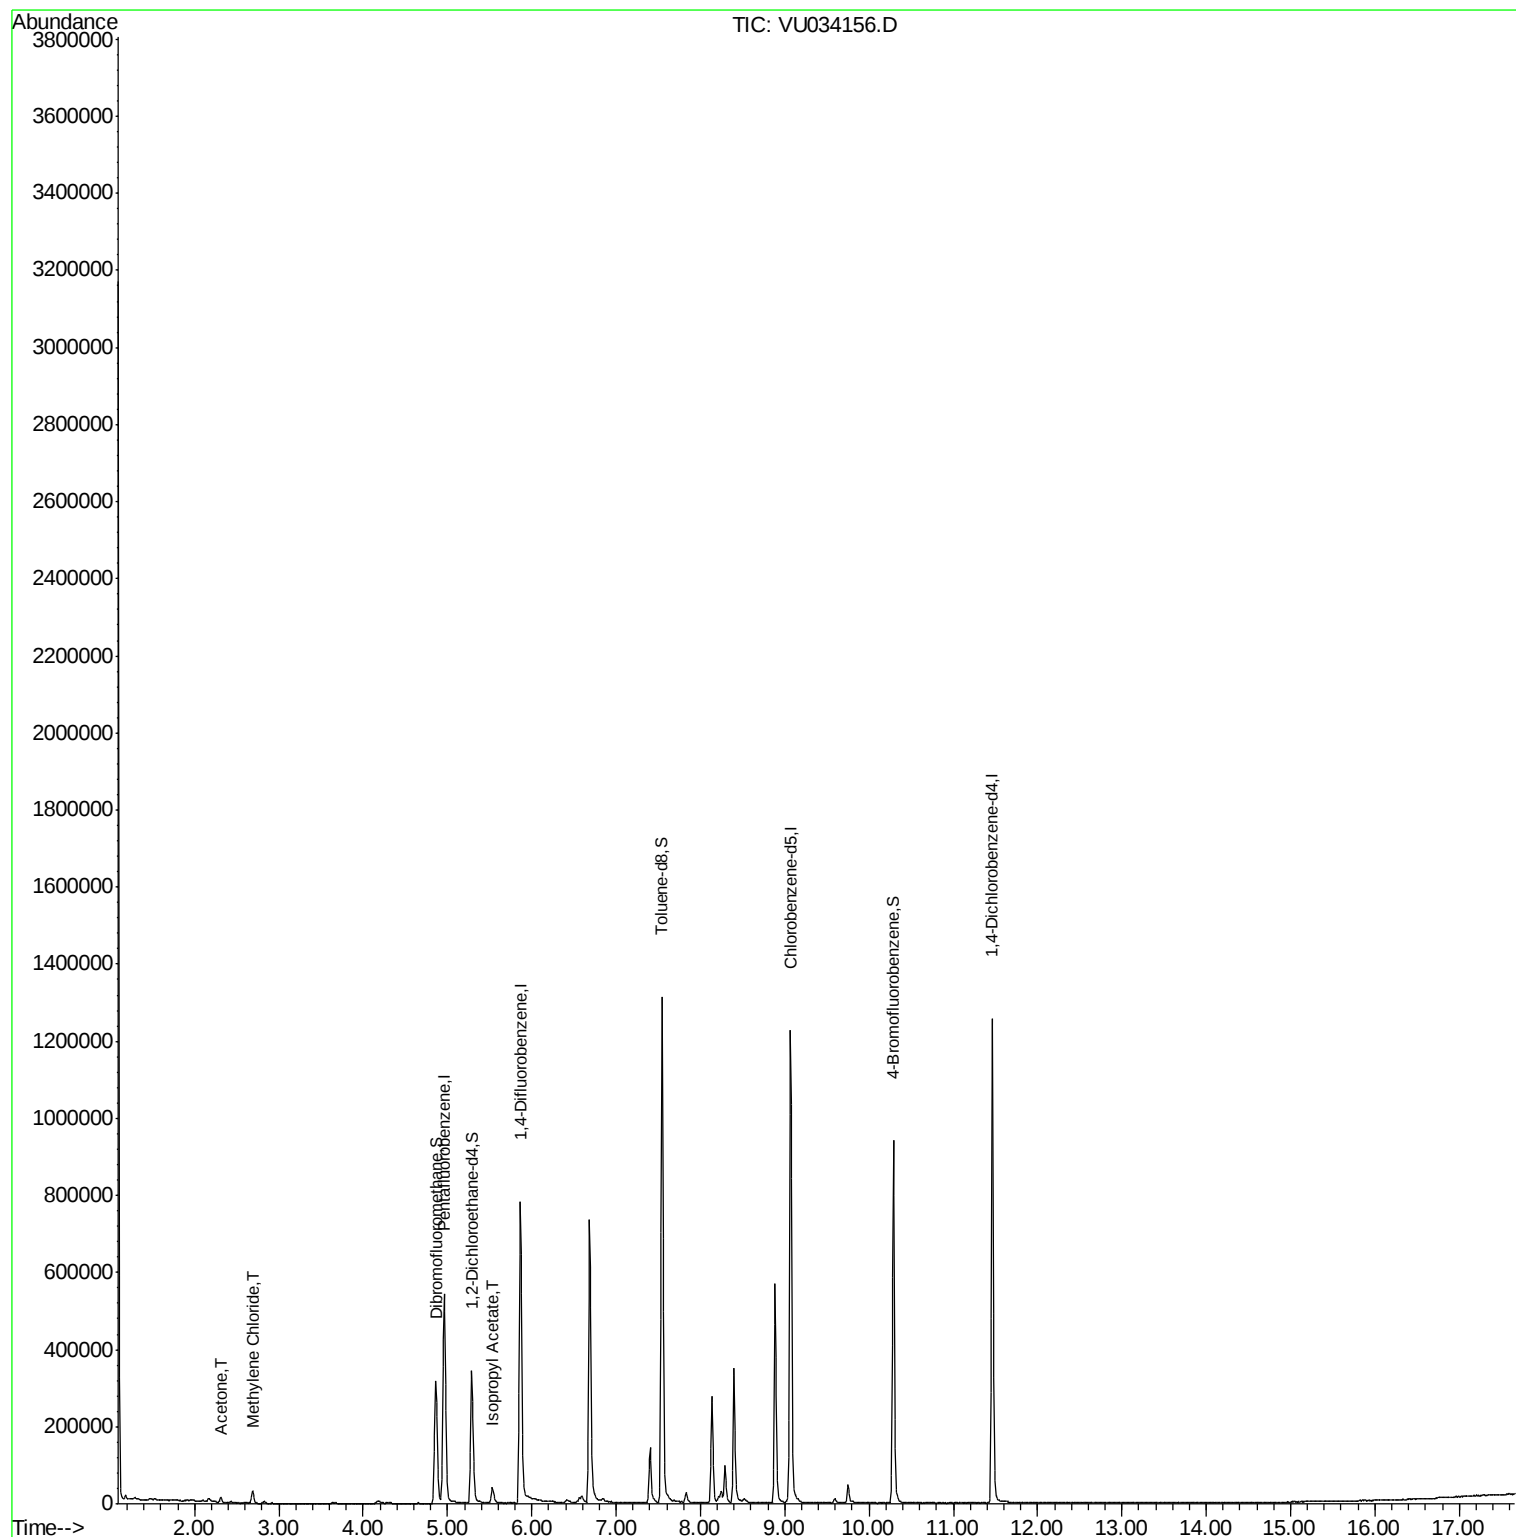

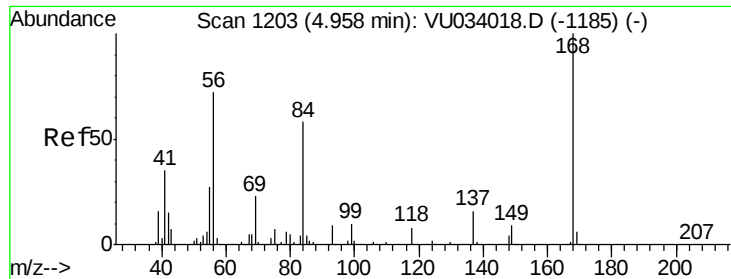

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.96 min Scan# 1204

Delta R.T. 0.00 min

Lab File: VU034156.D

Acq: 01 Sep 2019 05:15

Instrument :

MSVOA_U

ClientSampleId :


T9-12-13-L-(0)

Tot Ion:168 Resp: 432701

Ion Ratio Lower Upper

168 100

99 54.2 42.3 63.5

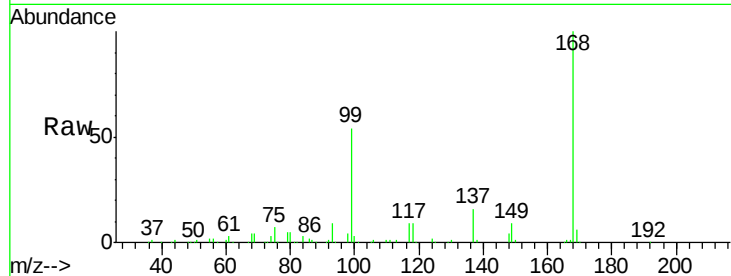

Abundance Ion 167.90 (167.60 to 168.60): VU034156.D (-1110) (-)

Ion 98.90 (98.60 to 99.60): VU034156.D (-1110) (-)

4.96

200000

150000



100000

50000

0

4.90 5.00 5.10

Time-->

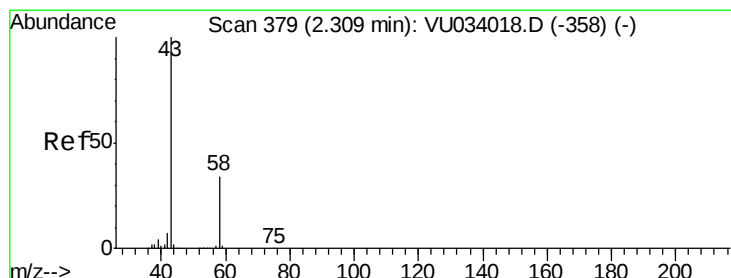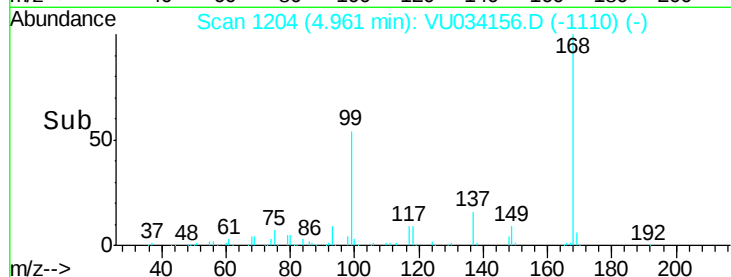

#16

Acetone

Concen: 6.107 ug/l

RT: 2.31 min Scan# 380

Delta R.T. 0.00 min

Lab File: VU034156.D


Acq: 01 Sep 2019 05:15

Tgt Ion: 43 Resp: 17276

Ion Ratio Lower Upper

43 100

58 31.5 26.8 40.2

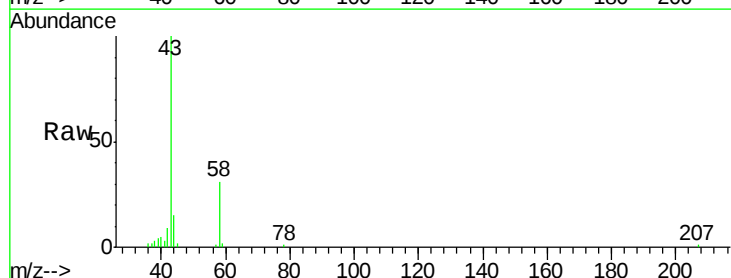

Abundance Ion 43.00 (42.70 to 43.70): VU034156.D (-286) (-)

Ion 58.00 (57.70 to 58.70): VU034156.D (-286) (-)

2.31

12000

10000

8000

6000


4000


2000

0

2.25 2.30 2.35 2.40

Time-->




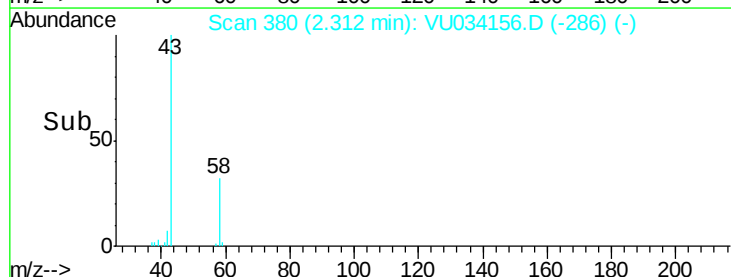


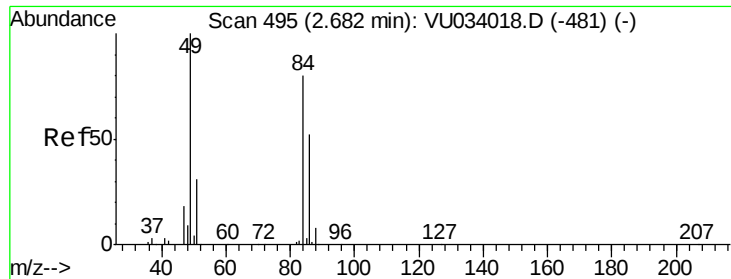

#20
Methvlene Chloride
Concen: 2.903 ug/l
RT: 2.69 min Scan# 497
Delta R.T. 0.01 min
Lab File: VU034156.D
Acq: 01 Sep 2019 05:15




Instrument :
MSVOA_U
ClientSampleId :
T9-12-13-L-(0)


Tot Ion:	84	Resp:	15549
Ion	Ratio	Lower	Upper
84	100		
49	125.5	100.2	150.4
51	36.3	30.8	46.2
86	59.8	52.5	78.7

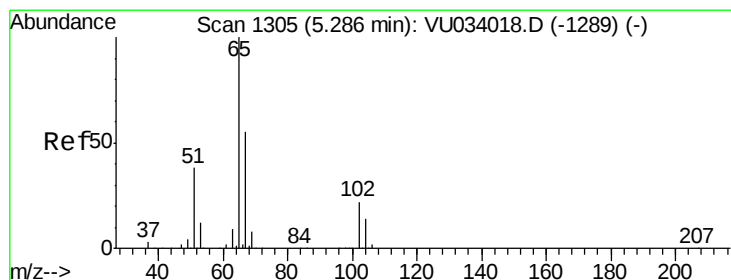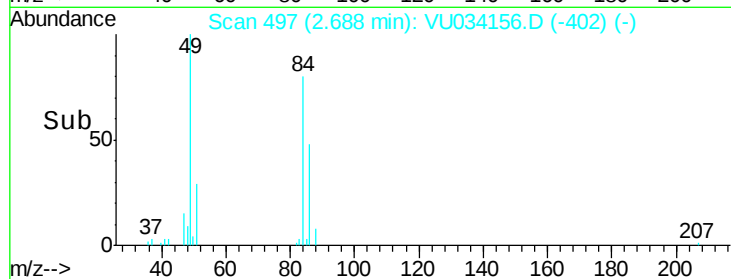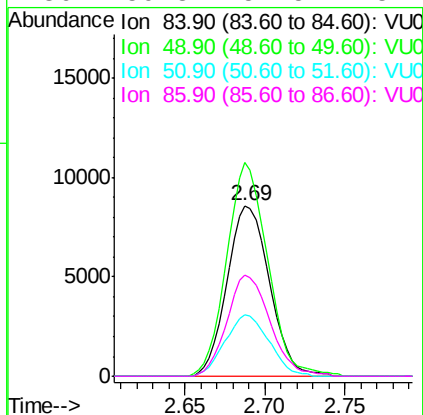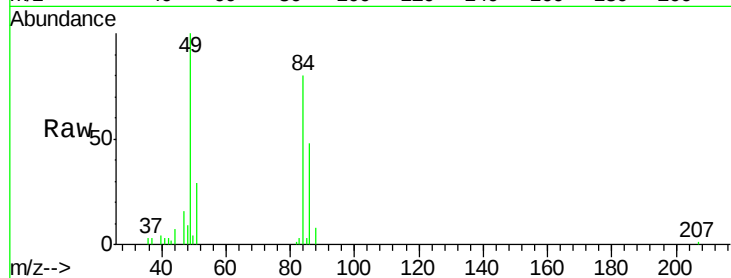

#33
1,2-Dichloroethane-d4
Concen: 49.886 ug/l
RT: 5.29 min Scan# 1306
Delta R.T. 0.00 min
Lab File: VU034156.D
Acq: 01 Sep 2019 05:15

Tgt Ion:	65	Resp:	276587
Ion	Ratio	Lower	Upper
65	100		
67	55.0	0.0	110.6


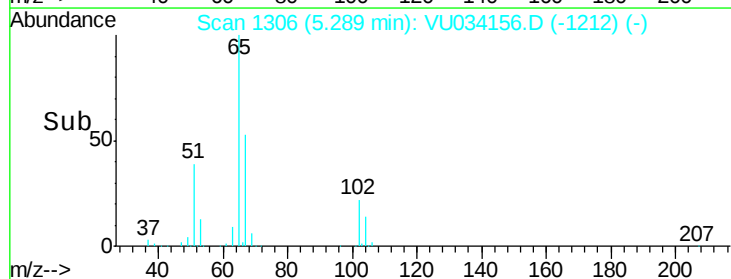
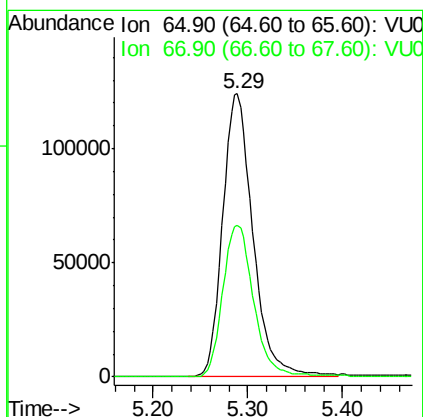
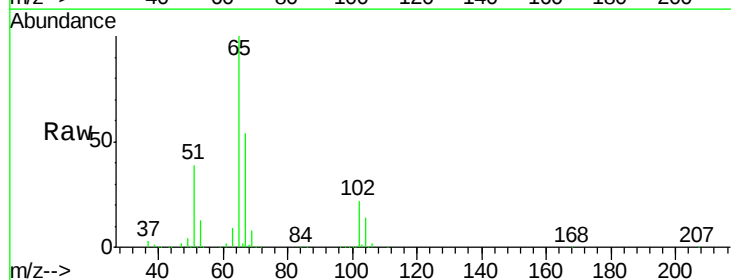


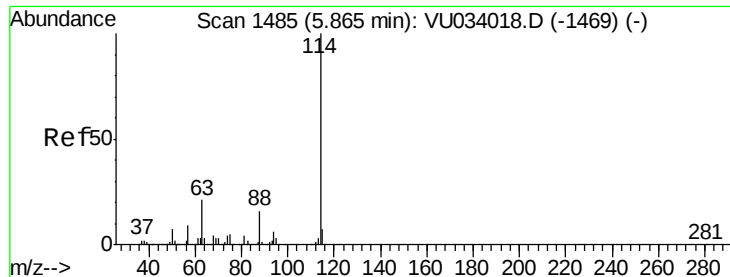

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 5.87 min Scan# 1486
 Delta R.T. 0.00 min
 Lab File: VU034156.D
 Acq: 01 Sep 2019 05:15




Instrument :
 MSVOA_U
 ClientSampleId :
 T9-12-13-L-(0)


Tot Ion:114 Resp: 703162
 Ion Ratio Lower Upper
 114 100
 63 20.9 0.0 42.0
 88 15.8 0.0 32.0

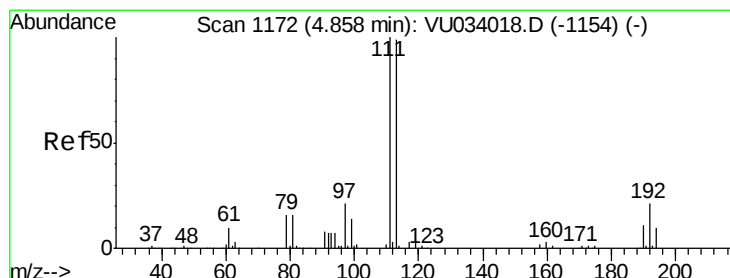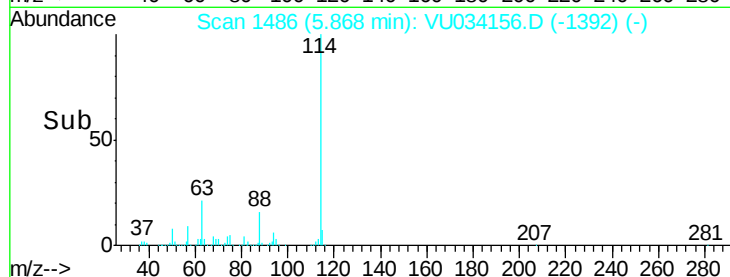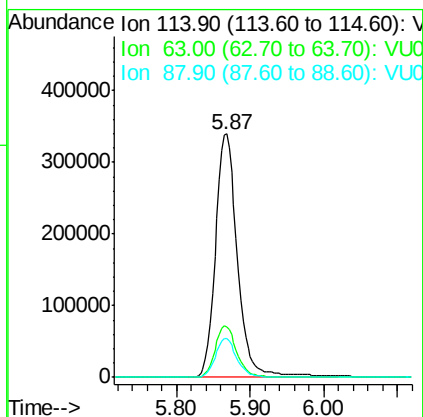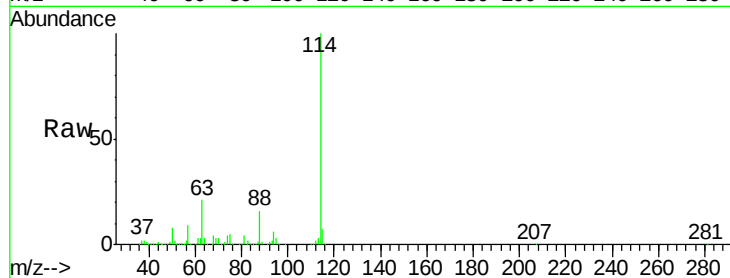

#35
 Dibromofluoromethane
 Concen: 47.242 ug/l
 RT: 4.86 min Scan# 1173
 Delta R.T. 0.00 min
 Lab File: VU034156.D
 Acq: 01 Sep 2019 05:15

Tgt Ion:113 Resp: 230401
 Ion Ratio Lower Upper
 113 100
 111 101.9 81.7 122.5
 192 21.4 17.1 25.7

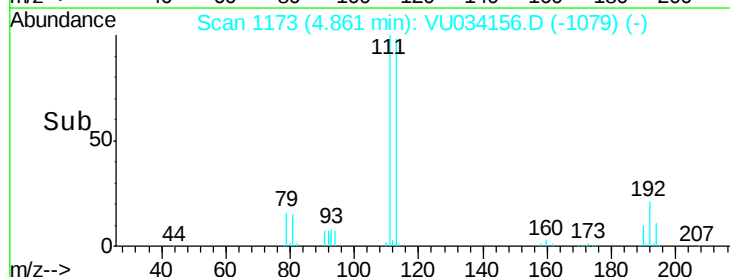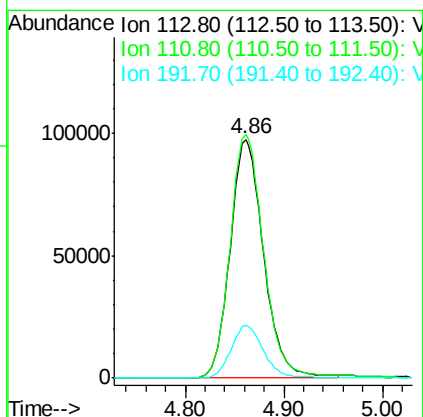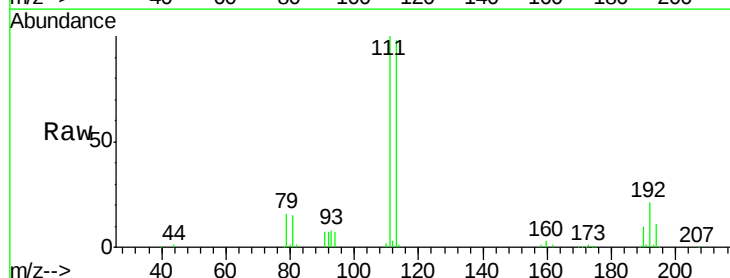

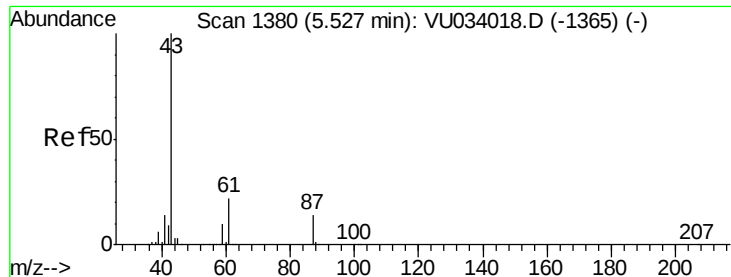

#43

Isopropyl Acetate

Concen: 4.338 ug/l

RT: 5.53 min Scan# 1382

Delta R.T. 0.01 min

Lab File: VU034156.D

Acq: 01 Sep 2019 05:15

Instrument :

MSVOA_U

ClientSampleId :

T9-12-13-L-(0)


Tot Ion: 43 Resp: 49149

Ion Ratio Lower Upper

43 100

61 22.0 17.2 25.8

87 13.5 10.8 16.2

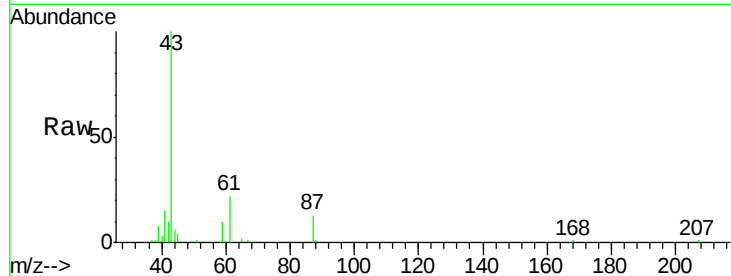


Abundance Ion 43.00 (42.70 to 43.70): VU034156.D (-1287) (-)

Ion 61.00 (60.70 to 61.70): VU034156.D (-1287) (-)

Ion 87.00 (86.70 to 87.70): VU034156.D (-1287) (-)

Time-->

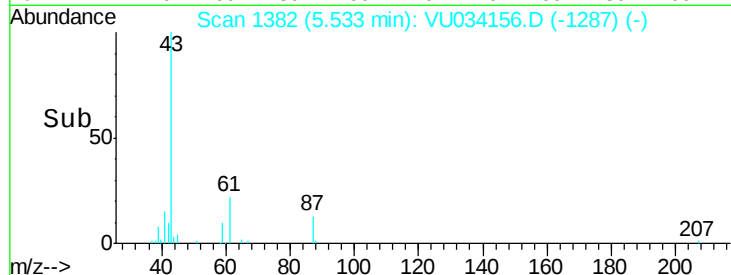


Abundance

Ion 43.00 (42.70 to 43.70): VU034156.D (-1287) (-)

Ion 61.00 (60.70 to 61.70): VU034156.D (-1287) (-)

Ion 87.00 (86.70 to 87.70): VU034156.D (-1287) (-)

Time-->

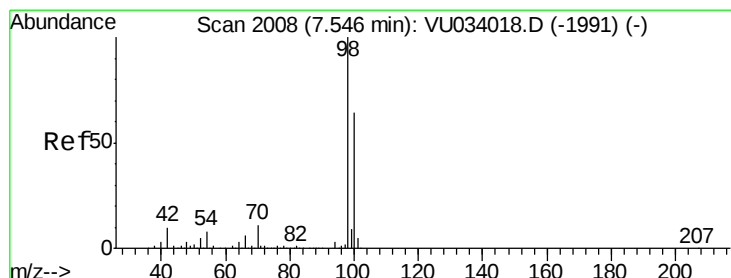

#50

Toluene-d8

Concen: 50.031 ug/l

RT: 7.55 min Scan# 2008

Delta R.T. -0.00 min

Lab File: VU034156.D


Acq: 01 Sep 2019 05:15

Tgt Ion: 98 Resp: 913642

Ion Ratio Lower Upper

98 100


100 64.5 50.3 75.5

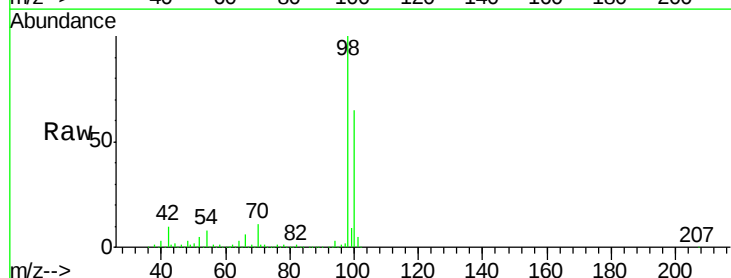

Abundance Ion 98.00 (97.70 to 98.70): VU034156.D (-1915) (-)

Ion 100.00 (99.70 to 100.70): VU034156.D (-1915) (-)

Time-->

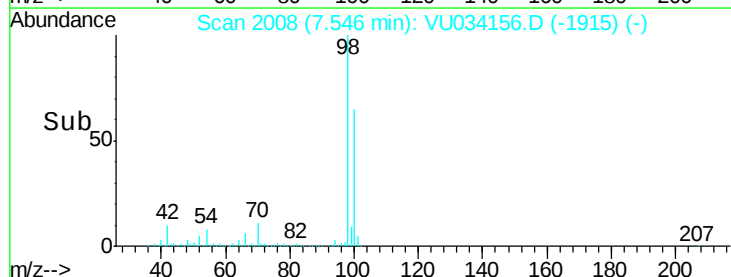


Abundance

Ion 98.00 (97.70 to 98.70): VU034156.D (-1915) (-)

Ion 100.00 (99.70 to 100.70): VU034156.D (-1915) (-)

Time-->

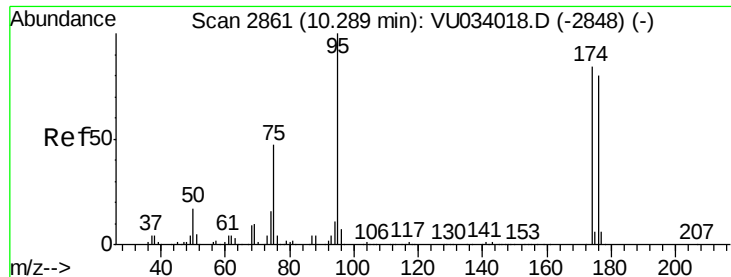

#62

4-Bromofluorobenzene

Concen: 45.673 ug/l

RT: 10.29 min Scan# 2861

Delta R.T. -0.00 min

Lab File: VU034156.D

Acq: 01 Sep 2019 05:15

Instrument :

MSVOA_U

ClientSampleId :

T9-12-13-L-(0)


Tot Ion: 95 Resp: 324443

Ion Ratio Lower Upper

95 100

174 84.8 0.0 168.8




176 80.9 0.0 161.8

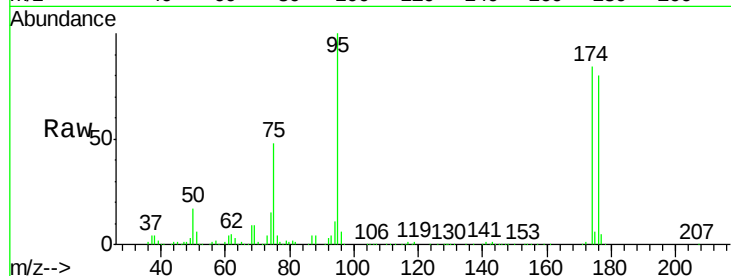

Abundance Ion 94.90 (94.60 to 95.60): VU034018.D (-2848) (-)

Ion 173.80 (173.50 to 174.50): VU034018.D (-2848) (-)

Ion 175.80 (175.50 to 176.50): VU034018.D (-2848) (-)

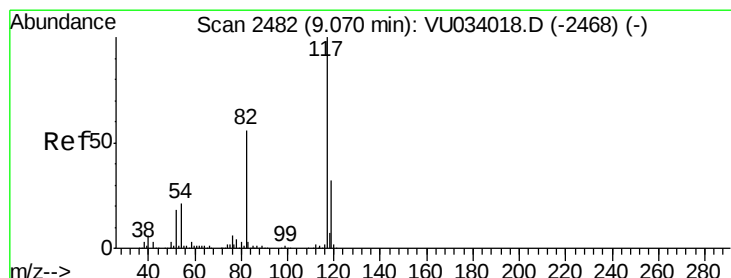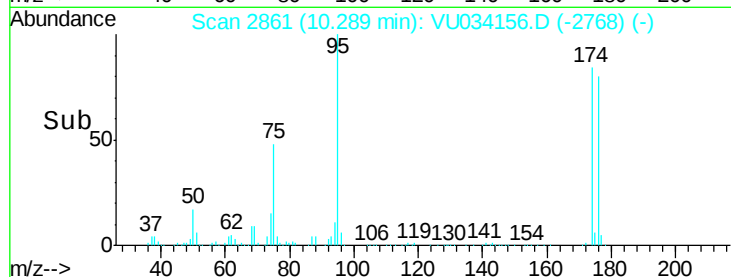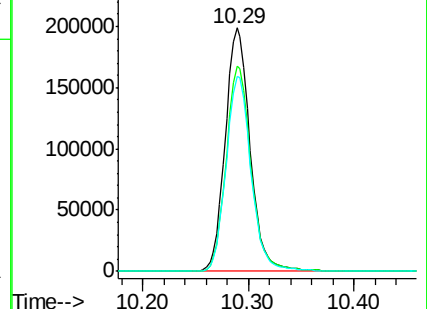

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 9.07 min Scan# 2482

Delta R.T. -0.00 min

Lab File: VU034156.D

Acq: 01 Sep 2019 05:15


Tgt Ion: 117 Resp: 707028

Ion Ratio Lower Upper

117 100

82 56.4 45.1 67.7



119 32.2 25.4 38.0

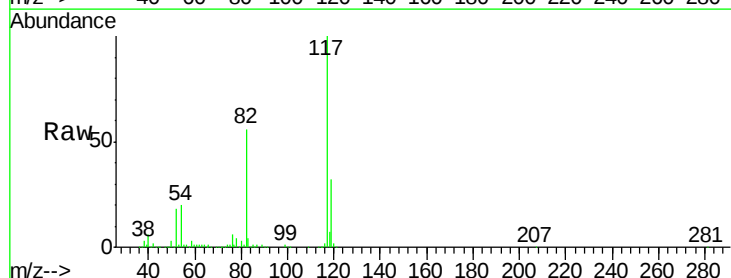


Abundance Ion 116.90 (116.60 to 117.60): VU034018.D (-2468) (-)

Ion 82.00 (81.70 to 82.70): VU034018.D (-2468) (-)

Ion 118.90 (118.60 to 119.60): VU034018.D (-2468) (-)

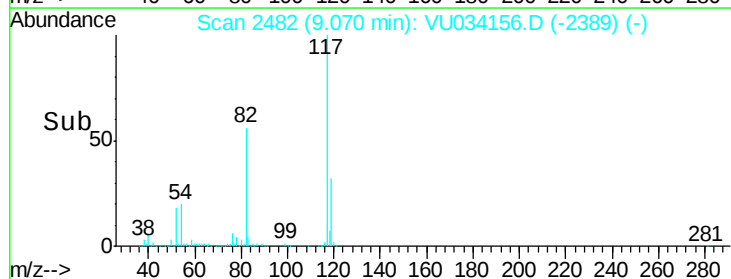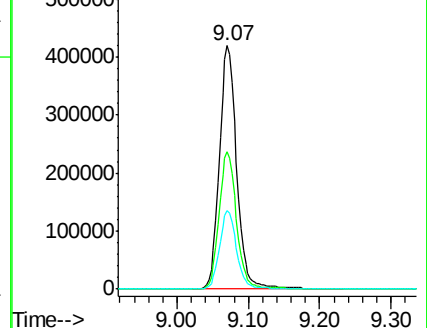

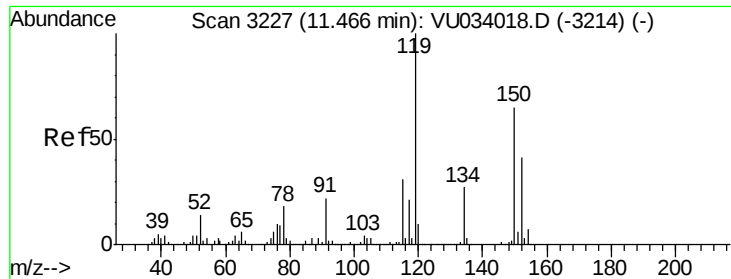

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 11.46 min Scan# 3226

Delta R.T. -0.00 min

Lab File: VU034156.D

Acq: 01 Sep 2019 05:15

Instrument :

MSVOA_U

ClientSampleId :

T9-12-13-L-(0)


Tot Ion:152 Resp: 349978

Ion Ratio Lower Upper

152 100

115 56.9 41.1 123.3

150 156.5 0.0 348.8

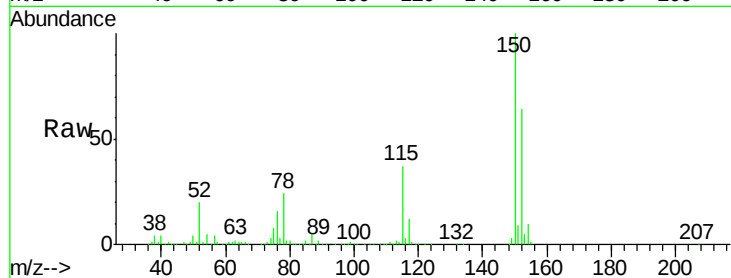

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

