


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU090219\
Data File : VU034158.D
Acq On : 01 Sep 2019 09:56
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
Title : SW846 8260
Last Update : Thu Aug 29 04:11:12 2019

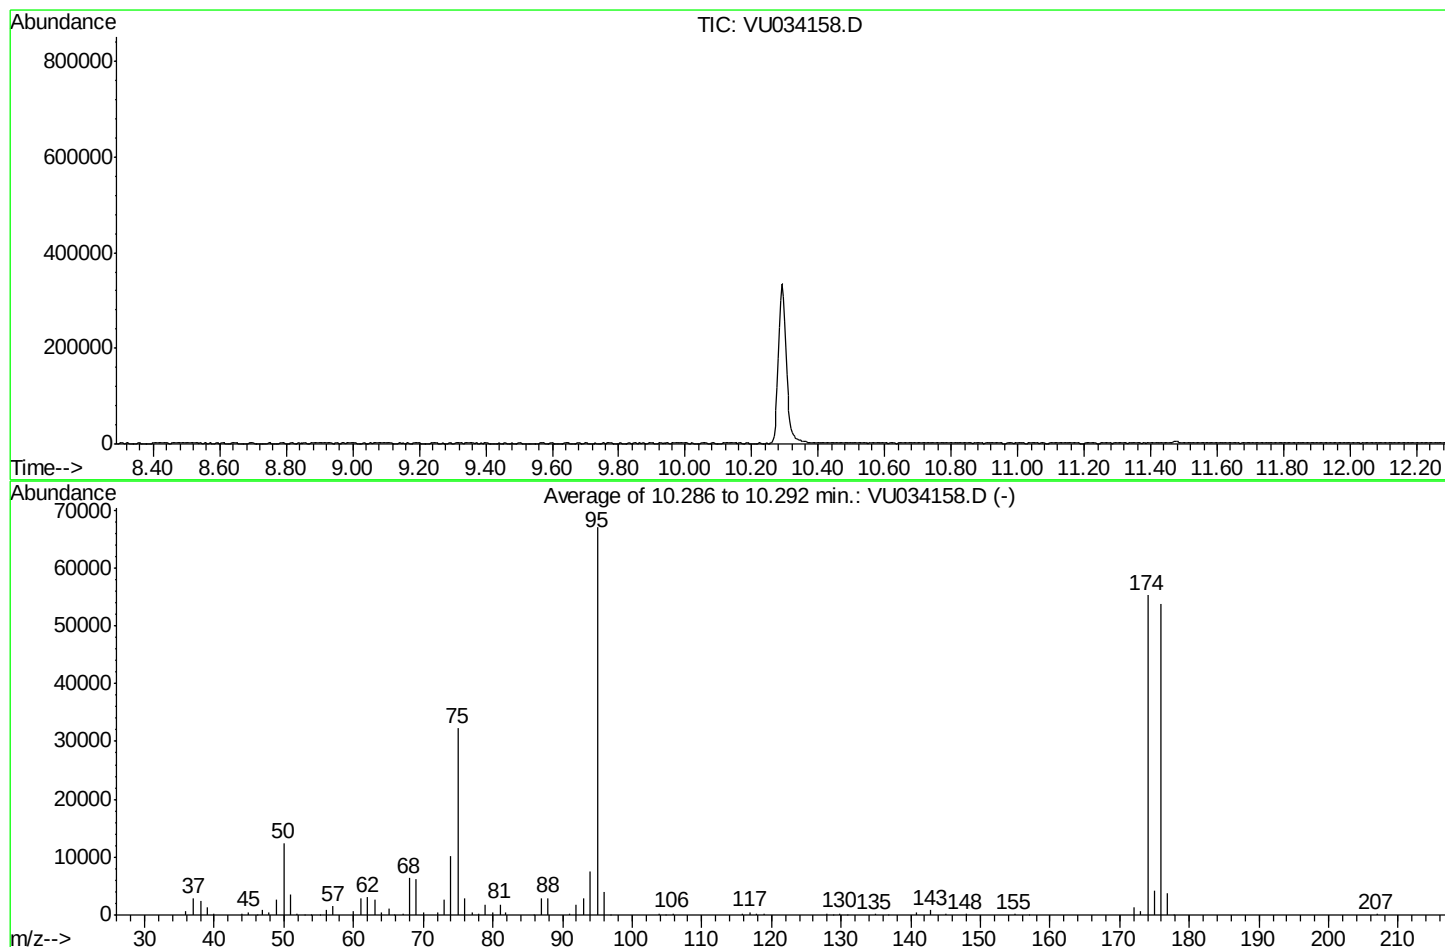

AutoFind: Scans 2860, 2861, 2862; Background Corrected with Scan 2848

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	12290	PASS
75	95	30	60	48.1	32256	PASS
95	95	100	100	100.0	67005	PASS
96	95	5	9	6.1	4092	PASS
173	174	0.00	2	1.2	645	PASS
174	95	50	100	82.4	55213	PASS
175	174	5	9	7.7	4268	PASS
176	174	95	101	97.3	53709	PASS
177	176	5	9	6.8	3671	PASS