


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090220\
 Data File : VU040013.D
 Acq On : 02 Sep 2020 08:58
 Operator : SY/MD
 Sample : BFB26
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB26

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Sep 09 07:43:27 2020

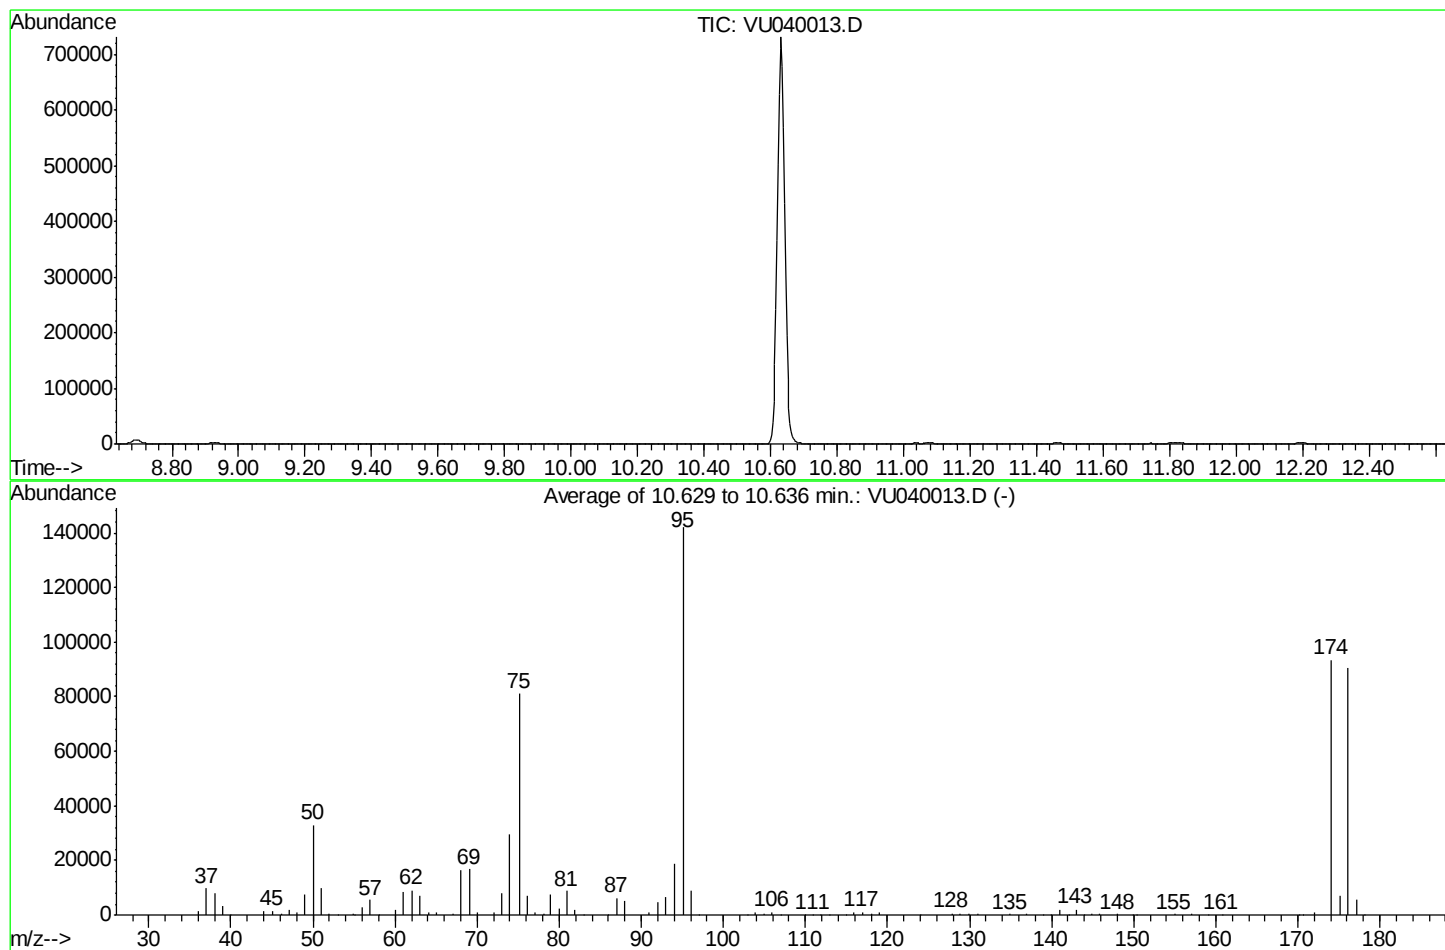

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	32912	PASS
75	95	30	80	57.1	81048	PASS
95	95	100	100	100.0	142037	PASS
96	95	5	9	6.4	9082	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	65.7	93370	PASS
175	174	5	9	7.6	7084	PASS
176	174	95	101	96.8	90362	PASS
177	176	5	9	6.4	5821	PASS

m/z	Abundance
44.00	349.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
36.10	1512.0
37.00	9954.0
38.00	8444.0
39.00	3200.0
40.00	156.0
44.00	1705.0
45.00	1517.0
46.10	341.0
47.10	1698.0
48.00	1082.0
49.00	7406.0
50.00	33576.0
51.10	10156.0
52.00	551.0
53.00	206.0
54.90	524.0
56.00	2877.0
57.00	5781.0
57.90	133.0
60.10	1846.0
61.10	8592.0
62.00	9159.0
63.00	7014.0
64.10	783.0
65.00	950.0
67.10	567.0
68.00	16568.0
69.00	17472.0
70.00	1210.0
72.00	959.0
73.00	8030.0
74.00	30144.0
75.10	81536.0
76.10	7271.0
77.00	1159.0
78.10	518.0
78.90	7586.0
80.00	2357.0
81.00	8896.0
82.00	1818.0
83.00	186.0
87.00	6683.0
88.00	5117.0
91.00	952.0
92.00	4687.0
93.00	6919.0
94.10	18560.0
95.10	142848.0
96.10	9218.0
97.00	321.0
103.00	105.0
103.90	842.0
104.90	342.0
106.00	1148.0
106.90	153.0
109.90	101.0
110.90	228.0
111.90	213.0
112.80	214.0
116.00	793.0
117.00	1251.0
118.00	541.0
119.00	1107.0
124.10	109.0
127.80	618.0
128.90	285.0
129.90	445.0
130.90	273.0
134.90	269.0
137.00	298.0
140.00	135.0
141.00	1888.0
142.10	232.0
143.00	1978.0
145.00	398.0
145.90	286.0
148.00	317.0
149.90	143.0
150.30	120.0
155.00	294.0
157.00	272.0
159.10	164.0
172.10	850.0
174.10	92712.0
175.10	7227.0
176.10	88400.0
177.10	5897.0
178.10	212.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
36.10	1539.0
37.00	10162.0
38.00	8344.0
39.00	3343.0
40.00	126.0
44.00	1785.0
45.00	1537.0
46.10	349.0
47.10	1807.0
48.00	1109.0
49.00	7656.0
50.00	33928.0
51.10	10143.0
52.00	525.0
53.00	153.0
54.90	448.0
56.00	2991.0
57.00	5598.0
57.90	124.0
60.10	1893.0
61.10	8686.0
62.00	9514.0
63.00	7219.0
64.10	878.0
65.00	852.0
67.00	564.0
68.00	16808.0
69.00	17464.0
70.00	1225.0
72.00	992.0
73.00	8167.0
74.00	30472.0
75.10	83768.0
76.10	7283.0
77.00	1131.0
78.10	464.0
78.90	7748.0
80.00	2356.0
80.90	9052.0
82.00	1806.0
83.00	177.0
86.00	103.0
87.00	6549.0
88.00	5300.0
91.00	864.0
92.00	4819.0
93.00	6654.0
94.10	19336.0
95.10	147136.0
96.10	9474.0
97.00	269.0
103.00	102.0
103.90	932.0
104.90	336.0
105.90	1048.0
106.90	179.0
110.00	152.0
110.90	260.0
111.90	211.0
112.80	182.0
114.90	108.0
115.90	784.0
116.90	1188.0
118.00	560.0
119.00	1105.0
124.00	148.0
127.80	619.0
128.90	330.0
130.00	466.0
130.90	279.0
134.90	306.0
136.90	296.0
139.90	122.0
141.00	1757.0
142.10	258.0
143.00	2153.0
144.90	303.0
145.90	316.0
148.00	294.0
149.90	199.0
155.00	348.0
157.00	288.0
159.00	236.0
160.80	101.0
170.20	117.0
172.10	817.0
174.10	96440.0
175.10	7290.0
176.10	93656.0
177.10	6035.0
178.10	215.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
36.00	1357.0
37.00	9084.0
38.00	7563.0
39.00	3304.0
40.00	141.0
44.00	1556.0
45.00	1482.0
46.10	283.0
47.10	1680.0
48.00	1096.0
49.00	7072.0
50.00	31232.0
51.00	9491.0
52.00	458.0
53.00	108.0
55.10	436.0
56.00	2742.0
57.00	4880.0
58.00	140.0
60.00	1762.0
61.00	8163.0
62.00	8483.0
63.00	6845.0
64.10	809.0
65.00	733.0
67.00	464.0
68.00	15613.0
69.10	15627.0
70.00	1105.0
72.00	843.0
73.00	7271.0
74.00	28136.0
75.10	77840.0
76.00	6547.0
77.00	922.0
78.90	7332.0
80.00	2128.0
80.90	8249.0
81.90	1624.0
83.00	166.0
85.90	175.0
87.00	5764.0
88.00	4742.0
90.90	703.0
92.00	4457.0
93.00	6044.0
94.10	18104.0
95.10	136128.0
96.10	8555.0
97.10	167.0
103.90	875.0
105.00	281.0
105.90	941.0
107.00	205.0
110.00	190.0
111.00	229.0
111.80	201.0
112.90	164.0
114.90	112.0
115.90	641.0
116.90	1099.0
118.00	518.0
119.00	943.0
124.00	207.0
127.90	485.0
128.80	295.0
130.00	505.0
131.00	264.0
135.00	341.0
136.90	239.0
139.00	101.0
141.00	1515.0
142.10	250.0
143.00	2043.0
144.00	100.0
144.90	240.0
145.90	264.0
148.10	275.0
149.90	167.0
155.00	343.0
157.00	261.0
159.00	274.0
170.10	162.0
170.60	145.0
172.10	826.0
174.10	90960.0
175.10	6736.0
176.10	89032.0
177.10	5531.0
178.10	179.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26