

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090221\
 Data File : VU044562.D
 Acq On : 02 Sep 2021 19:01
 Operator : SY/MD
 Sample : M3622-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY8

Quant Time: Sep 03 02:46:14 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 03 02:43:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	104948	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	108702	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.815	152	54294	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	40185	4.734	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.600%
7) Chloroethane-d5	1.919	69	39542	5.360	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.200%
11) 1,1-Dichloroethene-d2	2.575	65	16652	4.612	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	92.200%
20) 2-Butanone-d5	4.642	46	107709	45.884	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.760%
24) Chloroform-d	5.070	84	73243	4.880	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.600%
26) 1,2-Dichloroethane-d4	5.710	65	40138	4.904	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.000%
32) Benzene-d6	5.735	84	148687	4.857	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.200%
36) 1,2-Dichloropropane-d6	6.697	67	45638	4.661	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.200%
41) Toluene-d8	7.902	98	129423	4.768	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.400%
43) trans-1,3-Dichloroprop...	8.185	79	15494	4.406	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.200%
46) 2-Hexanone-d5	8.645	63	94600	49.744	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.480%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	40750	4.941	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.800%
66) 1,2-Dichlorobenzene-d4	12.198	152	50755	5.533	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.600%
Target Compounds						Qvalue
13) Acetone	2.655	43	4189	2.149	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090221\
Data File : VU044562.D
Acq On : 02 Sep 2021 19:01
Operator : SY/MD
Sample : M3622-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY8


Quant Time: Sep 03 02:46:14 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 03 02:43:14 2021
Response via : Initial Calibration

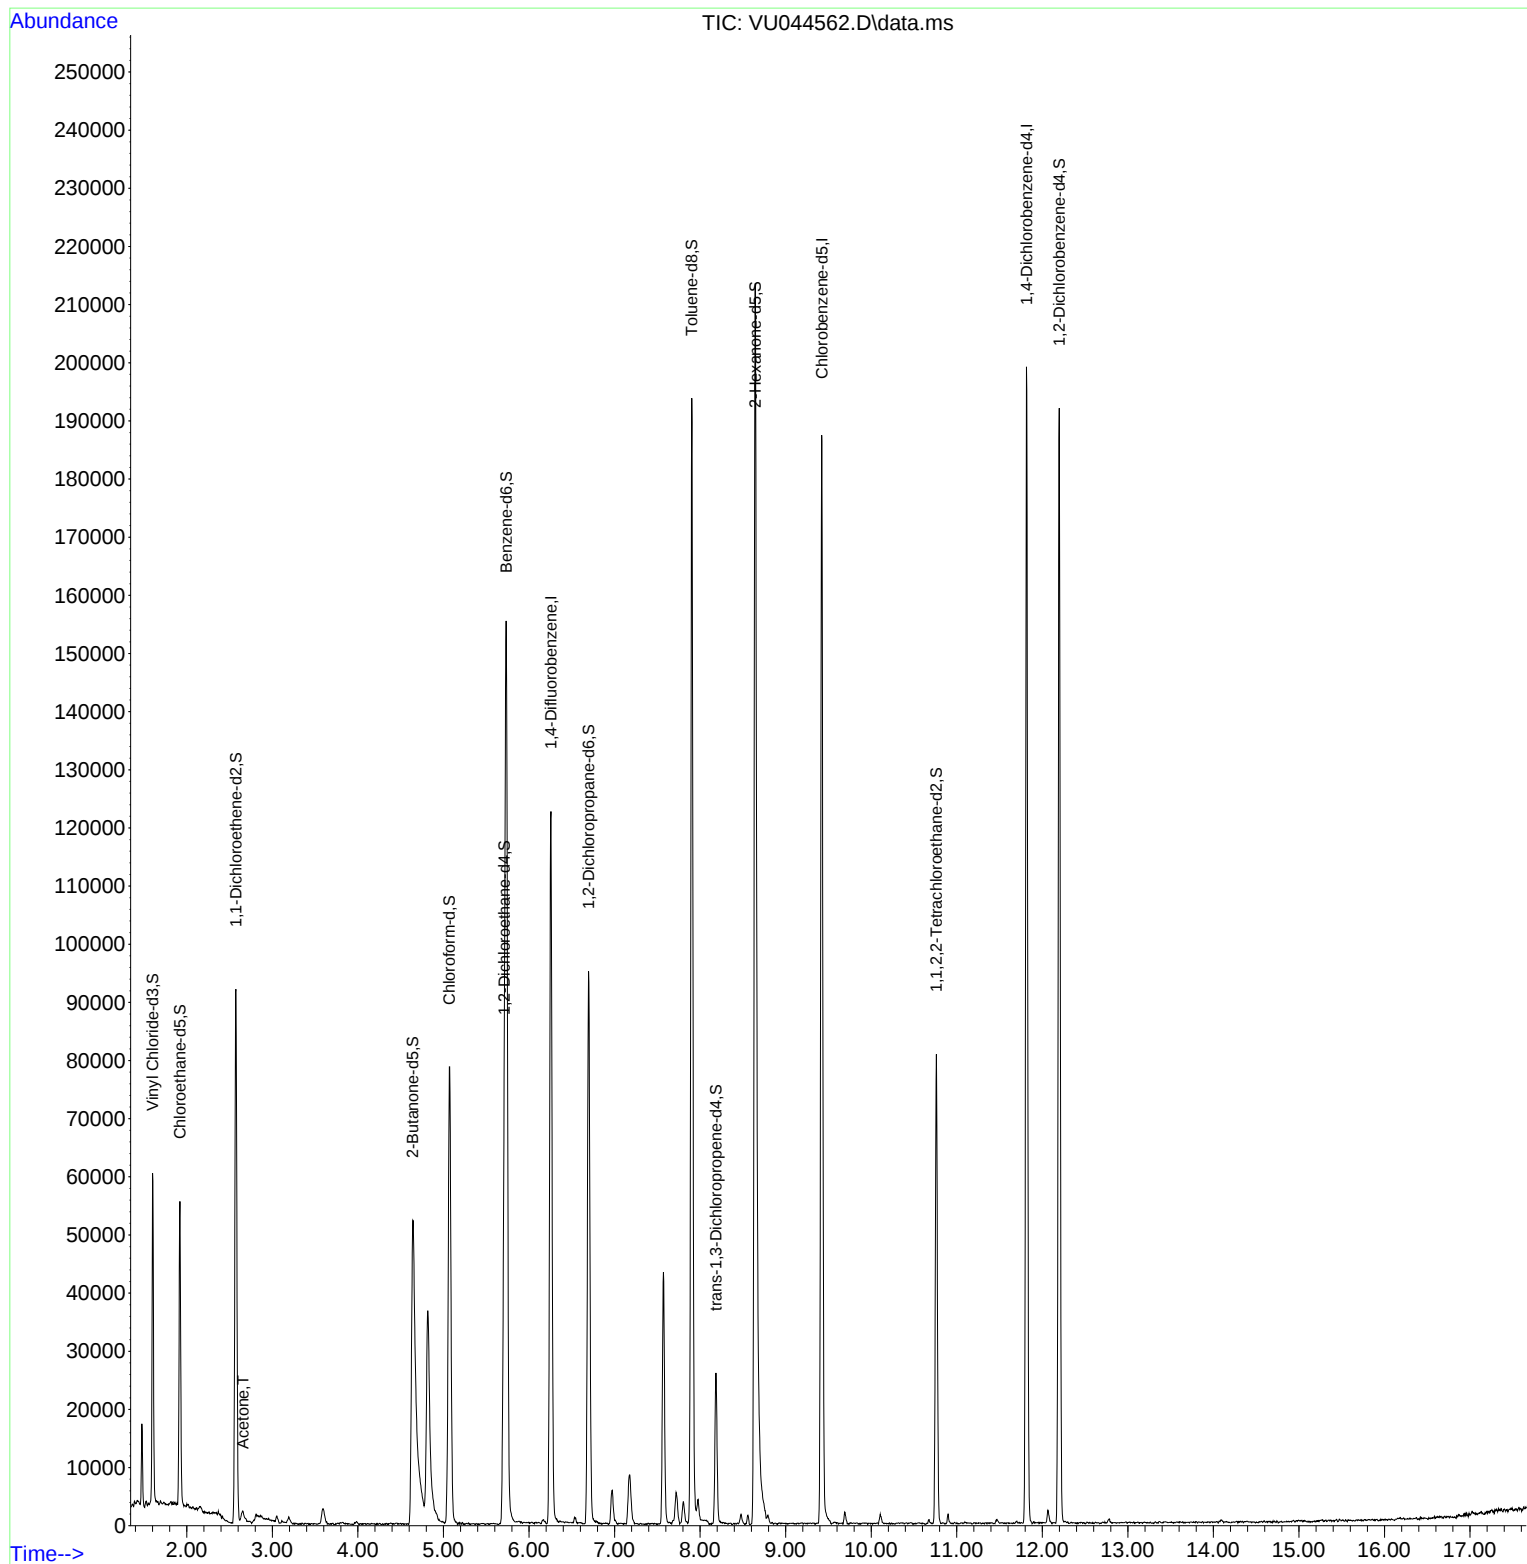

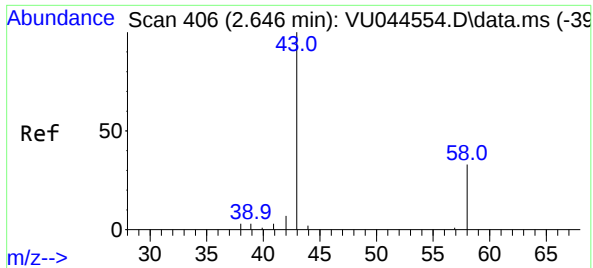

#13
 Acetone
 Concen: 2.149 ug/L
 RT: 2.655 min Scan# 409
 Delta R.T. 0.009 min
 Lab File: VU044562.D
 Acq: 02 Sep 2021 19:01

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY8

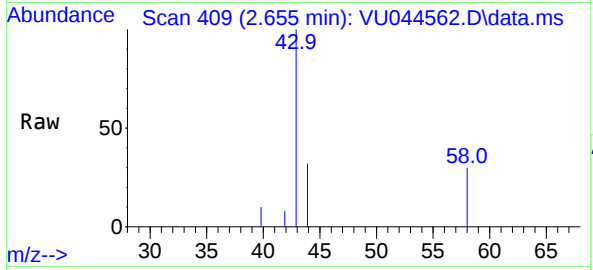

Tgt Ion: 43 Resp: 4189
 Ion Ratio Lower Upper
 43 100
 58 25.4 0.0 45.4

