

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090221\
 Data File : VU044563.D
 Acq On : 02 Sep 2021 19:25
 Operator : SY/MD
 Sample : M3596-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F3W01

Quant Time: Sep 03 02:46:25 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 03 02:43:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	102124	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	105651	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.815	152	52384	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	39567	4.790	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.800%
7) Chloroethane-d5	1.919	69	38383	5.347	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.000%
11) 1,1-Dichloroethene-d2	2.571	65	16469	4.687	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	93.800%
20) 2-Butanone-d5	4.642	46	105729	46.286	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.580%
24) Chloroform-d	5.070	84	70922	4.856	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.200%
26) 1,2-Dichloroethane-d4	5.710	65	40081	5.033	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.600%
32) Benzene-d6	5.735	84	149113	5.012	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.200%
36) 1,2-Dichloropropane-d6	6.697	67	45654	4.797	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.000%
41) Toluene-d8	7.902	98	128505	4.871	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.400%
43) trans-1,3-Dichloroprop...	8.185	79	15164	4.436	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.800%
46) 2-Hexanone-d5	8.645	63	95484	51.658	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.320%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	39807	4.966	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.400%
66) 1,2-Dichlorobenzene-d4	12.198	152	50618	5.719	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.400%
Target Compounds						
3) Chloromethane	1.523	50	1253	0.091	ug/L	96
25) Chloroform	5.095	83	5906	0.363	ug/L	99
34) Trichloroethene	6.546	95	7875	0.889	ug/L	97
47) Tetrachloroethene	8.558	164	110936	18.104	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090221\
Data File : VU044563.D
Acq On : 02 Sep 2021 19:25
Operator : SY/MD
Sample : M3596-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3W01

Quant Time: Sep 03 02:46:25 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 03 02:43:14 2021
Response via : Initial Calibration




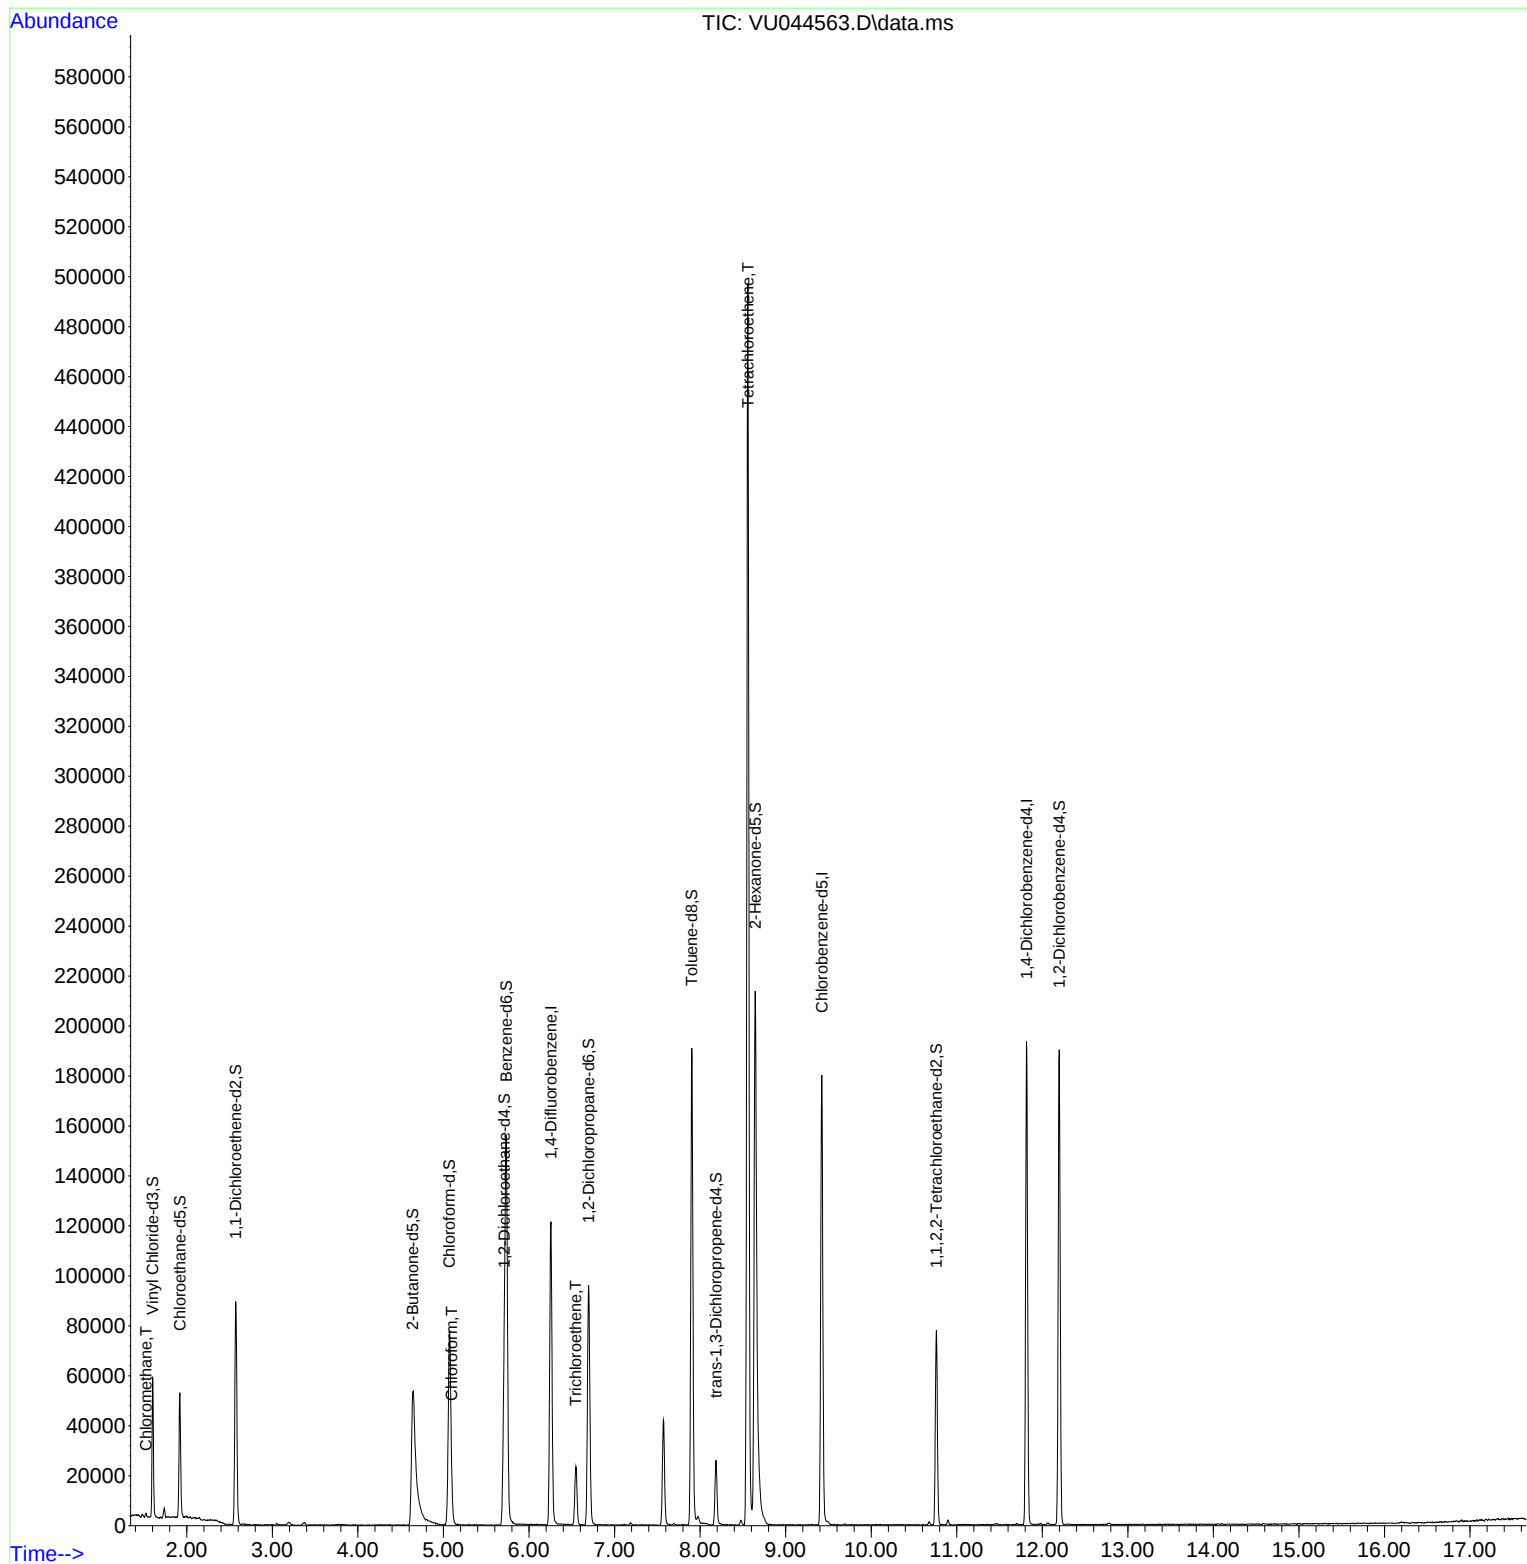


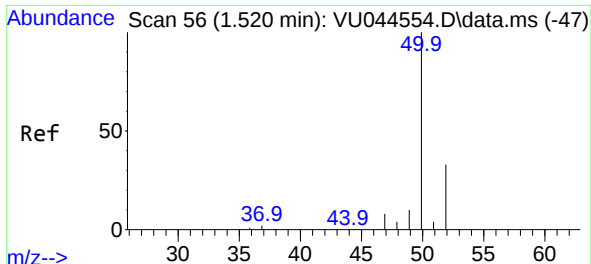

#3
Chloromethane
Concen: 0.091 ug/L
RT: 1.523 min Scan# 57
Delta R.T. 0.003 min
Lab File: VU044563.D
Acq: 02 Sep 2021 19:25




Instrument :
MSVOA_U
ClientSampled :
F3W01


Tgt Ion: 50 Resp: 1253
Ion Ratio Lower Upper
50 100
52 34.6 22.8 42.4

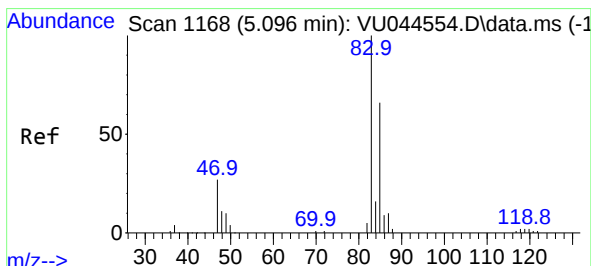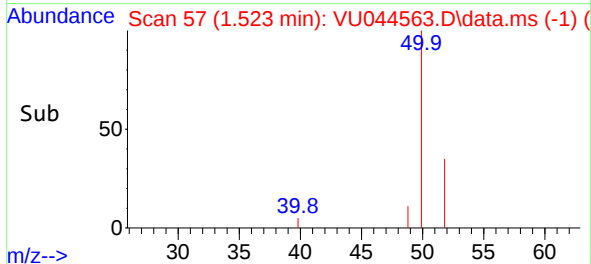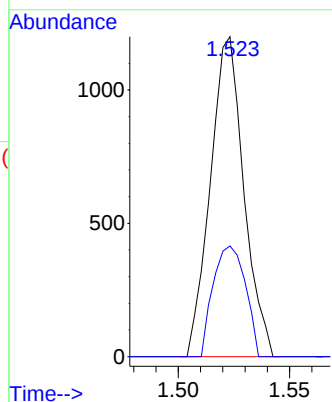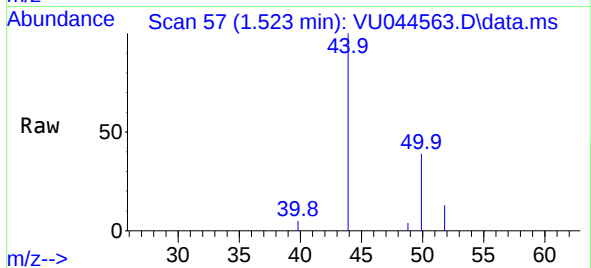

#25
Chloroform
Concen: 0.363 ug/L
RT: 5.095 min Scan# 1168
Delta R.T. -0.000 min
Lab File: VU044563.D
Acq: 02 Sep 2021 19:25

Tgt Ion: 83 Resp: 5906
Ion Ratio Lower Upper
83 100
85 65.8 45.3 84.1

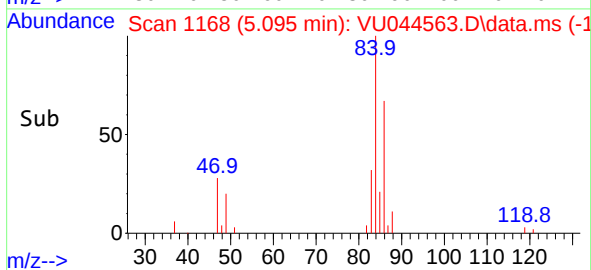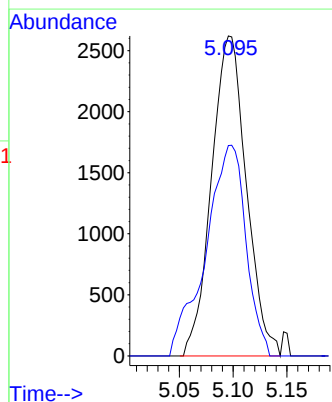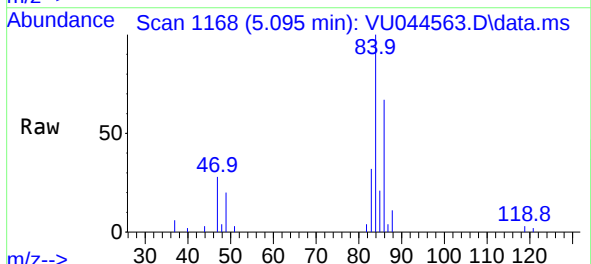




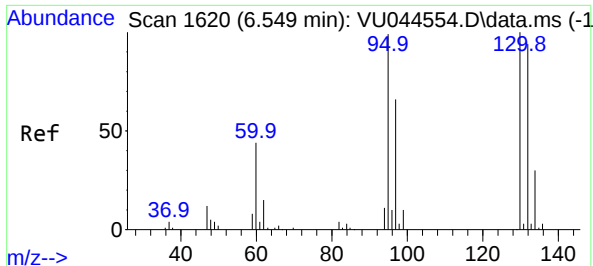


#34
Trichloroethene
Concen: 0.889 ug/L
RT: 6.546 min Scan# 1619
Delta R.T. -0.003 min
Lab File: VU044563.D
Acq: 02 Sep 2021 19:25

Instrument :
MSVOA_U
ClientSampleId :
F3W01

Tgt Ion: 95 Resp: 7875

Ion	Ratio	Lower	Upper
95	100		
97	61.1	45.6	84.8
132	91.7	63.4	117.8
130	91.8	65.8	122.2

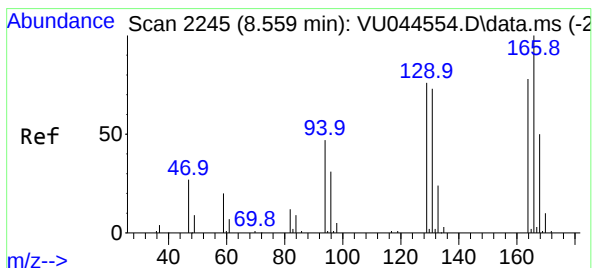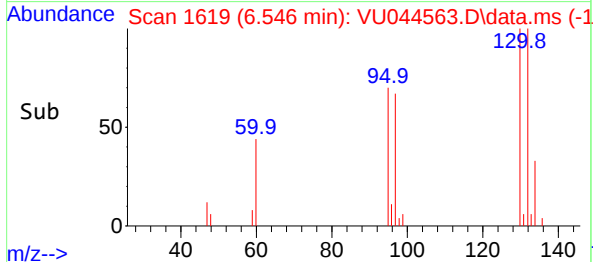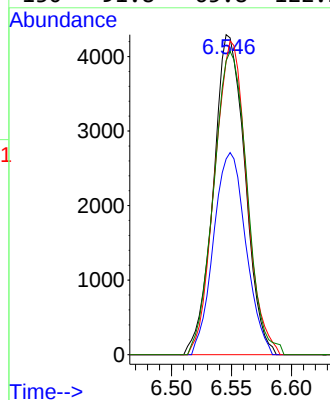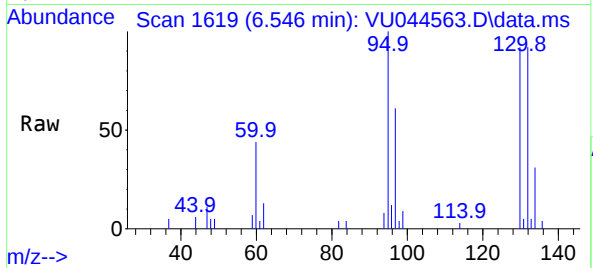

#47
Tetrachloroethene
Concen: 18.104 ug/L
RT: 8.558 min Scan# 2245
Delta R.T. -0.000 min
Lab File: VU044563.D
Acq: 02 Sep 2021 19:25

Tgt Ion: 164 Resp: 110936

Ion	Ratio	Lower	Upper
164	100		
129	96.0	71.0	131.8
131	91.7	68.0	126.4
166	130.3	89.0	165.4

