

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090221\
 Data File : VU044559.D
 Acq On : 02 Sep 2021 17:48
 Operator : SY/MD
 Sample : M3622-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU044559.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	94	rBV	58197	63926	5.62%	1.227%
2	1.919	171	180	192	rBV	53354	67575	5.94%	1.297%
3	2.086	223	232	240	rBV	21734	30534	2.69%	0.586%
4	2.144	240	250	265	rVB	249588	360676	31.73%	6.924%
5	2.572	369	383	398	rBV	92186	150428	13.23%	2.888%
6	4.649	1011	1029	1067	rBV3	44469	195239	17.18%	3.748%
7	5.073	1144	1161	1181	rBV	77222	175206	15.41%	3.364%
8	5.732	1344	1366	1394	rBV2	159153	408773	35.96%	7.847%
9	6.256	1513	1529	1547	rBV	122351	235737	20.74%	4.526%
10	6.549	1607	1620	1642	rVB2	75312	144748	12.73%	2.779%
11	6.697	1653	1666	1684	rBV	96329	190893	16.79%	3.665%
12	7.571	1924	1938	1954	rBV2	43845	77472	6.82%	1.487%
13	7.903	2025	2041	2056	rBV	195714	335912	29.55%	6.449%
14	8.186	2116	2129	2144	rBV2	26416	46167	4.06%	0.886%
15	8.558	2231	2245	2261	rVV	673410	1136722	100.00%	21.822%
16	8.645	2261	2272	2314	rVB2	201774	505125	44.44%	9.697%
17	9.423	2500	2514	2550	rBV	187502	320963	28.24%	6.162%
18	10.761	2918	2930	2947	rVB	81421	131169	11.54%	2.518%
19	11.816	3247	3258	3275	rBV	201402	317748	27.95%	6.100%
20	12.198	3365	3377	3394	rBV	195011	313951	27.62%	6.027%




Sum of corrected areas: 5208964

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090221\
Data File : VU044559.D
Acq On : 02 Sep 2021 17:48
Operator : SY/MD
Sample : M3622-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

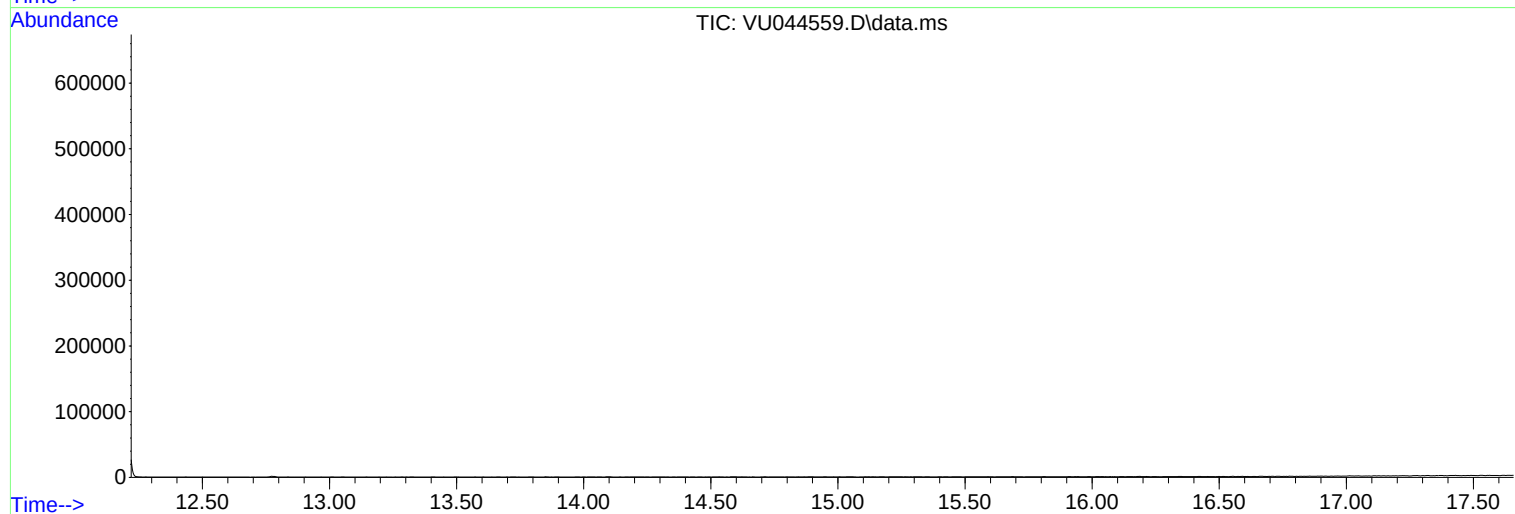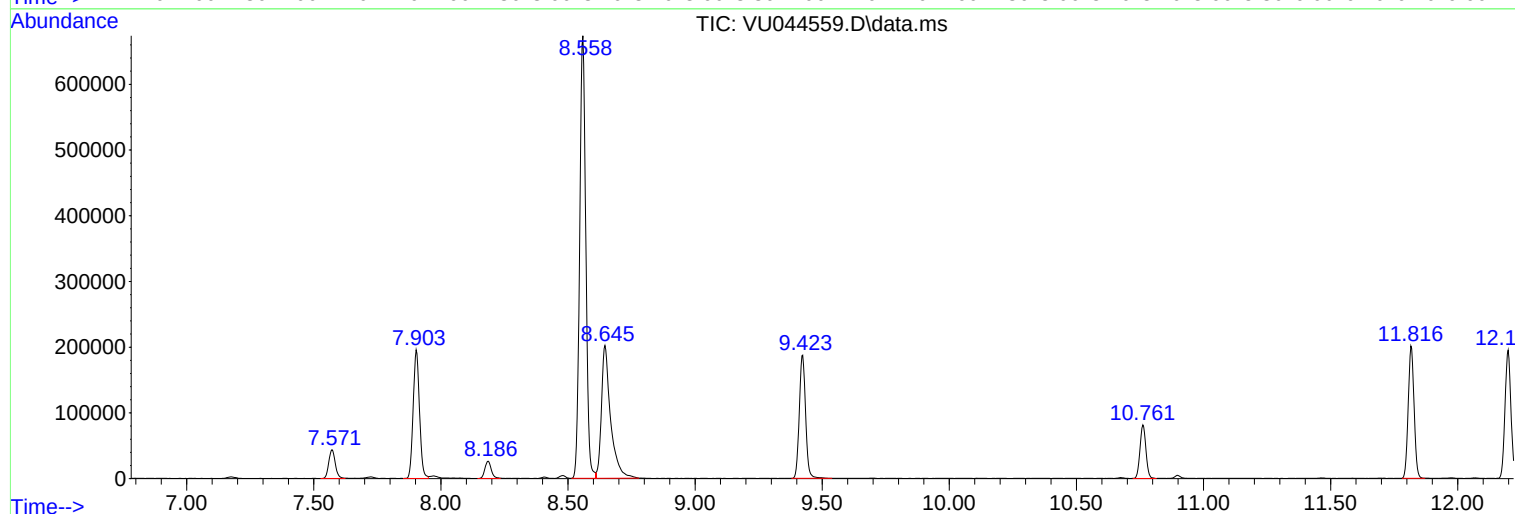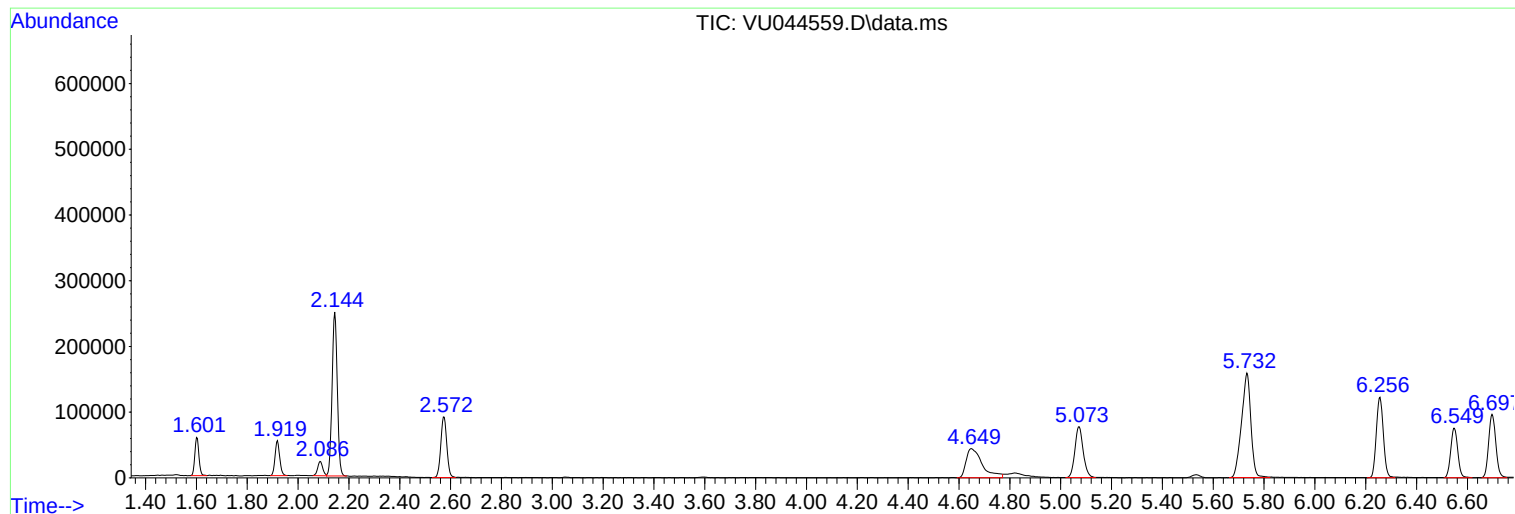

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090221\
Data File : VU044559.D
Acq On : 02 Sep 2021 17:48
Operator : SY/MD
Sample : M3622-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY5










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorodichloromethane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.086	0.65 ug/L	30534	1,4-Difluorobenzene	6.256

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
2			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
3			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
4			1-Butyne, 3,3-dimethyl-	82	C6H10	000917-92-0	7
5			1-Hexyne	82	C6H10	000693-02-7	7

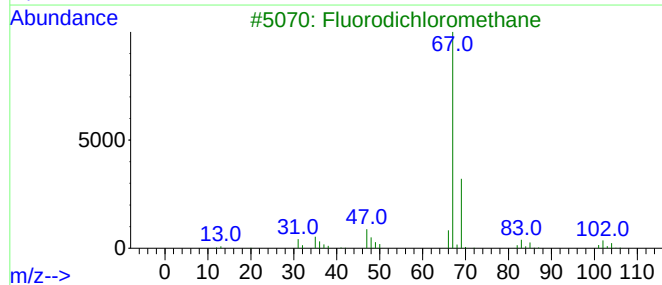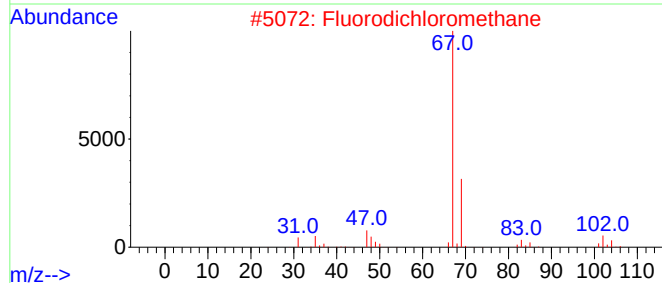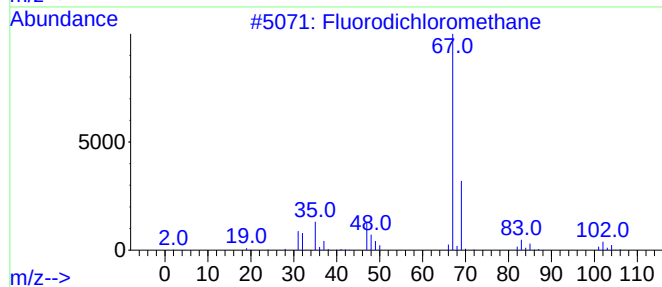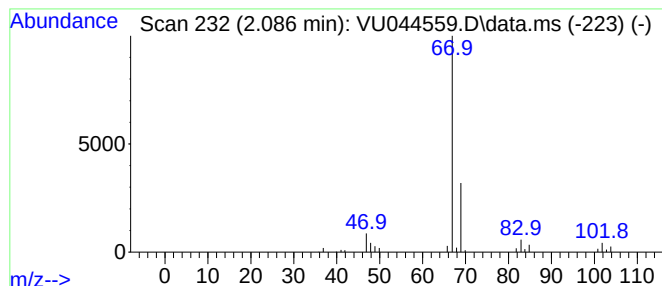

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090221\
Data File : VU044559.D
Acq On : 02 Sep 2021 17:48
Operator : SY/MD
Sample : M3622-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Fluorodichlorom...	2.086	0.7	ug/L	30534	1	6.256	235737	5.0