

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090221\
 Data File : VU044560.D
 Acq On : 02 Sep 2021 18:12
 Operator : SY/MD
 Sample : M3622-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU044560.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	92	rBV	60084	64744	4.01%	1.147%
2	1.919	171	180	193	rVB	52304	68138	4.22%	1.207%
3	2.086	224	232	240	rBV	18451	26185	1.62%	0.464%
4	2.144	240	250	266	rVB	238943	349975	21.67%	6.199%
5	2.572	372	383	398	rBV	92947	151267	9.37%	2.679%
6	4.645	1012	1028	1053	rBV3	45920	173931	10.77%	3.081%
7	5.070	1145	1160	1184	rBV	77803	176816	10.95%	3.132%
8	5.732	1344	1366	1386	rBV2	158757	410518	25.42%	7.271%
9	6.253	1511	1528	1549	rBV	123698	233599	14.46%	4.137%
10	6.549	1603	1620	1634	rBV	66670	125912	7.80%	2.230%
11	6.697	1651	1666	1683	rBV	99370	190914	11.82%	3.381%
12	7.571	1924	1938	1953	rBV	43600	77431	4.79%	1.371%
13	7.903	2028	2041	2058	rBV	193283	338137	20.94%	5.989%
14	8.186	2114	2129	2152	rBV	26073	45332	2.81%	0.803%
15	8.559	2231	2245	2261	rBV	939694	1615013	100.00%	28.605%
16	8.645	2261	2272	2323	rVB	199938	522461	32.35%	9.254%
17	9.420	2501	2513	2531	rBV	185486	314323	19.46%	5.567%
18	10.761	2918	2930	2947	rVB	80203	131135	8.12%	2.323%
19	11.816	3246	3258	3275	rBV	198626	315674	19.55%	5.591%
20	12.198	3365	3377	3397	rBV	194042	314445	19.47%	5.569%




Sum of corrected areas: 5645950

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090221\
Data File : VU044560.D
Acq On : 02 Sep 2021 18:12
Operator : SY/MD
Sample : M3622-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

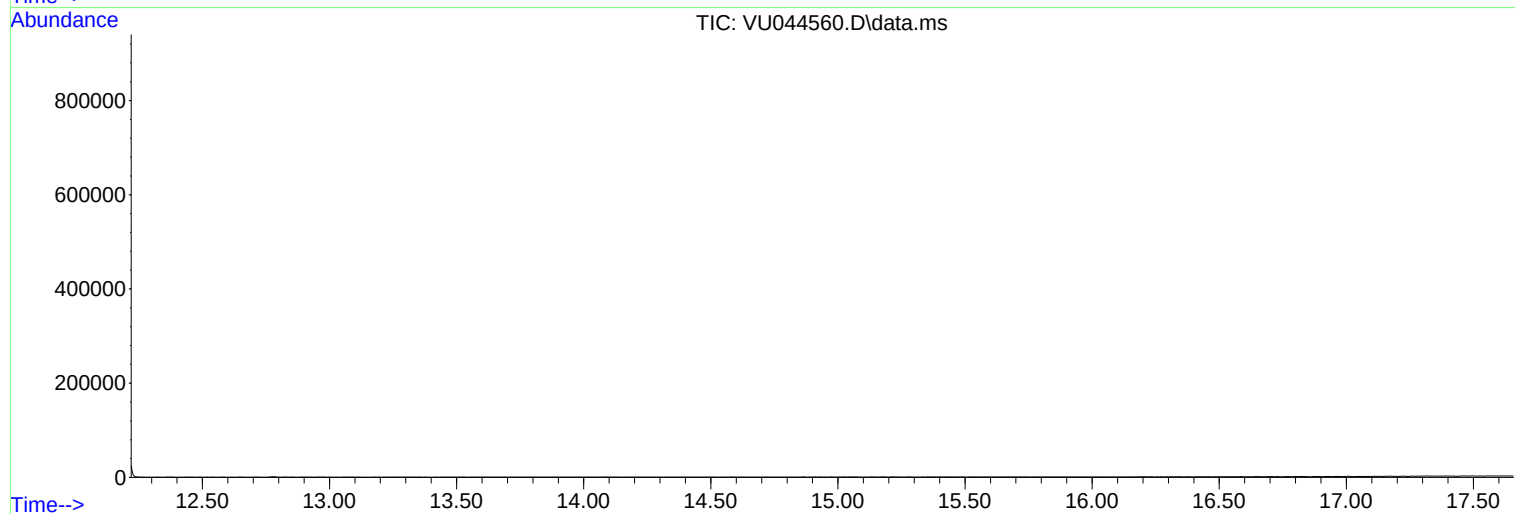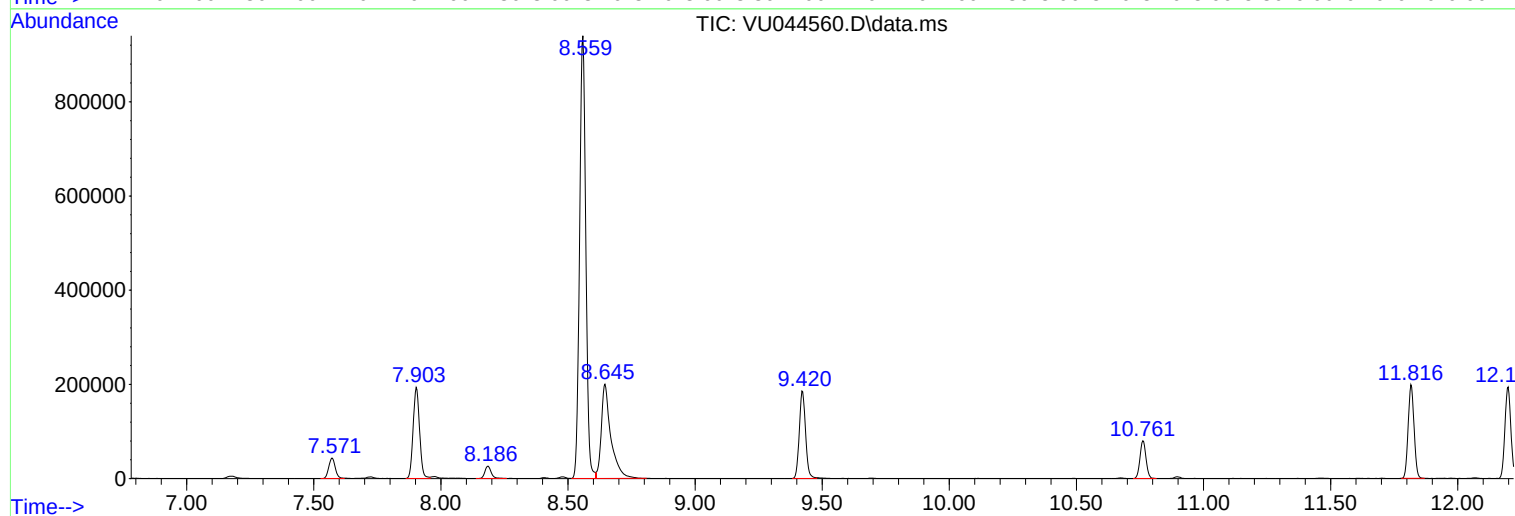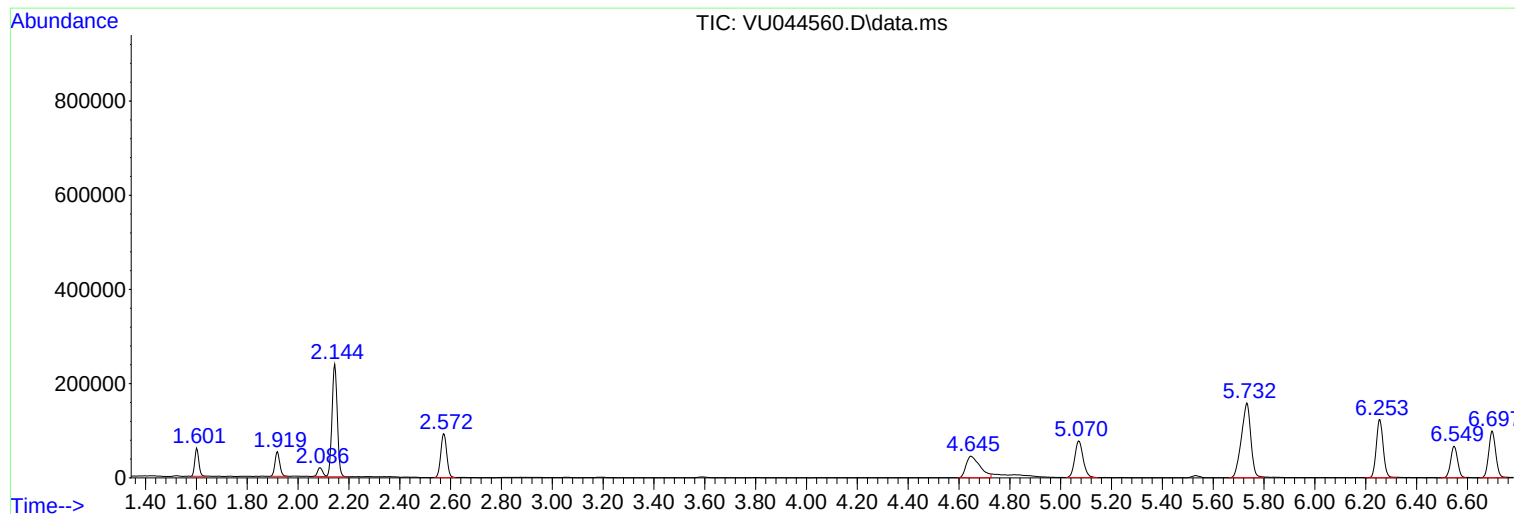

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090221\
Data File : VU044560.D
Acq On : 02 Sep 2021 18:12
Operator : SY/MD
Sample : M3622-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY6










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorodichloromethane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.086	0.56 ug/L	26185	1,4-Difluorobenzene	6.253

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
2			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
3			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
4			1-Butyne, 3,3-dimethyl-	82	C6H10	000917-92-0	7
5			Chlorine dioxide	67	ClO2	010049-04-4	4

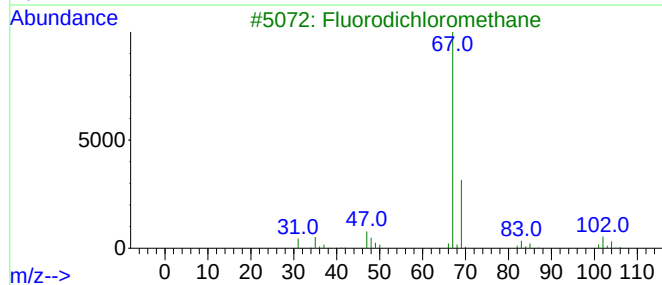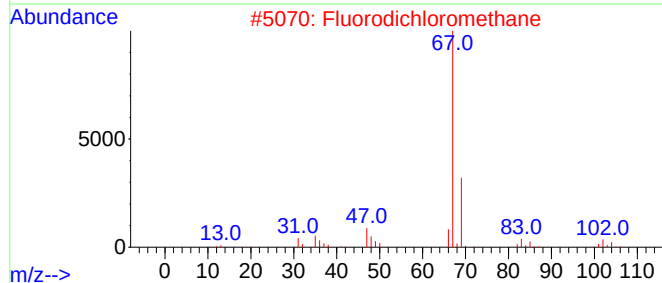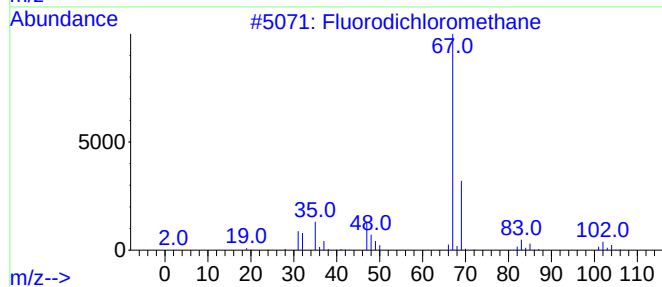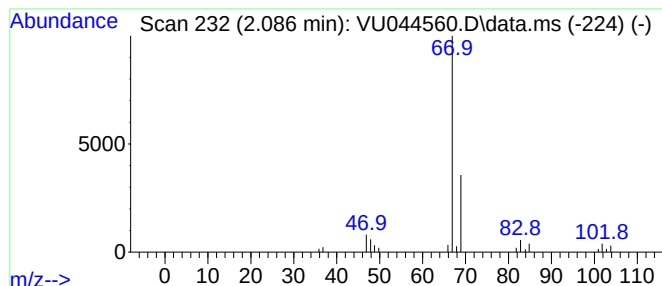

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090221\
Data File : VU044560.D
Acq On : 02 Sep 2021 18:12
Operator : SY/MD
Sample : M3622-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Fluorodichlorom...	2.086	0.6	ug/L	26185	1	6.253	233599	5.0