
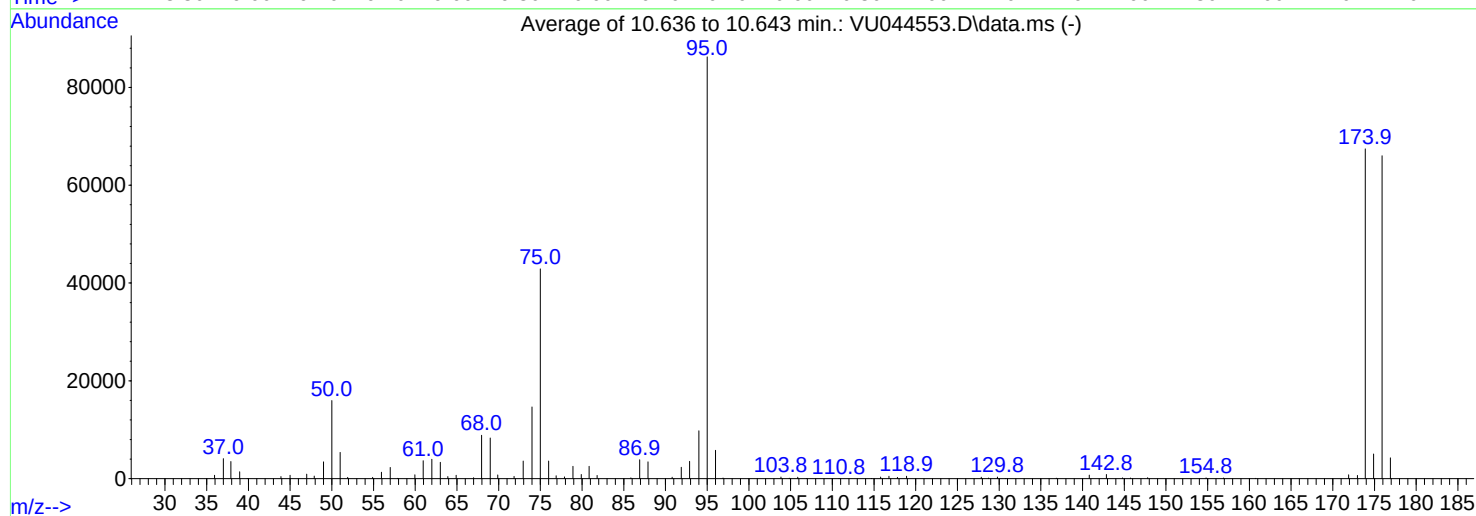


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090221\
 Data File : VU044553.D
 Acq On : 02 Sep 2021 14:13
 Operator : SY/MD
 Sample : BFB012
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB012

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Sep 08 02:31:37 2021

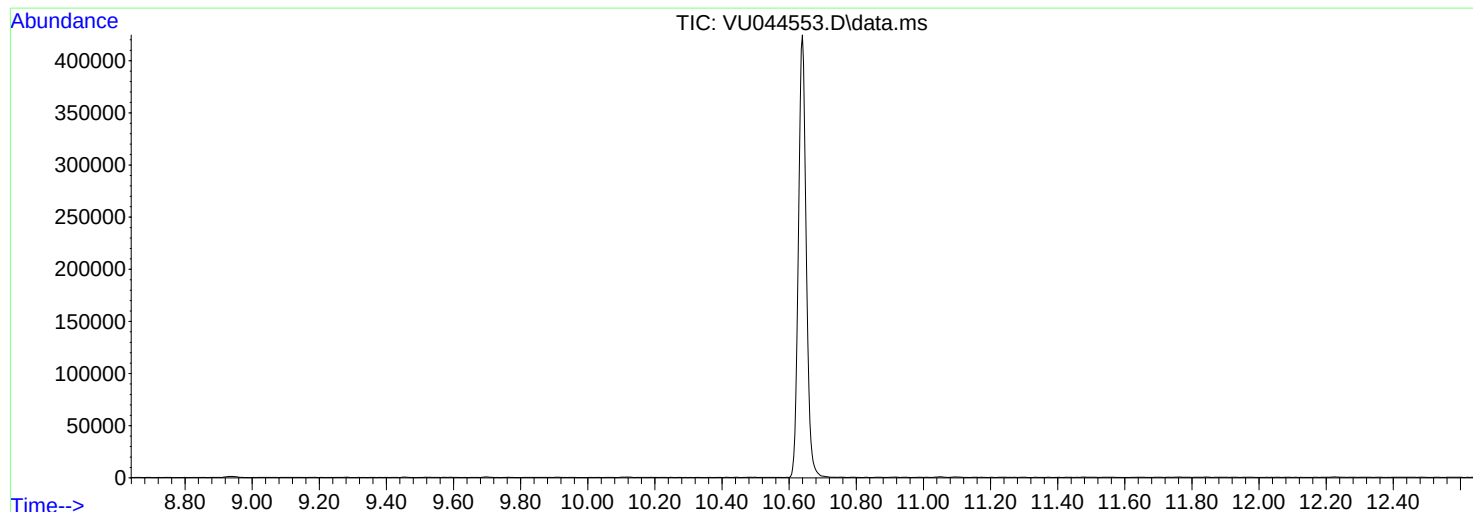

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	15953	PASS
75	95	30	80	49.7	42904	PASS
95	95	100	100	100.0	86251	PASS
96	95	5	9	6.7	5789	PASS
173	174	0.00	2	1.0	666	PASS
174	95	50	120	78.2	67427	PASS
175	174	5	9	7.5	5025	PASS
176	174	95	101	97.9	66016	PASS
177	176	5	9	6.4	4258	PASS

m/z	Abundance
35.90	630.0
37.00	3814.0
37.90	3408.0
38.90	1363.0
39.90	199.0
43.90	858.0
45.00	659.0
47.00	963.0
47.90	471.0
49.00	3182.0
50.00	15224.0
51.00	5121.0
51.90	254.0
54.90	199.0
55.90	1214.0
57.00	2221.0
57.90	123.0
60.00	795.0
60.90	3387.0
62.00	3791.0
63.00	3242.0
63.90	422.0
64.90	677.0
67.00	164.0
68.00	8512.0
69.00	7980.0
69.90	692.0
71.80	463.0
72.90	3448.0
74.00	13821.0
75.00	41128.0
76.00	3319.0
76.90	599.0
77.90	299.0
78.90	2395.0
79.90	728.0
80.80	2415.0
81.80	606.0
85.90	132.0
86.90	3670.0
87.90	3312.0
90.80	287.0
91.90	2163.0
92.90	3316.0
94.00	9406.0
95.00	83376.0
96.00	5468.0
96.90	110.0
103.90	350.0
104.80	110.0
105.80	270.0
114.70	102.0
115.80	287.0
116.80	461.0
117.80	267.0
118.90	495.0
127.90	253.0
128.70	129.0
129.80	323.0
130.80	101.0
136.80	105.0
140.80	695.0
142.90	846.0
144.80	130.0
145.80	119.0
147.80	192.0
154.80	156.0
156.90	142.0
160.70	102.0
171.90	778.0
172.90	644.0
173.90	66296.0
174.90	4896.0
175.90	65312.0
176.90	4126.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012

m/z	Abundance
39.80	126.0
43.90	419.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012

m/z	Abundance
36.00	726.0
37.00	4213.0
37.90	3513.0
39.00	1420.0
40.00	131.0
43.90	836.0
45.00	734.0
47.00	885.0
47.90	583.0
49.00	3571.0
50.00	16210.0
51.00	5438.0
51.90	276.0
54.90	292.0
56.00	1387.0
57.00	2320.0
59.90	766.0
61.00	3880.0
62.00	3982.0
63.00	3353.0
63.90	379.0
64.90	656.0
67.00	204.0
67.90	8926.0
69.00	8459.0
69.90	792.0
71.90	437.0
73.00	3655.0
74.00	15039.0
75.00	43352.0
76.00	3766.0
76.90	586.0
77.90	381.0
78.90	2589.0
79.90	912.0
80.90	2587.0
81.80	672.0
85.80	181.0
86.90	3987.0
87.90	3453.0
90.80	264.0
91.90	2442.0
92.90	3583.0
94.00	9837.0
95.00	86328.0
96.00	5917.0
96.90	147.0
103.80	330.0
104.90	106.0
105.90	328.0
115.80	361.0
116.80	539.0
117.80	290.0
118.90	499.0
127.80	349.0
128.80	147.0
129.80	297.0
136.90	102.0
140.80	708.0
142.80	845.0
144.80	193.0
145.70	137.0
147.80	223.0
154.80	169.0
156.90	103.0
171.90	782.0
173.00	695.0
173.90	66296.0
174.90	4989.0
175.90	64264.0
176.90	4294.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012

m/z	Abundance
35.90	716.0
37.00	4213.0
37.90	3610.0
39.00	1473.0
39.90	163.0
43.90	848.0
45.00	721.0
47.00	955.0
47.90	552.0
49.00	3524.0
50.00	16424.0
51.00	5547.0
51.90	262.0
54.90	258.0
56.00	1343.0
57.00	2381.0
57.90	107.0
60.00	785.0
61.00	3775.0
62.00	4061.0
63.00	3408.0
63.90	436.0
64.90	715.0
67.00	194.0
68.00	9132.0
69.00	8543.0
69.90	804.0
71.90	472.0
72.90	3718.0
74.00	15119.0
75.00	44232.0
76.00	3699.0
76.90	630.0
77.90	377.0
78.90	2613.0
79.90	885.0
80.80	2580.0
81.80	697.0
85.80	166.0
86.90	3974.0
87.90	3526.0
90.80	288.0
91.90	2396.0
92.90	3668.0
94.00	10100.0
95.00	89048.0
96.00	5983.0
96.90	130.0
103.90	362.0
104.90	121.0
105.90	318.0
106.90	101.0
110.80	105.0
115.80	344.0
116.80	507.0
117.80	279.0
118.90	527.0
127.90	324.0
128.80	149.0
129.80	347.0
136.90	105.0
140.80	747.0
142.90	885.0
144.80	171.0
145.80	146.0
147.80	221.0
154.80	159.0
156.90	131.0
160.80	117.0
171.90	831.0
173.00	658.0
173.90	69688.0
174.90	5191.0
175.90	68472.0
176.90	4355.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012