


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090222\
 Data File : VU050595.D
 Acq On : 02 Sep 2022 10:38
 Operator : SY/MD
 Sample : BFB118
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB118

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis
 Last Update : Mon Sep 05 01:05:15 2022

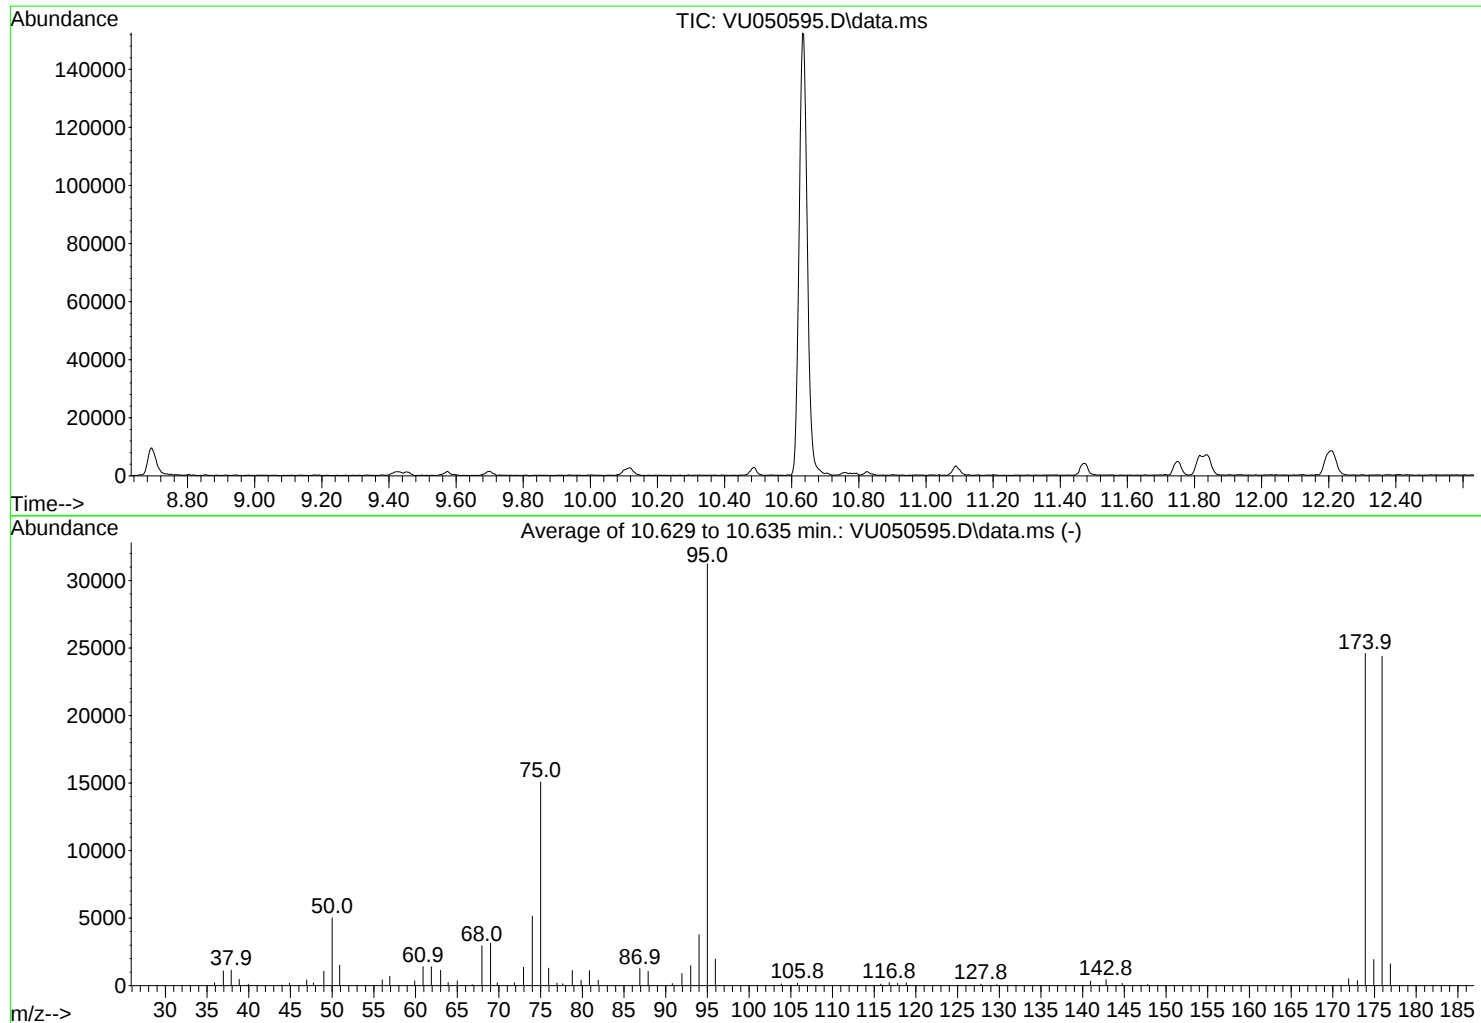

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	5016	PASS
75	95	30	80	48.2	15068	PASS
95	95	100	100	100.0	31235	PASS
96	95	5	9	6.3	1967	PASS
173	174	0.00	2	1.5	365	PASS
174	95	50	120	78.7	24592	PASS
175	174	5	9	7.8	1930	PASS
176	174	95	101	99.2	24389	PASS
177	176	5	9	6.6	1614	PASS

m/z	Abundance
44.00	307.0

Instrument :
MSVOA_U
ClientSampleId :
BFB118

m/z	Abundance
35.90	205.0
36.90	1043.0
37.90	1115.0
38.90	481.0
39.90	102.0
43.90	324.0
44.80	151.0
47.00	463.0
47.70	220.0
49.00	1076.0
50.00	4821.0
50.90	1551.0
56.00	452.0
56.90	683.0
59.90	389.0
60.90	1346.0
61.90	1360.0
63.00	1137.0
63.90	243.0
65.00	325.0
66.80	107.0
68.00	2850.0
69.00	3041.0
69.80	248.0
71.80	197.0
73.00	1287.0
74.00	4976.0
75.00	14113.0
76.00	1295.0
77.00	195.0
77.60	137.0
78.80	1063.0
79.90	380.0
80.90	978.0
81.90	347.0
86.90	1155.0
87.90	1031.0
90.80	164.0
91.90	847.0
93.00	1321.0
94.00	3690.0
95.00	29488.0
96.00	1860.0
103.90	125.0
105.80	179.0
115.80	112.0
116.70	228.0
117.80	177.0
118.80	197.0
129.70	132.0
141.00	332.0
142.70	405.0
144.80	163.0
171.90	427.0
172.90	360.0
173.90	23032.0
174.90	1808.0
175.90	22416.0
176.90	1433.0

Instrument :
MSVOA_U
ClientSampleId :
BFB118

m/z	Abundance
35.90	216.0
36.90	1113.0
37.90	1168.0
38.80	453.0
39.90	112.0
43.90	355.0
44.90	185.0
47.00	410.0
47.70	214.0
49.00	1076.0
50.00	5164.0
50.90	1533.0
56.00	447.0
56.90	709.0
59.90	351.0
60.90	1447.0
61.90	1417.0
63.00	1136.0
63.90	238.0
65.00	344.0
66.80	108.0
67.90	3064.0
69.00	3222.0
69.80	207.0
71.80	240.0
72.90	1406.0
74.00	5318.0
75.00	15466.0
75.90	1305.0
76.90	181.0
77.60	147.0
78.80	1155.0
79.90	415.0
80.80	1142.0
81.90	421.0
86.90	1343.0
87.90	1070.0
90.80	161.0
92.00	931.0
93.00	1489.0
94.00	3860.0
95.00	32184.0
96.00	2002.0
103.80	132.0
105.80	199.0
115.80	117.0
116.80	220.0
117.80	181.0
118.80	221.0
127.80	150.0
129.70	123.0
141.00	336.0
142.80	430.0
144.80	164.0
147.80	124.0
171.90	554.0
172.90	377.0
173.90	25280.0
174.90	1981.0
175.90	25288.0
176.90	1680.0

Instrument :
MSVOA_U
ClientSampleId :
BFB118

m/z	Abundance
35.90	211.0
37.00	1109.0
37.90	1159.0
38.90	441.0
40.00	115.0
43.90	378.0
45.00	203.0
46.80	380.0
47.80	175.0
49.00	1055.0
50.00	5062.0
50.90	1431.0
56.00	369.0
56.90	676.0
59.90	281.0
60.90	1442.0
61.90	1420.0
63.00	1123.0
63.90	238.0
65.00	371.0
67.90	2925.0
69.00	3169.0
69.80	168.0
71.90	233.0
72.90	1404.0
74.00	5157.0
75.00	15626.0
75.90	1265.0
76.90	182.0
77.70	135.0
78.80	1173.0
79.80	392.0
80.80	1244.0
81.90	396.0
86.90	1317.0
87.90	1106.0
90.80	127.0
92.00	924.0
93.00	1614.0
94.00	3760.0
95.00	32032.0
95.90	2039.0
103.80	124.0
105.80	171.0
115.80	130.0
116.90	231.0
117.80	153.0
118.90	234.0
127.80	174.0
140.90	336.0
142.90	513.0
144.70	172.0
147.80	133.0
171.90	574.0
173.00	358.0
173.90	25464.0
174.90	2001.0
175.90	25464.0
176.90	1729.0

Instrument :
MSVOA_U
ClientSampleId :
BFB118