

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU090319\
 Data File : VU034204.D
 Acq On : 02 Sep 2019 15:59
 Operator : JC/SP
 Sample : K4544-38
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 T16-17-C4-(2.25)

Quant Time: Sep 03 05:55:38 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 29 04:11:12 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.96	168	432521	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.87	114	716059	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.07	117	715022	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.46	152	346307	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	5.29	65	283007	51.07	ug/l	0.00
Spiked Amount			Recovery	=	102.14%	
35) Dibromofluoromethane	4.86	113	235542	47.43	ug/l	0.00
Spiked Amount			Recovery	=	94.86%	
50) Toluene-d8	7.55	98	934752	50.26	ug/l	0.00
Spiked Amount			Recovery	=	100.52%	
62) 4-Bromofluorobenzene	10.29	95	323768	44.76	ug/l	0.00
Spiked Amount			Recovery	=	89.52%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.32	50	536	Below Cal	#	84
5) Bromomethane	1.63	94	291	Below Cal	#	68
8) Diethyl Ether	2.09	74	740	0.258	ug/l #	30
11) Tert butyl alcohol	2.82	59	3910	3.059	ug/l #	73
13) Acrolein	2.19	56	219	0.407	ug/l #	70
16) Acetone	2.31	43	13535	4.786	ug/l	95
18) Methyl Acetate	2.61	43	3659	0.501	ug/l #	76
20) Methylene Chloride	2.69	84	8706	1.626	ug/l	90
31) Cyclohexane	4.96	56	7928	0.958	ug/l #	1
36) 1,1-Dichloropropene	4.96	75	31446	4.643	ug/l #	48
38) Carbon Tetrachloride	4.96	117	40153	6.142	ug/l #	16
43) Isopropyl Acetate	5.53	43	83094	7.201	ug/l	98
48) Methyl methacrylate	6.52	41	4449	0.799	ug/l #	14
49) 1,4-Dioxane	6.68	88	114	0.817	ug/l #	1
51) 4-Methyl-2-Pentanone	7.40	43	77791	9.762	ug/l #	46
54) cis-1,3-Dichloropropene	7.40	75	36765	4.265	ug/l #	65
56) Ethyl methacrylate	7.93	69	203	0.994	ug/l #	27
57) 1,3-Dichloropropane	8.40	76	6519	0.719	ug/l #	42
59) 2-Hexanone	8.40	43	85753	14.255	ug/l #	52
74) N-amyl acetate	9.93	43	2686	0.275	ug/l #	46
76) 1,2,3-Trichloropropane	10.29	75	155169	19.880	ug/l #	37
81) trans-1,4-Dichloro-2-buten	10.29	75	155169	66.942	ug/l #	100
95) Naphthalene	13.79	128	45	1.792	ug/l #	70

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU090319\
Data File : VU034204.D
Acq On : 02 Sep 2019 15:59
Operator : JC/SP
Sample : K4544-38
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
T16-17-C4-(2.25)

Quant Time: Sep 03 05:55:38 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 29 04:11:12 2019
Response via : Initial Calibration

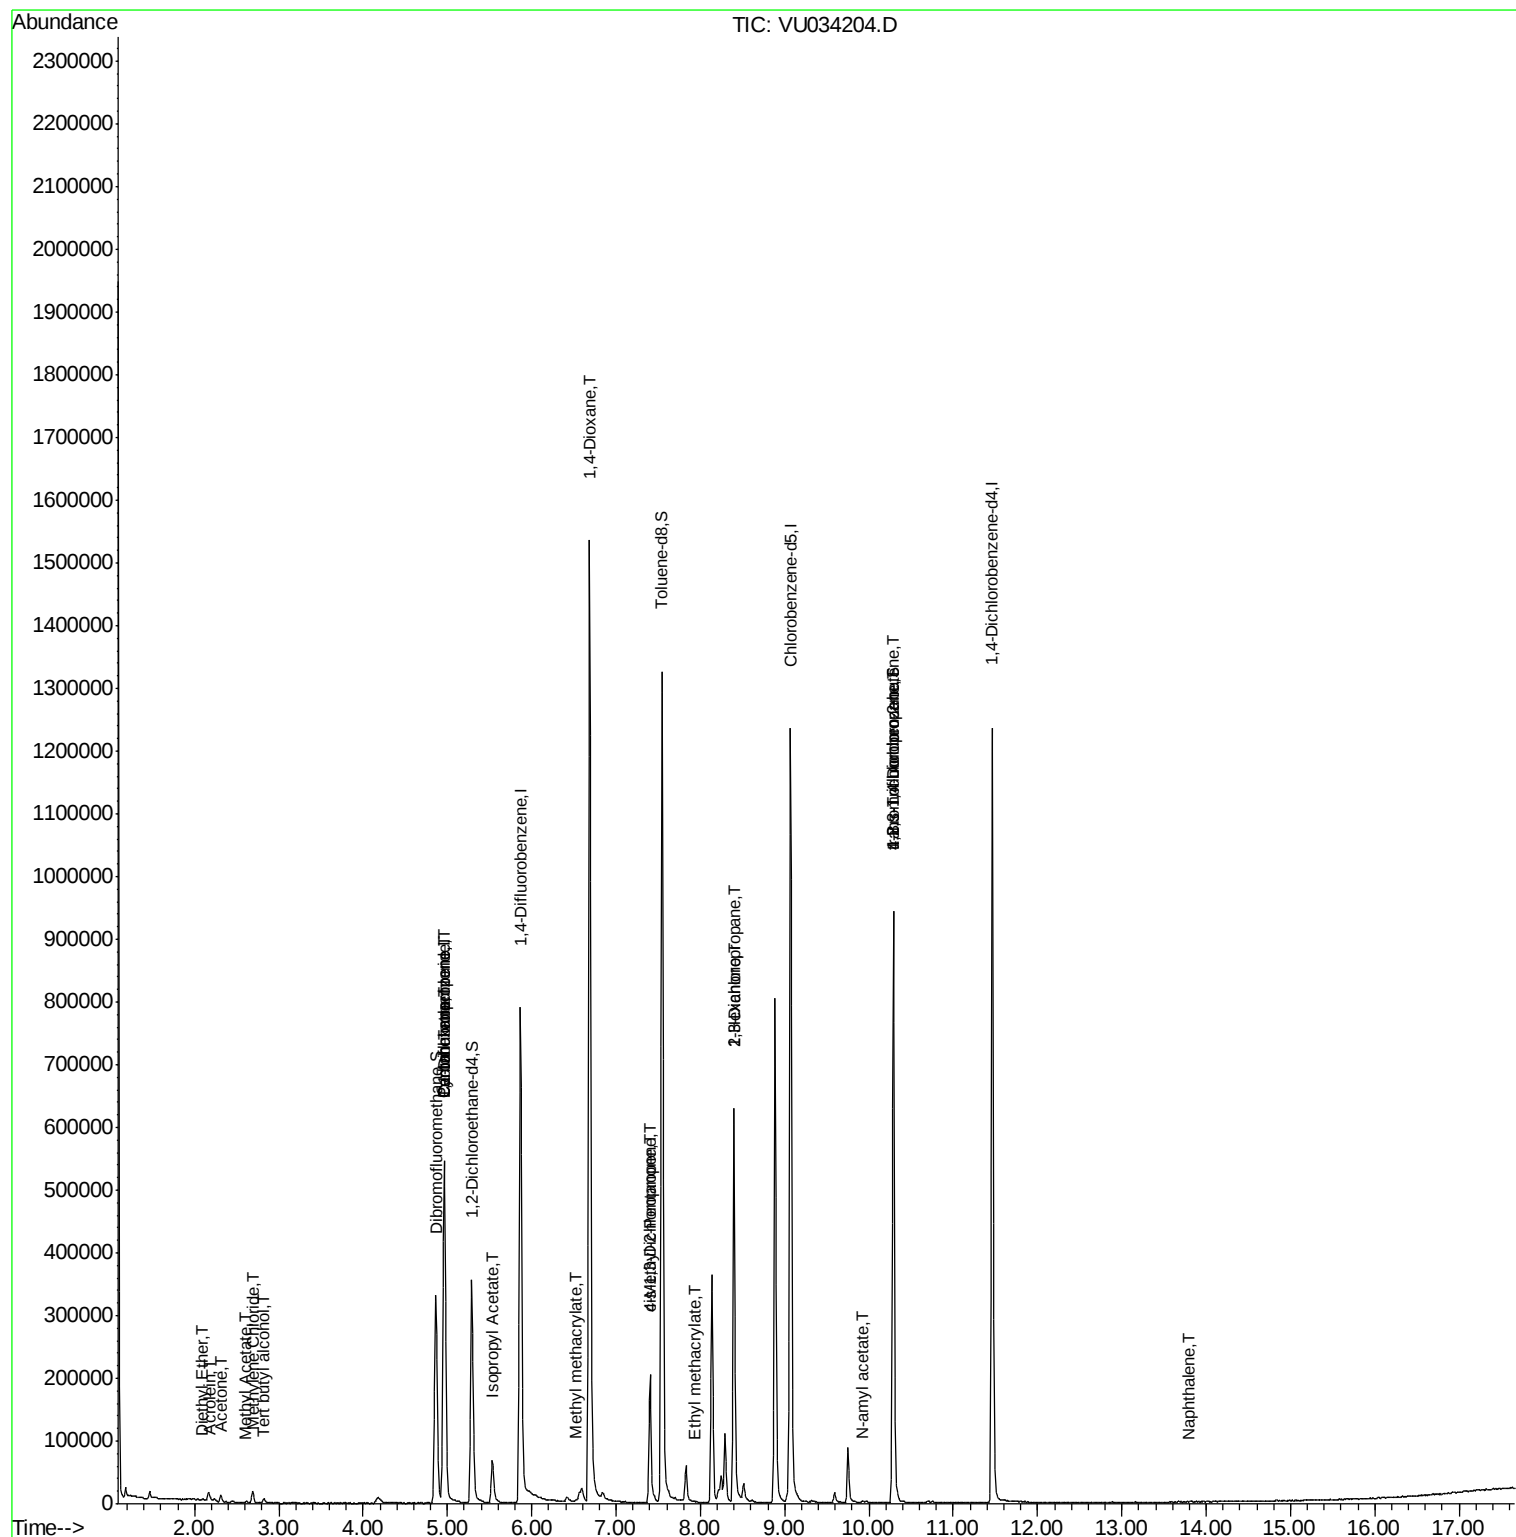



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.96 min Scan# 1204

Delta R.T. 0.00 min

Lab File: VU034204.D

Acq: 02 Sep 2019 15:59

Instrument :

MSVOA_U

ClientSampleId :


T16-17-C4-(2.25)

Tgt Ion:168 Resp: 432521

Ion Ratio Lower Upper

168 100

99 54.6 42.3 63.5



Abundance Ion 167.90 (167.60 to 168.60): VU034018.D (-1185) (-)

Ion 98.90 (98.60 to 99.60): VU034018.D (-1185) (-)

4.96

200000

150000


100000

50000

0

4.85 4.90 4.95 5.00 5.05

Time-->



#3

Chloromethane

Concen: Below Cal

RT: 1.32 min Scan# 73

Delta R.T. 0.00 min

Lab File: VU034204.D


Acq: 02 Sep 2019 15:59

Tgt Ion: 50 Resp: 536

Ion Ratio Lower Upper

50 100

52 24.0 26.2 39.4#



Abundance Ion 49.90 (49.60 to 50.60): VU034018.D (-63) (-)

Ion 51.90 (51.60 to 52.60): VU034018.D (-63) (-)

1.32

600

500

400

300


200

100

0

1.30 1.32 1.34 1.36

Time-->





#5

Bromomethane

Concen: Below Cal

RT: 1.63 min Scan# 167

Delta R.T. 0.03 min

Lab File: VU034204.D

Acq: 02 Sep 2019 15:59

Instrument :

MSVOA_U

ClientSampleId :


T16-17-C4-(2.25)

Tgt Ion: 94 Resp: 291

Ion Ratio Lower Upper




94 100

96 64.2 76.3 114.5#



Abundance Ion 93.90 (93.60 to 94.60): VU0

Ion 95.90 (95.60 to 96.60): VU0

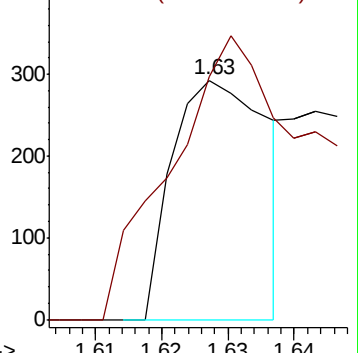

#8

Diethyl Ether

Concen: 0.258 ug/l

RT: 2.09 min Scan# 312

Delta R.T. 0.00 min

Lab File: VU034204.D


Acq: 02 Sep 2019 15:59

Tgt Ion: 74 Resp: 740

Ion Ratio Lower Upper



74 100


45 174.9 51.8 155.5#



Abundance Ion 74.00 (73.70 to 74.70): VU0

Ion 45.00 (44.70 to 45.70): VU0

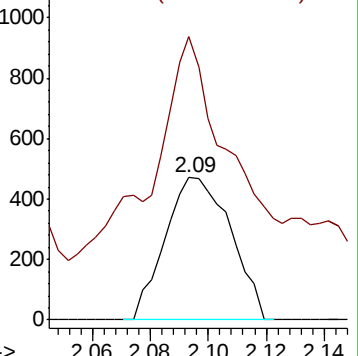

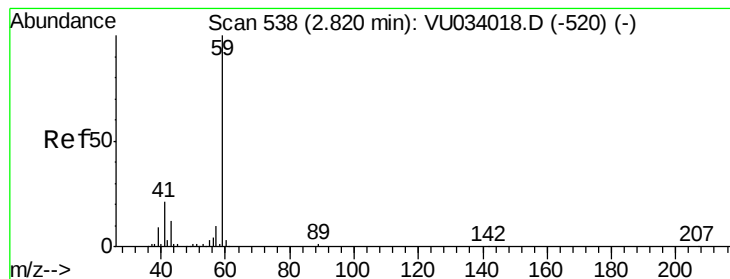

#11

Tert butyl alcohol

Concen: 3.059 ug/l

RT: 2.82 min Scan# 538

Delta R.T. 0.00 min

Lab File: VU034204.D

Acq: 02 Sep 2019 15:59

Instrument :

MSVOA_U

ClientSampleId :


T16-17-C4-(2.25)

Tgt Ion: 59 Resp: 3910

Ion Ratio Lower Upper




59 100

57 0.0 8.0 12.0#

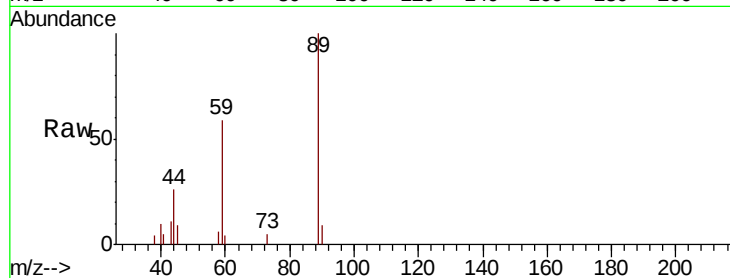

Abundance Ion 59.00 (58.70 to 59.70): VU034204.D (-445) (-)

Ion 57.00 (56.70 to 57.70): VU034204.D (-445) (-)

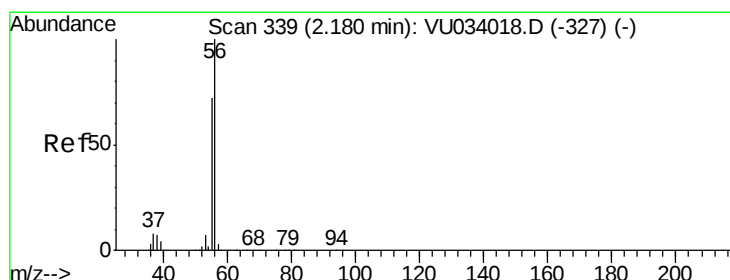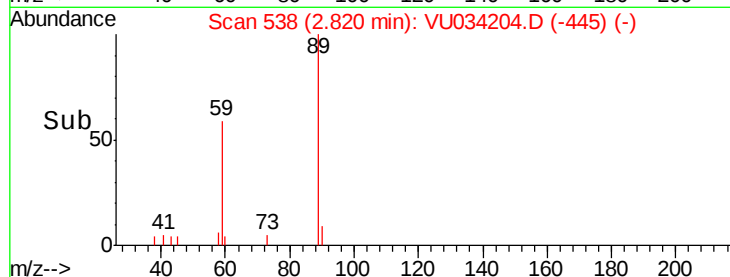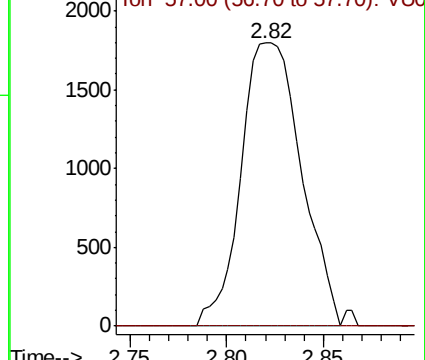

#13

Acrolein

Concen: 0.407 ug/l

RT: 2.19 min Scan# 342

Delta R.T. 0.01 min

Lab File: VU034204.D


Acq: 02 Sep 2019 15:59

Tgt Ion: 56 Resp: 219

Ion Ratio Lower Upper



56 100


55 46.1 57.1 85.7#

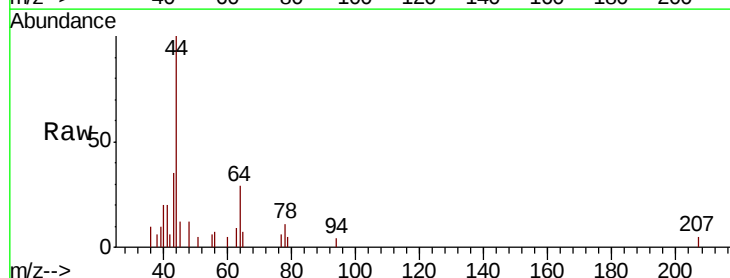

Abundance Ion 56.00 (55.70 to 56.70): VU034204.D (-246) (-)

Ion 55.00 (54.70 to 55.70): VU034204.D (-246) (-)

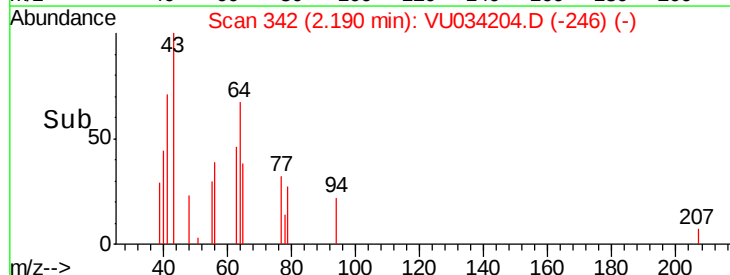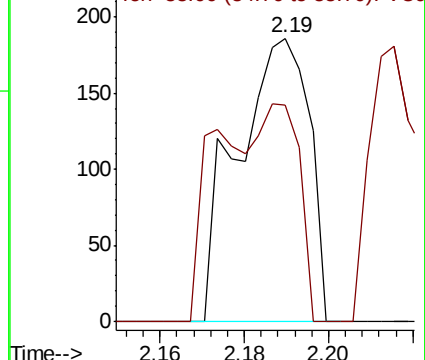

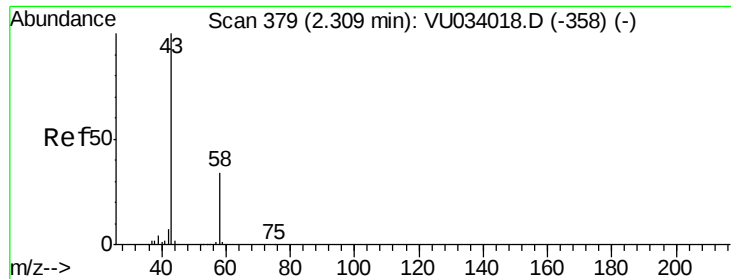

#16

Acetone

Concen: 4.786 ug/l

RT: 2.31 min Scan# 380

Delta R.T. 0.00 min

Lab File: VU034204.D

Acq: 02 Sep 2019 15:59

Instrument :

MSVOA_U

ClientSampleId :





T16-17-C4-(2.25)

Tgt Ion: 43 Resp: 13535

Ion Ratio Lower Upper

43 100

58 36.2 26.8 40.2

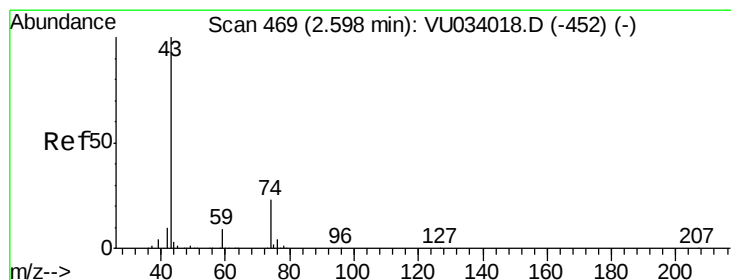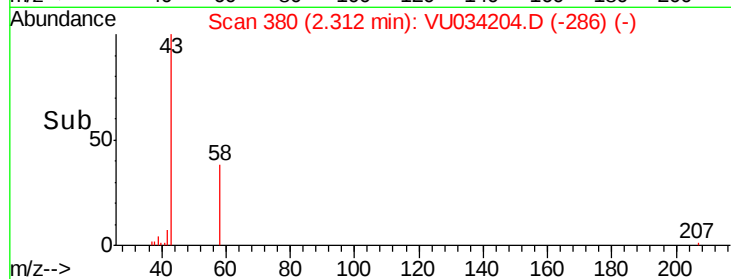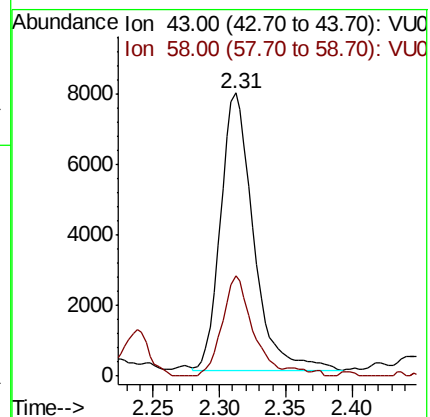

#18

Methyl Acetate

Concen: 0.501 ug/l

RT: 2.61 min Scan# 473

Delta R.T. 0.01 min

Lab File: VU034204.D




Acq: 02 Sep 2019 15:59


Tgt Ion: 43 Resp: 3659

Ion Ratio Lower Upper

43 100

74 12.2 19.2 28.8#

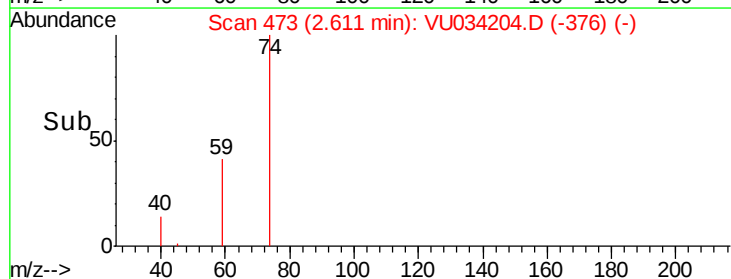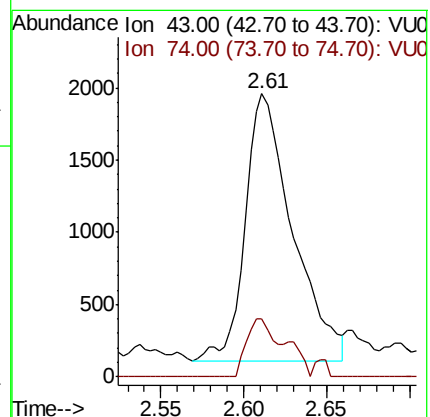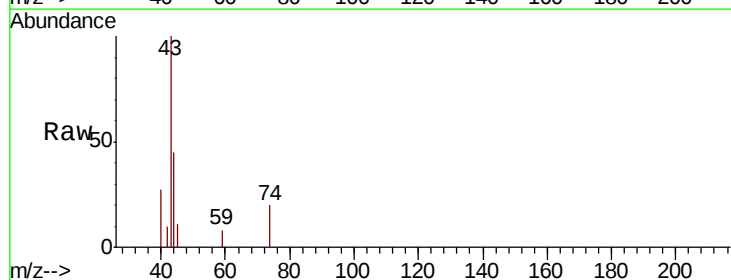



#20

Methylene Chloride

Concen: 1.626 ug/l

RT: 2.69 min Scan# 498

Delta R.T. 0.01 min

Lab File: VU034204.D

Acq: 02 Sep 2019 15:59

Instrument :

MSVOA_U

ClientSampleId :

T16-17-C4-(2.25)

Tgt Ion: 84 Resp: 8706


Ion Ratio Lower Upper

84 100

49 113.9 100.2 150.4

51 42.1 30.8 46.2

86 56.6 52.5 78.7






Abundance Ion 83.90 (83.60 to 84.60): VU0

Ion 48.90 (48.60 to 49.60): VU0

Ion 50.90 (50.60 to 51.60): VU0

Ion 85.90 (85.60 to 86.60): VU0

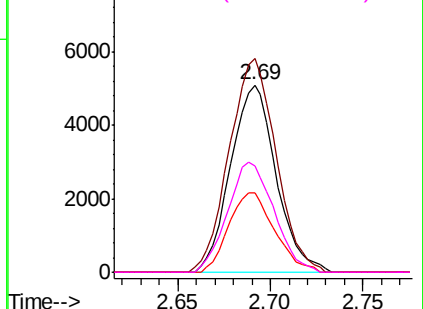

#31

Cyclohexane

Concen: 0.958 ug/l

RT: 4.96 min Scan# 1204

Delta R.T. -0.01 min

Lab File: VU034204.D

Acq: 02 Sep 2019 15:59


Tgt Ion: 56 Resp: 7928

Ion Ratio Lower Upper

56 100

69 190.7 25.4 38.0#



84 152.9 65.8 98.8#




Abundance Ion 56.00 (55.70 to 56.70): VU0

Ion 69.00 (68.70 to 69.70): VU0

Ion 84.00 (83.70 to 84.70): VU0




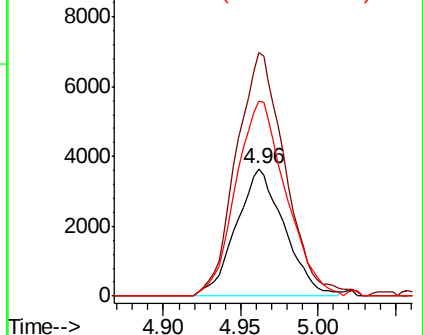




#33
 1,2-Dichloroethane-d4
 Concen: 51.065 ug/l
 RT: 5.29 min Scan# 1306
 Delta R.T. 0.00 min
 Lab File: VU034204.D
 Acq: 02 Sep 2019 15:59




Instrument :
 MSVOA_U
 ClientSampleId :
 T16-17-C4-(2.25)


Tgt Ion: 65 Resp: 283007
 Ion Ratio Lower Upper
 65 100
 67 53.7 0.0 110.6

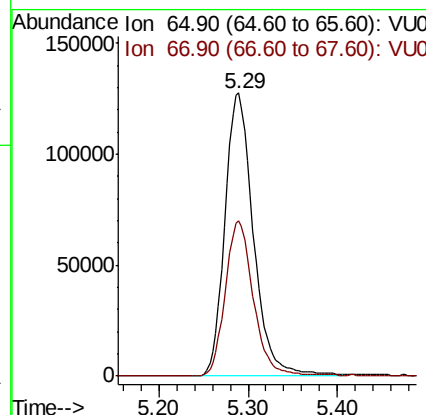

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 5.87 min Scan# 1486
 Delta R.T. 0.00 min
 Lab File: VU034204.D
 Acq: 02 Sep 2019 15:59

Tgt Ion: 114 Resp: 716059
 Ion Ratio Lower Upper
 114 100
 63 21.4 0.0 42.0
 88 16.1 0.0 32.0


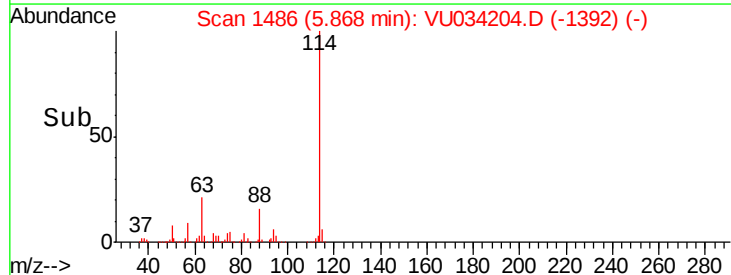
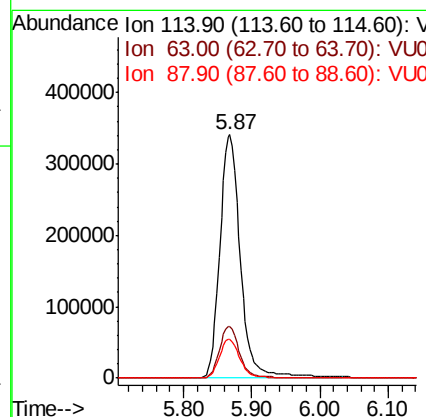





#35
 Dibromofluoromethane
 Concen: 47.426 ug/l
 RT: 4.86 min Scan# 1173
 Delta R.T. 0.00 min
 Lab File: VU034204.D
 Acq: 02 Sep 2019 15:59




Instrument :
 MSVOA_U
 ClientSampleId :
 T16-17-C4-(2.25)


Tgt Ion	Ratio	Lower	Upper
113	100		
111	104.3	81.7	122.5
192	21.9	17.1	25.7

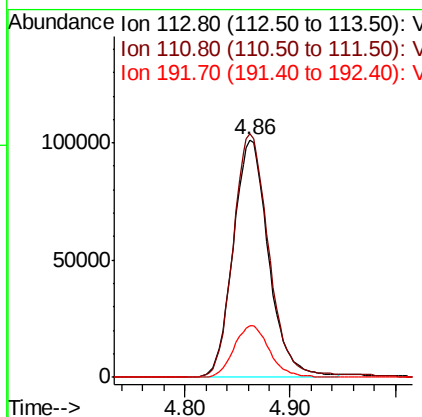

#36
 1,1-Dichloropropene
 Concen: 4.643 ug/l
 RT: 4.96 min Scan# 1204
 Delta R.T. -0.15 min
 Lab File: VU034204.D
 Acq: 02 Sep 2019 15:59

Tgt Ion	Ratio	Lower	Upper
75	100		
110	7.9	17.8	53.5#
77	0.0	25.0	37.4#

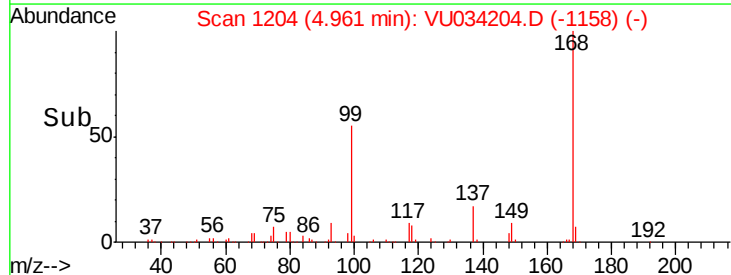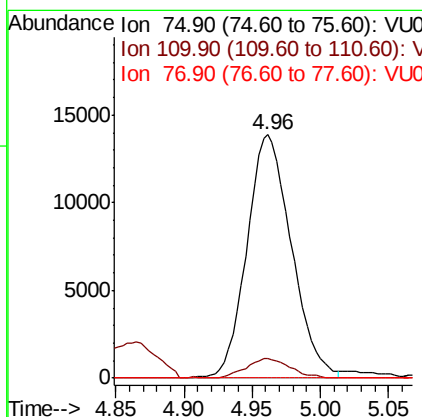


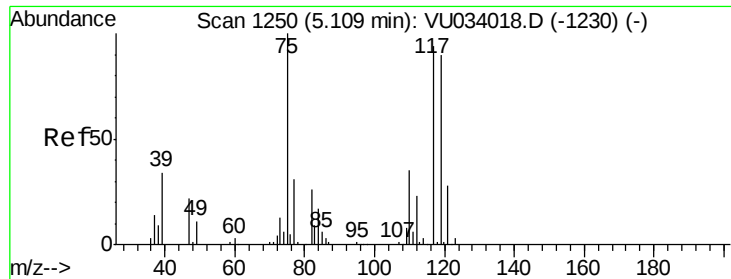




#38
Carbon Tetrachloride
Concen: 6.142 ug/l
RT: 4.96 min Scan# 1205
Delta R.T. -0.14 min
Lab File: VU034204.D
Acq: 02 Sep 2019 15:59

Instrument :
MSVOA_U
ClientSampleId :
T16-17-C4-(2.25)

Tgt Ion:117 Resp: 40153
Ion Ratio Lower Upper
117 100
119 5.2 77.0 115.4#
121 0.0 23.9 35.9#




Abundance Ion 116.80 (116.50 to 117.50): V
Ion 118.80 (118.50 to 119.50): V
Ion 120.80 (120.50 to 121.50): V


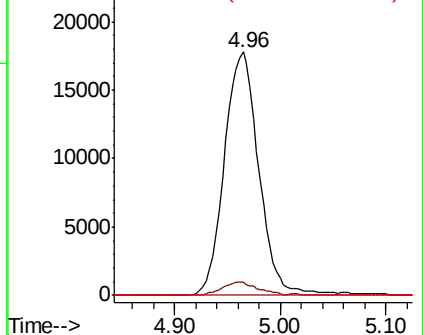



#43
Isopropyl Acetate
Concen: 7.201 ug/l
RT: 5.53 min Scan# 1382
Delta R.T. 0.01 min
Lab File: VU034204.D
Acq: 02 Sep 2019 15:59

Tgt Ion: 43 Resp: 83094
Ion Ratio Lower Upper
43 100
61 20.4 17.2 25.8
87 12.7 10.8 16.2



Abundance Ion 43.00 (42.70 to 43.70): VU0
Ion 61.00 (60.70 to 61.70): VU0
Ion 87.00 (86.70 to 87.70): VU0




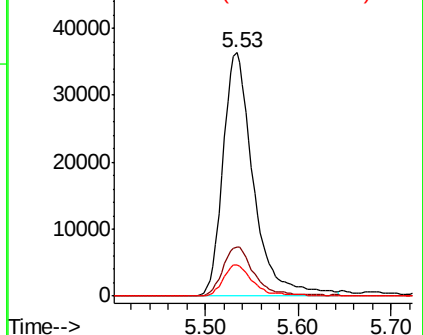




#48
Methyl methacrylate
Concen: 0.799 ug/l
RT: 6.52 min Scan# 1690
Delta R.T. -0.08 min
Lab File: VU034204.D
Acq: 02 Sep 2019 15:59




Instrument :
MSVOA_U
ClientSampleId :
T16-17-C4-(2.25)


Tgt Ion: 41 Resp: 4449
Ion Ratio Lower Upper
41 100
69 0.0 69.5 104.3#
39 0.0 40.3 60.5#

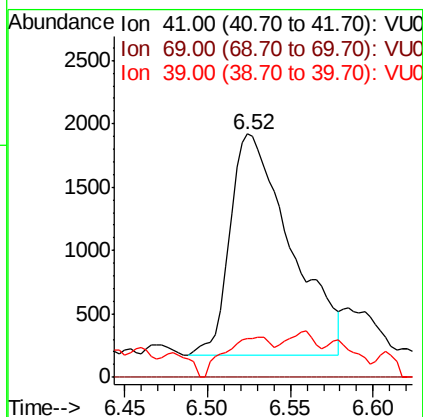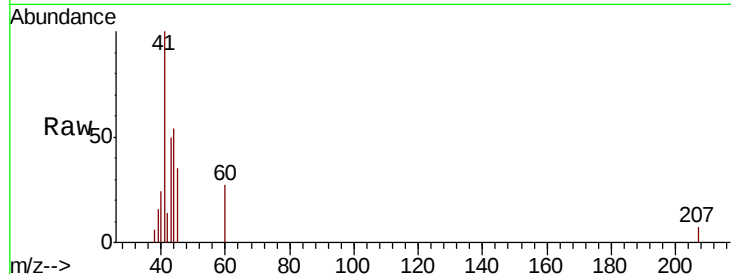

#49
1,4-Dioxane
Concen: 0.817 ug/l
RT: 6.68 min Scan# 1740
Delta R.T. 0.09 min
Lab File: VU034204.D
Acq: 02 Sep 2019 15:59

Tgt Ion: 88 Resp: 114
Ion Ratio Lower Upper
88 100
43 1320670.2 24.8 37.2#
58 7070.2 59.3 88.9#



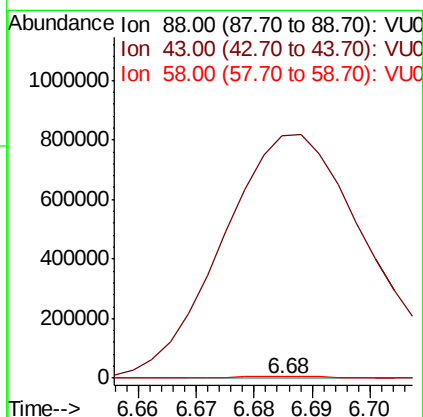



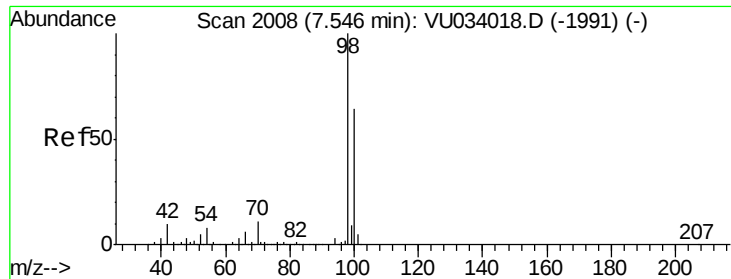

#50
Toluene-d8
Concen: 50.265 ug/l
RT: 7.55 min Scan# 2008
Delta R.T. 0.00 min
Lab File: VU034204.D
Acq: 02 Sep 2019 15:59




Instrument :
MSVOA_U
ClientSampleId :
T16-17-C4-(2.25)


Tgt Ion: 98 Resp: 934752
Ion Ratio Lower Upper
98 100
100 64.1 50.3 75.5

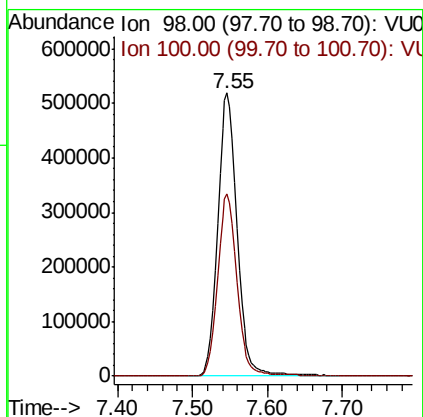

#51
4-Methyl-2-Pentanone
Concen: 9.762 ug/l
RT: 7.40 min Scan# 1963
Delta R.T. -0.04 min
Lab File: VU034204.D
Acq: 02 Sep 2019 15:59

Tgt Ion: 43 Resp: 77791
Ion Ratio Lower Upper
43 100
58 6.8 32.2 48.4#

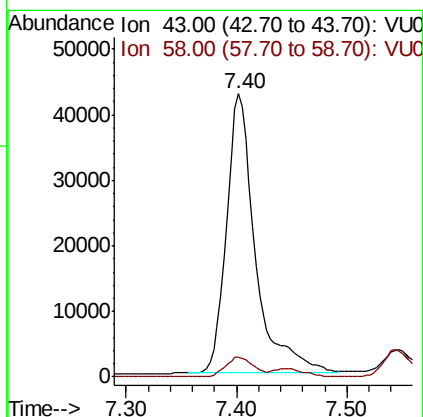







#54

cis-1,3-Dichloropropene
 Concen: 4.265 ug/l
 RT: 7.40 min Scan# 1963
 Delta R.T. 0.15 min
 Lab File: VU034204.D
 Acq: 02 Sep 2019 15:59

Instrument :
 MSVOA_U
 ClientSampleId :
 T16-17-C4-(2.25)




Tgt Ion: 75 Resp: 36765
 Ion Ratio Lower Upper
 75 100
 77 0.6 25.2 37.8#
 39 30.0 34.6 51.8#

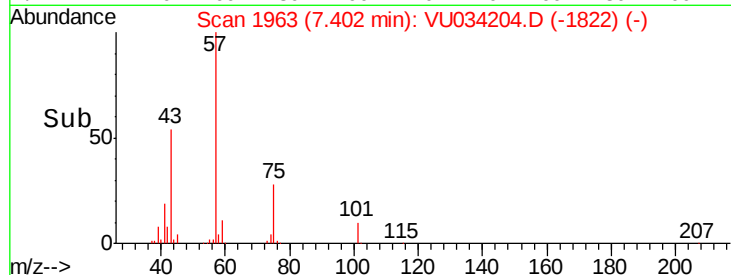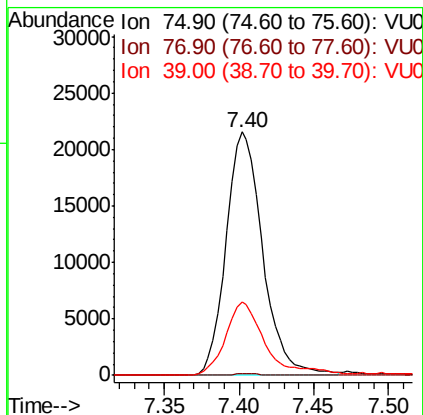


#56

Ethyl methacrylate
 Concen: 0.994 ug/l
 RT: 7.93 min Scan# 2128
 Delta R.T. -0.07 min
 Lab File: VU034204.D
 Acq: 02 Sep 2019 15:59

Tgt Ion: 69 Resp: 203
 Ion Ratio Lower Upper
 69 100
 41 0.0 50.7 76.1#
 39 0.0 24.2 36.2#



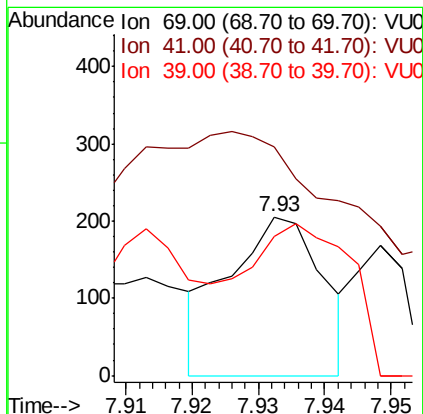



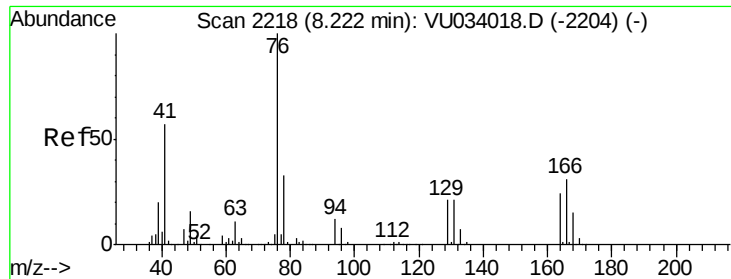

#57
 1,3-Dichloropropane
 Concen: 0.719 ug/l
 RT: 8.40 min Scan# 2273
 Delta R.T. 0.18 min
 Lab File: VU034204.D
 Acq: 02 Sep 2019 15:59




Instrument :
 MSVOA_U
 ClientSampleId :
 T16-17-C4-(2.25)


Tgt Ion: 76 Resp: 6519
 Ion Ratio Lower Upper
 76 100
 78 0.0 26.2 39.4#

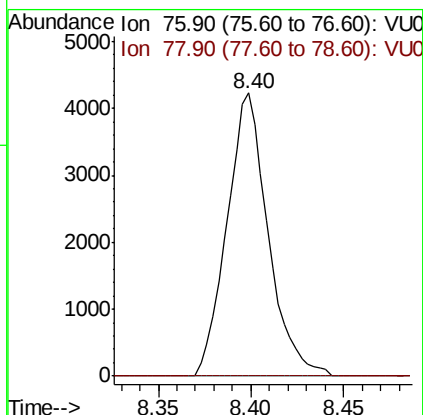

#59
 2-Hexanone
 Concen: 14.255 ug/l
 RT: 8.40 min Scan# 2273
 Delta R.T. 0.05 min
 Lab File: VU034204.D
 Acq: 02 Sep 2019 15:59

Tgt Ion: 43 Resp: 85753
 Ion Ratio Lower Upper
 43 100
 58 21.7 28.4 85.3#

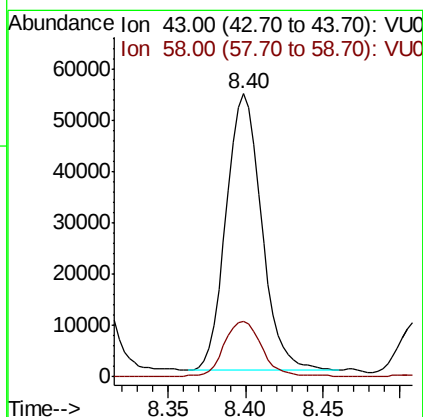



#62

4-Bromofluorobenzene

Concen: 44.757 ug/l

RT: 10.29 min Scan# 2861

Delta R.T. 0.00 min

Lab File: VU034204.D

Acq: 02 Sep 2019 15:59

Instrument :

MSVOA_U

ClientSampleId :

T16-17-C4-(2.25)


Tgt Ion: 95 Resp: 323768

Ion Ratio Lower Upper

95 100

174 85.1 0.0 168.8

176 81.8 0.0 161.8




Abundance Ion 94.90 (94.60 to 95.60): VU034204.D (-2848) (-)

Ion 173.80 (173.50 to 174.50): VU034204.D (-2848) (-)

Ion 175.80 (175.50 to 176.50): VU034204.D (-2848) (-)

Time-->




Abundance

Ion 94.90 (94.60 to 95.60): VU034204.D (-2768) (-)

Ion 173.80 (173.50 to 174.50): VU034204.D (-2768) (-)

Ion 175.80 (175.50 to 176.50): VU034204.D (-2768) (-)

Time-->



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 9.07 min Scan# 2482

Delta R.T. 0.00 min

Lab File: VU034204.D

Acq: 02 Sep 2019 15:59


Tgt Ion: 117 Resp: 715022

Ion Ratio Lower Upper

117 100

82 56.3 45.1 67.7

119 32.5 25.4 38.0




Abundance Ion 116.90 (116.60 to 117.60): VU034204.D (-2468) (-)

Ion 82.00 (81.70 to 82.70): VU034204.D (-2468) (-)

Ion 118.90 (118.60 to 119.60): VU034204.D (-2468) (-)

Time-->




Abundance

Ion 116.90 (116.60 to 117.60): VU034204.D (-2389) (-)

Ion 82.00 (81.70 to 82.70): VU034204.D (-2389) (-)

Ion 118.90 (118.60 to 119.60): VU034204.D (-2389) (-)

Time-->

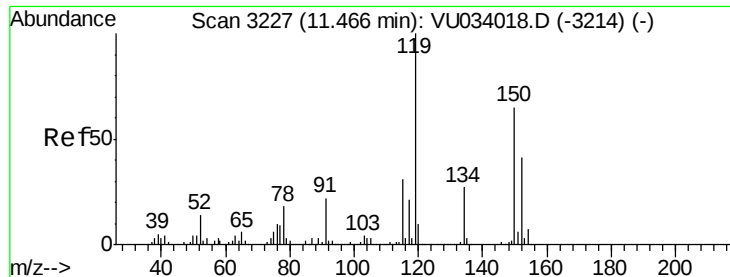

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 11.46 min Scan# 3226

Delta R.T. -0.00 min

Lab File: VU034204.D

Acq: 02 Sep 2019 15:59

Instrument :

MSVOA_U

ClientSampleId :

T16-17-C4-(2.25)


Tgt Ion:152 Resp: 346307

Ion Ratio Lower Upper

152 100

115 56.7 41.1 123.3




150 156.6 0.0 348.8

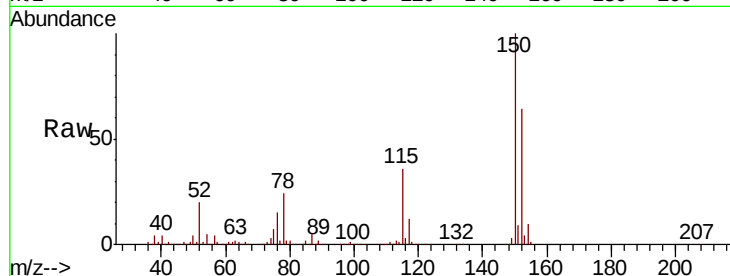

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

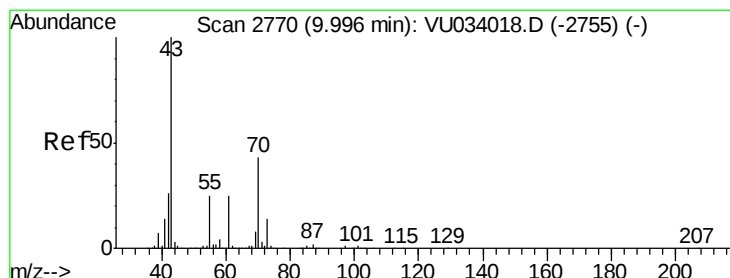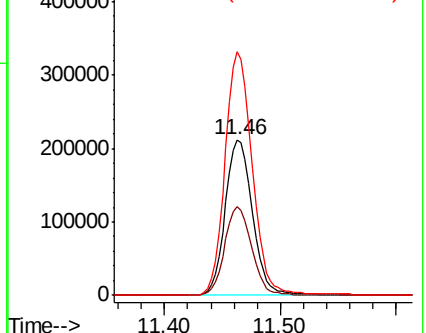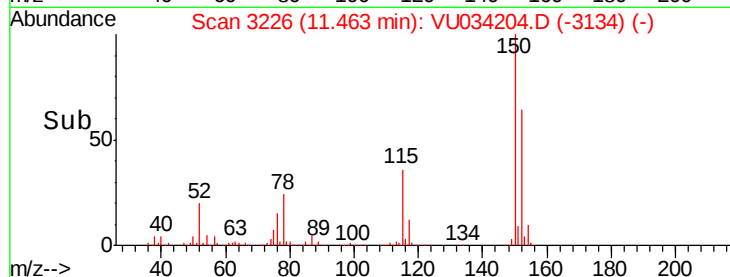

#74

N-ethyl acetate

Concen: 0.275 ug/l

RT: 9.93 min Scan# 2748

Delta R.T. -0.07 min

Lab File: VU034204.D

Acq: 02 Sep 2019 15:59

Tgt Ion: 43 Resp: 2686


Ion Ratio Lower Upper

43 100

70 0.0 35.2 52.8#

55 8.0 20.5 30.7#

61 0.0 20.0 30.0#


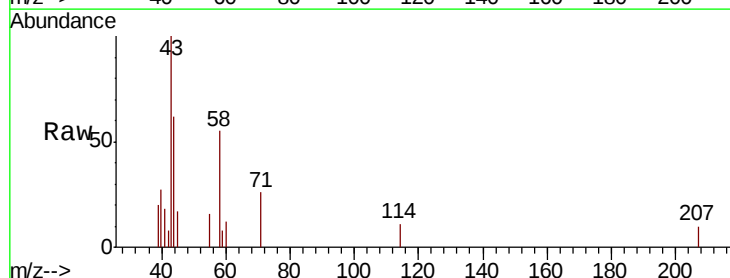



Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 55.00 (54.70 to 55.70): VU0

Ion 61.00 (60.70 to 61.70): VU0

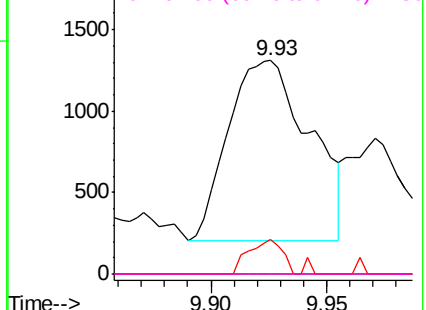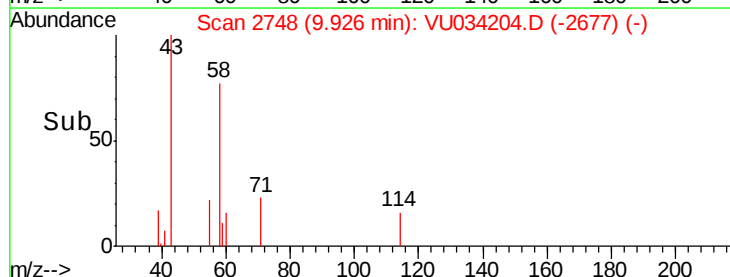

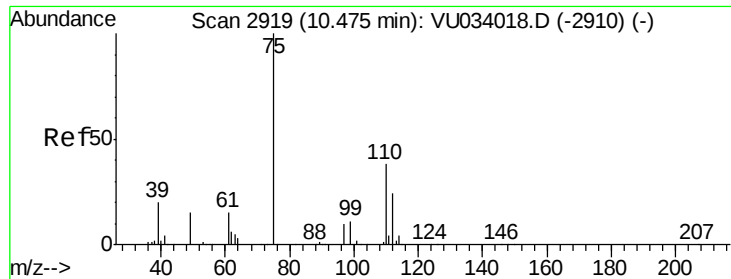

#76

1,2,3-Trichloropropane

Concen: 19.880 ug/l

RT: 10.29 min Scan# 2861

Delta R.T. -0.19 min

Lab File: VU034204.D

Acq: 02 Sep 2019 15:59

Instrument :

MSVOA_U

ClientSampleId :


T16-17-C4-(2.25)

Tgt Ion: 75 Resp: 155169

Ion Ratio Lower Upper




75 100

77 1.3 20.1 60.2#



Abundance Ion 74.90 (74.60 to 75.60): VU0

Ion 77.00 (76.70 to 77.70): VU0

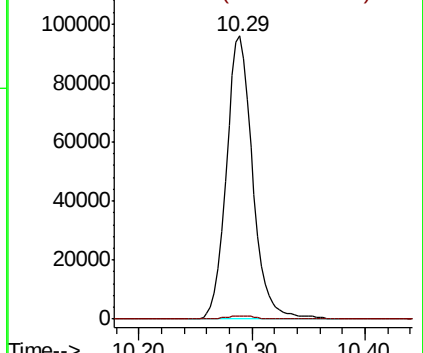

#81

trans-1,4-Dichloro-2-butene

Concen: 66.942 ug/l

RT: 10.29 min Scan# 2861

Delta R.T. -0.21 min

Lab File: VU034204.D

Acq: 02 Sep 2019 15:59


Tgt Ion: 75 Resp: 155169

Ion Ratio Lower Upper

75 100

53 0.2 0.0 0.0#



89 0.0 0.0 0.0




Abundance Ion 74.90 (74.60 to 75.60): VU0

Ion 53.00 (52.70 to 53.70): VU0

Ion 88.90 (88.60 to 89.60): VU0

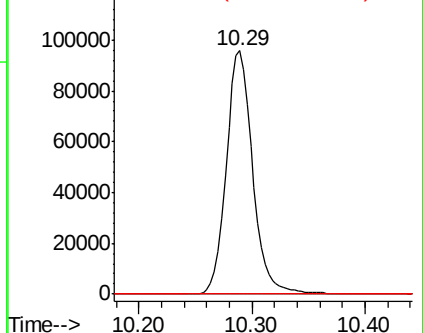

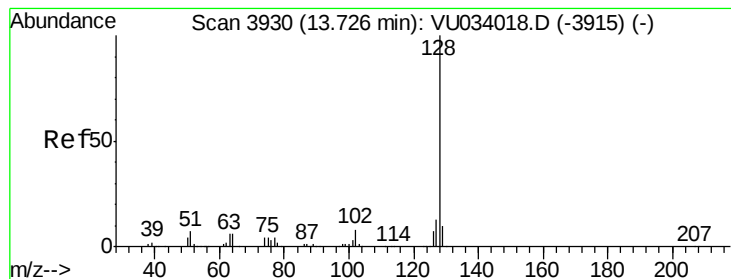

#95

Naphthalene

Concen: 1.792 ug/l

RT: 13.79 min Scan# 3951

Delta R.T. 0.07 min

Lab File: VU034204.D


Acq: 02 Sep 2019 15:59

Instrument :

MSVOA_U

ClientSampleId :

T16-17-C4-(2.25)

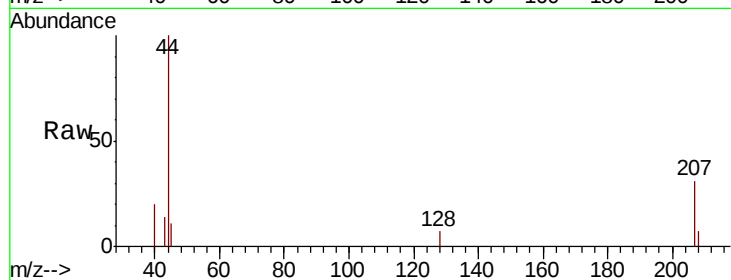


Tgt Ion:128 Resp: 45

Ion Ratio Lower Upper

128 100

127 0.0 10.2 15.4#

129 0.0 8.4 12.6#

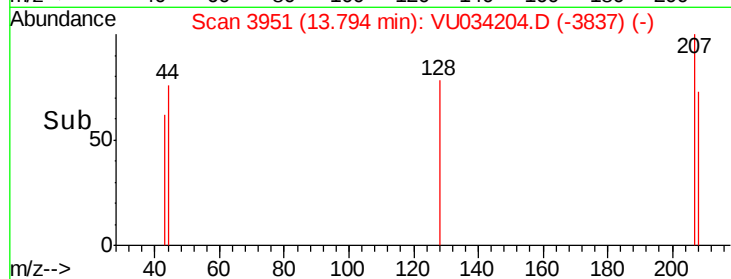

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

