

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090320\
 Data File : VU040029.D
 Acq On : 03 Sep 2020 11:09
 Operator : SY/MD
 Sample : VV0903WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK01

Quant Time: Sep 04 03:12:16 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 04 02:55:57 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	110994	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	110429	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	48518	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	28488	4.70	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.00%
7) Chloroethane-d5	1.92	69	26199	5.19	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.80%
11) 1,1-Dichloroethene-d2	2.58	63	50506	3.25	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.00%
20) 2-Butanone-d5	4.65	46	131240	54.14	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.28%
24) Chloroform-d	5.08	84	70560	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.60%
26) 1,2-Dichloroethane-d4	5.72	65	44967	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.00%
32) Benzene-d6	5.74	84	130373	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.20%
36) 1,2-Dichloropropane-d6	6.70	67	43870	5.16	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.20%
41) Toluene-d8	7.91	98	108321	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.00%
43) trans-1,3-Dichloropropene-	8.19	79	17744	4.55	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.00%
46) 2-Hexanone-d5	8.64	63	94577	51.15	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.30%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	38255	5.21	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.20%
64) 1,2-Dichlorobenzene-d4	12.19	152	41421	5.28	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.60%


Target Compounds					Ovalue
16) Methylene chloride	3.06	84	2418	0.215 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU090320\
Data File : VU040029.D
Acq On : 03 Sep 2020 11:09
Operator : SY/MD
Sample : VV0903WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK01

Quant Time: Sep 04 03:12:16 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 04 02:55:57 2020
Response via : Initial Calibration

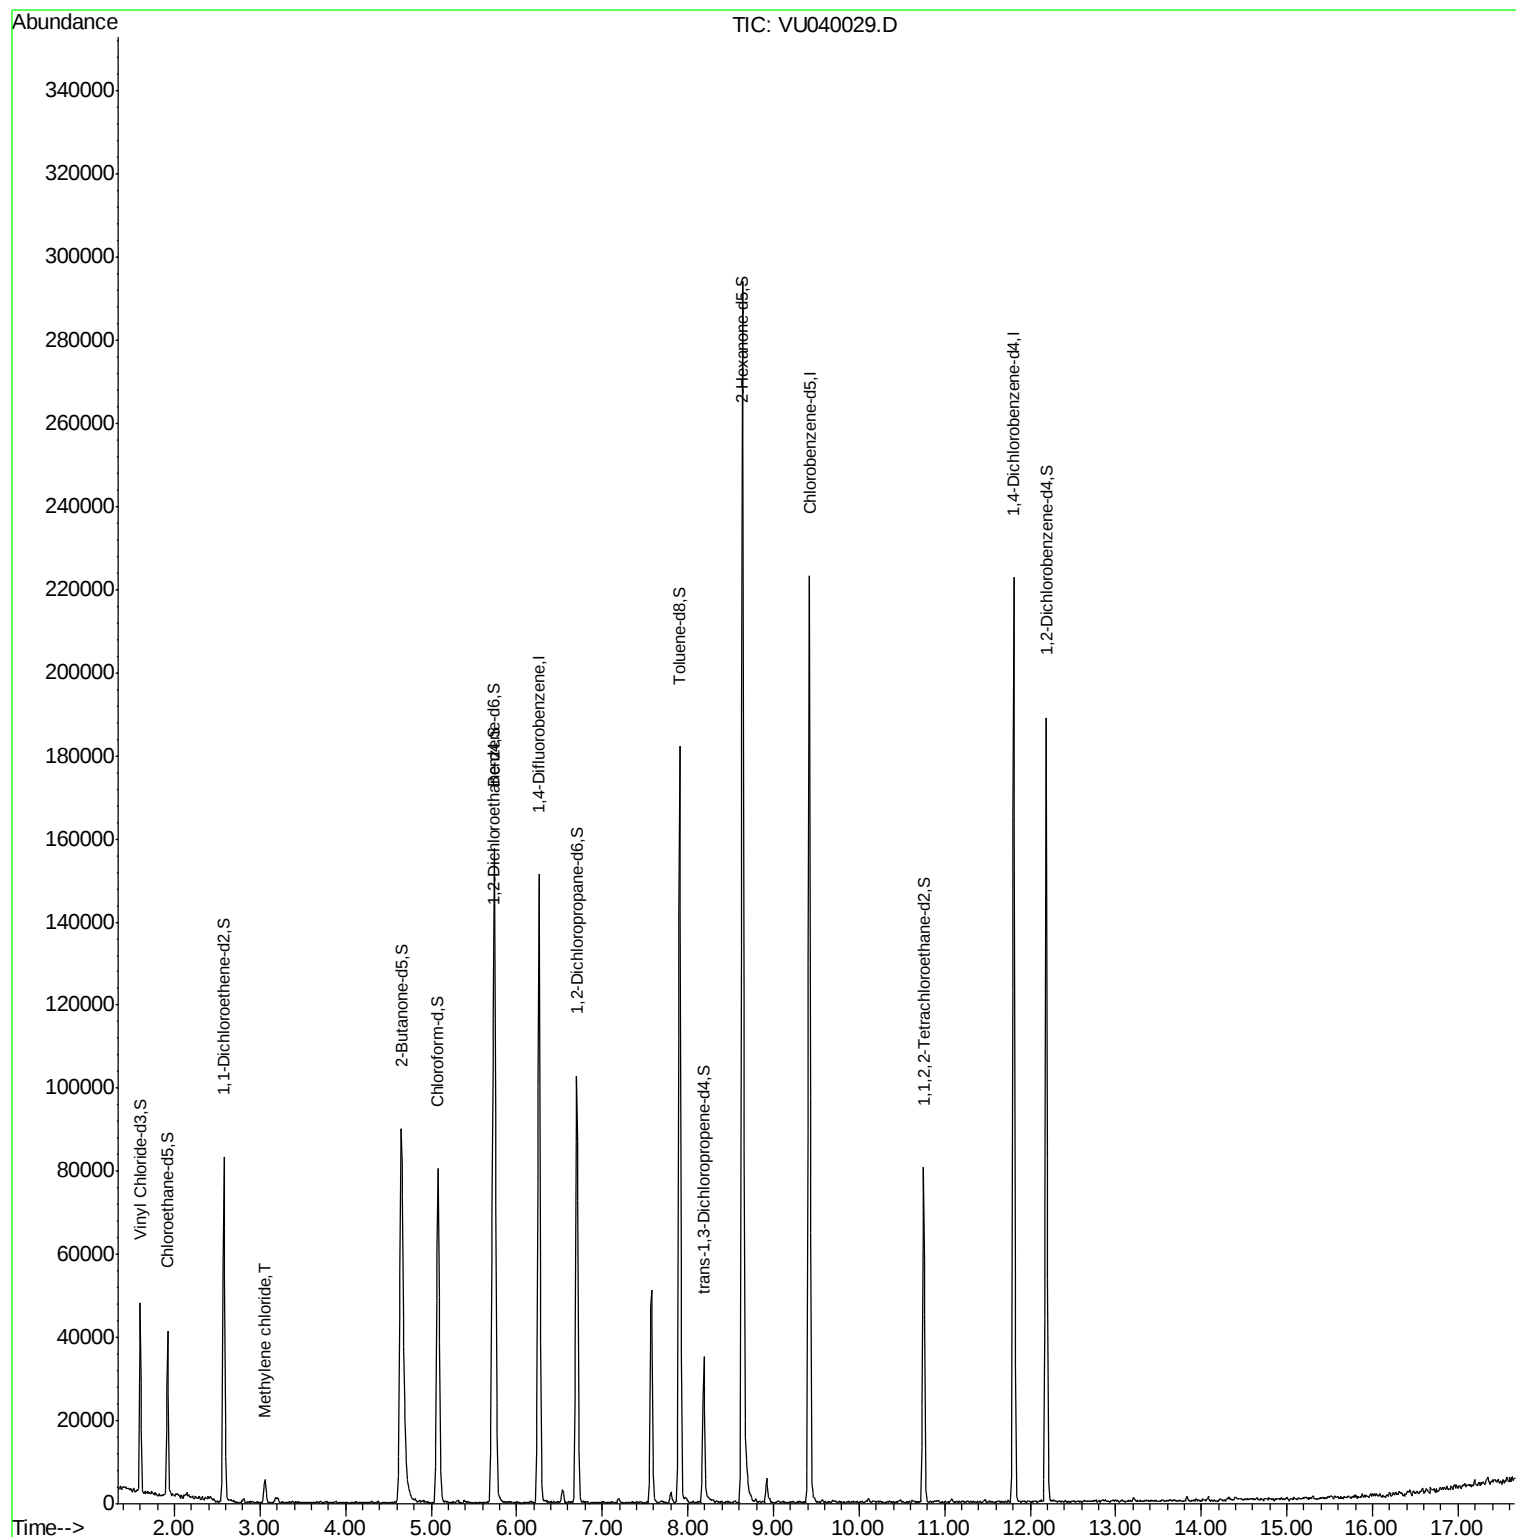

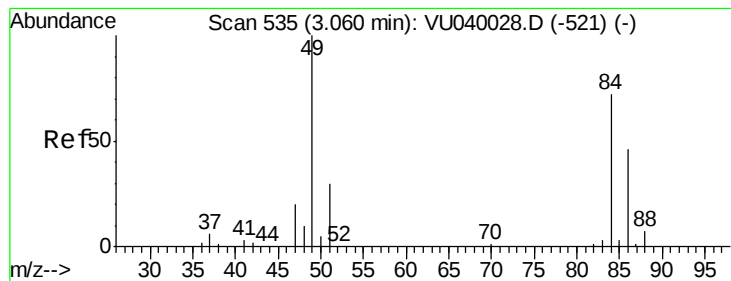

#16
Methylene chloride
Concen: 0.215 ug/L
RT: 3.06 min Scan# 534
Delta R.T. -0.00 min
Lab File: VU040029.D
Acq: 03 Sep 2020 11:09

Instrument :
MSVOA_U
ClientSampleId :
VBLK01

Tot Ion: 84 Resp: 2418

Ion	Ratio	Lower	Upper
84	100		
86	54.9	45.2	84.0
49	133.2	104.0	193.2

