

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090320\
 Data File : VU040031.D
 Acq On : 03 Sep 2020 14:21
 Operator : SY/MD
 Sample : L3891-03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW289

Quant Time: Sep 04 03:18:43 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 04 02:55:57 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	121949	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	119736	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	53285	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	28649	4.30	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.00%
7) Chloroethane-d5	1.92	69	25498	4.60	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.00%
11) 1,1-Dichloroethene-d2	2.58	63	50542	2.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.20%#
20) 2-Butanone-d5	4.64	46	128144	48.12	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.24%
24) Chloroform-d	5.08	84	68964	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.60%
26) 1,2-Dichloroethane-d4	5.72	65	44713	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.20%
32) Benzene-d6	5.74	84	126891	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.80%
36) 1,2-Dichloropropane-d6	6.70	67	41751	4.53	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.60%
41) Toluene-d8	7.91	98	105632	4.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.60%
43) trans-1,3-Dichloropropene-	8.19	79	17452	4.12	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.40%
46) 2-Hexanone-d5	8.64	63	92957	46.36	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.72%
57) 1,1,2,2-Tetrachloroethane-	10.76	84	38395	4.82	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.40%
64) 1,2-Dichlorobenzene-d4	12.19	152	43780	5.08	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.60%


Target Compounds					Ovalue
13) Acetone	2.64	43	2970	1.205 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090320\
Data File : VU040031.D
Acq On : 03 Sep 2020 14:21
Operator : SY/MD
Sample : L3891-03
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW289

Quant Time: Sep 04 03:18:43 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 04 02:55:57 2020
Response via : Initial Calibration

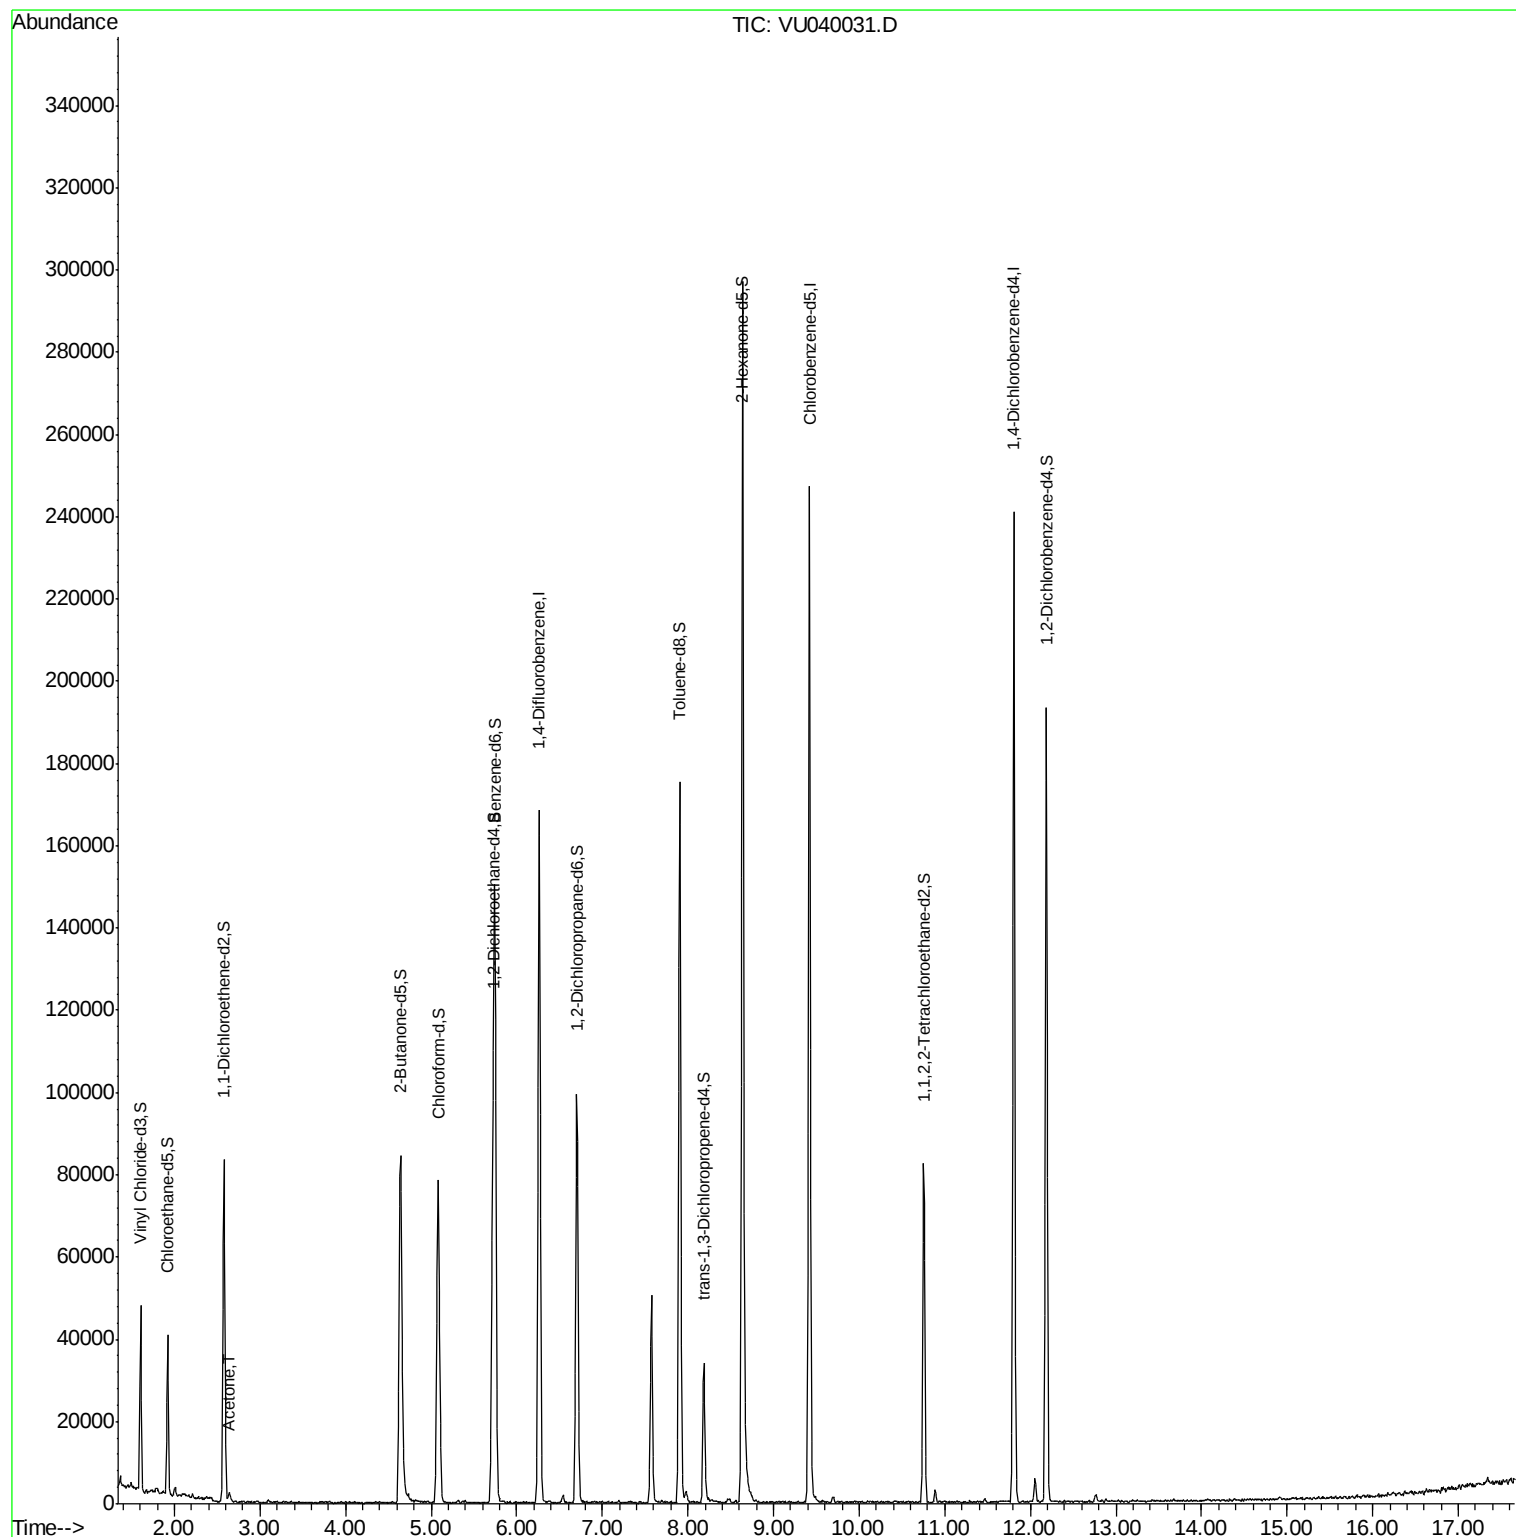

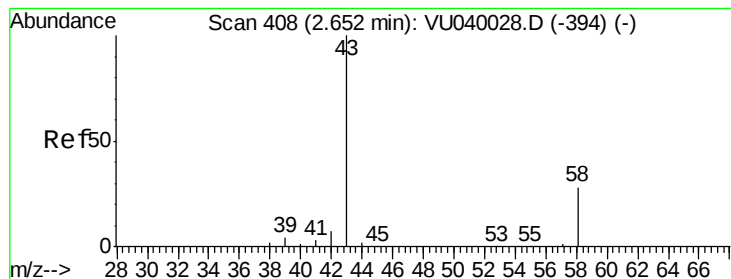

#13
 Acetone
 Concen: 1.205 ug/L
 RT: 2.64 min Scan# 405
 Delta R.T. -0.01 min
 Lab File: VU040031.D
 Acq: 03 Sep 2020 14:21

Instrument :
 MSVOA_U
 ClientSampleId :
 EW289

Tot Ion: 43 Resp: 2970
 Ion Ratio Lower Upper
 43 100
 58 27.3 0.0 55.4

