

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050608.D
 Acq On : 03 Sep 2022 13:39
 Operator : SY/MD
 Sample : N4399-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVJ6

Quant Time: Sep 05 01:06:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Sep 05 01:05:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	291287	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	283232	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	106395	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	97972	39.324	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	78.640%	
7) Chloroethane-d5	1.906	69	78993	46.886	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	93.780%	
11) 1,1-Dichloroethene-d2	2.562	63	134743	30.605	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	61.200%	
21) 2-Butanone-d5	4.629	46	191438	105.025	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	105.020%	
24) Chloroform-d	5.063	84	231503	49.027	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	98.060%	
26) 1,2-Dichloroethane-d4	5.700	65	152791	52.952	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	105.900%	
32) Benzene-d6	5.726	84	462889	49.454	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	98.900%	
36) 1,2-Dichloropropane-d6	6.690	67	160307	52.166	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	104.340%	
41) Toluene-d8	7.899	98	370031	46.230	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	92.460%	
43) trans-1,3-Dichloroprop...	8.179	79	56639	44.545	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	89.100%	
47) 2-Hexanone-d5	8.636	63	73851	95.540	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	95.540%	
56) 1,1,2,2-Tetrachloroeth...	10.754	84	239412	51.482	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	102.960%	
66) 1,2-Dichlorobenzene-d4	12.192	152	126355	50.732	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	101.460%	
Target Compounds						
13) Acetone	2.639	43	8849	6.436	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050608.D
Acq On : 03 Sep 2022 13:39
Operator : SY/MD
Sample : N4399-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVJ6

Quant Time: Sep 05 01:06:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Sep 05 01:05:15 2022
Response via : Initial Calibration

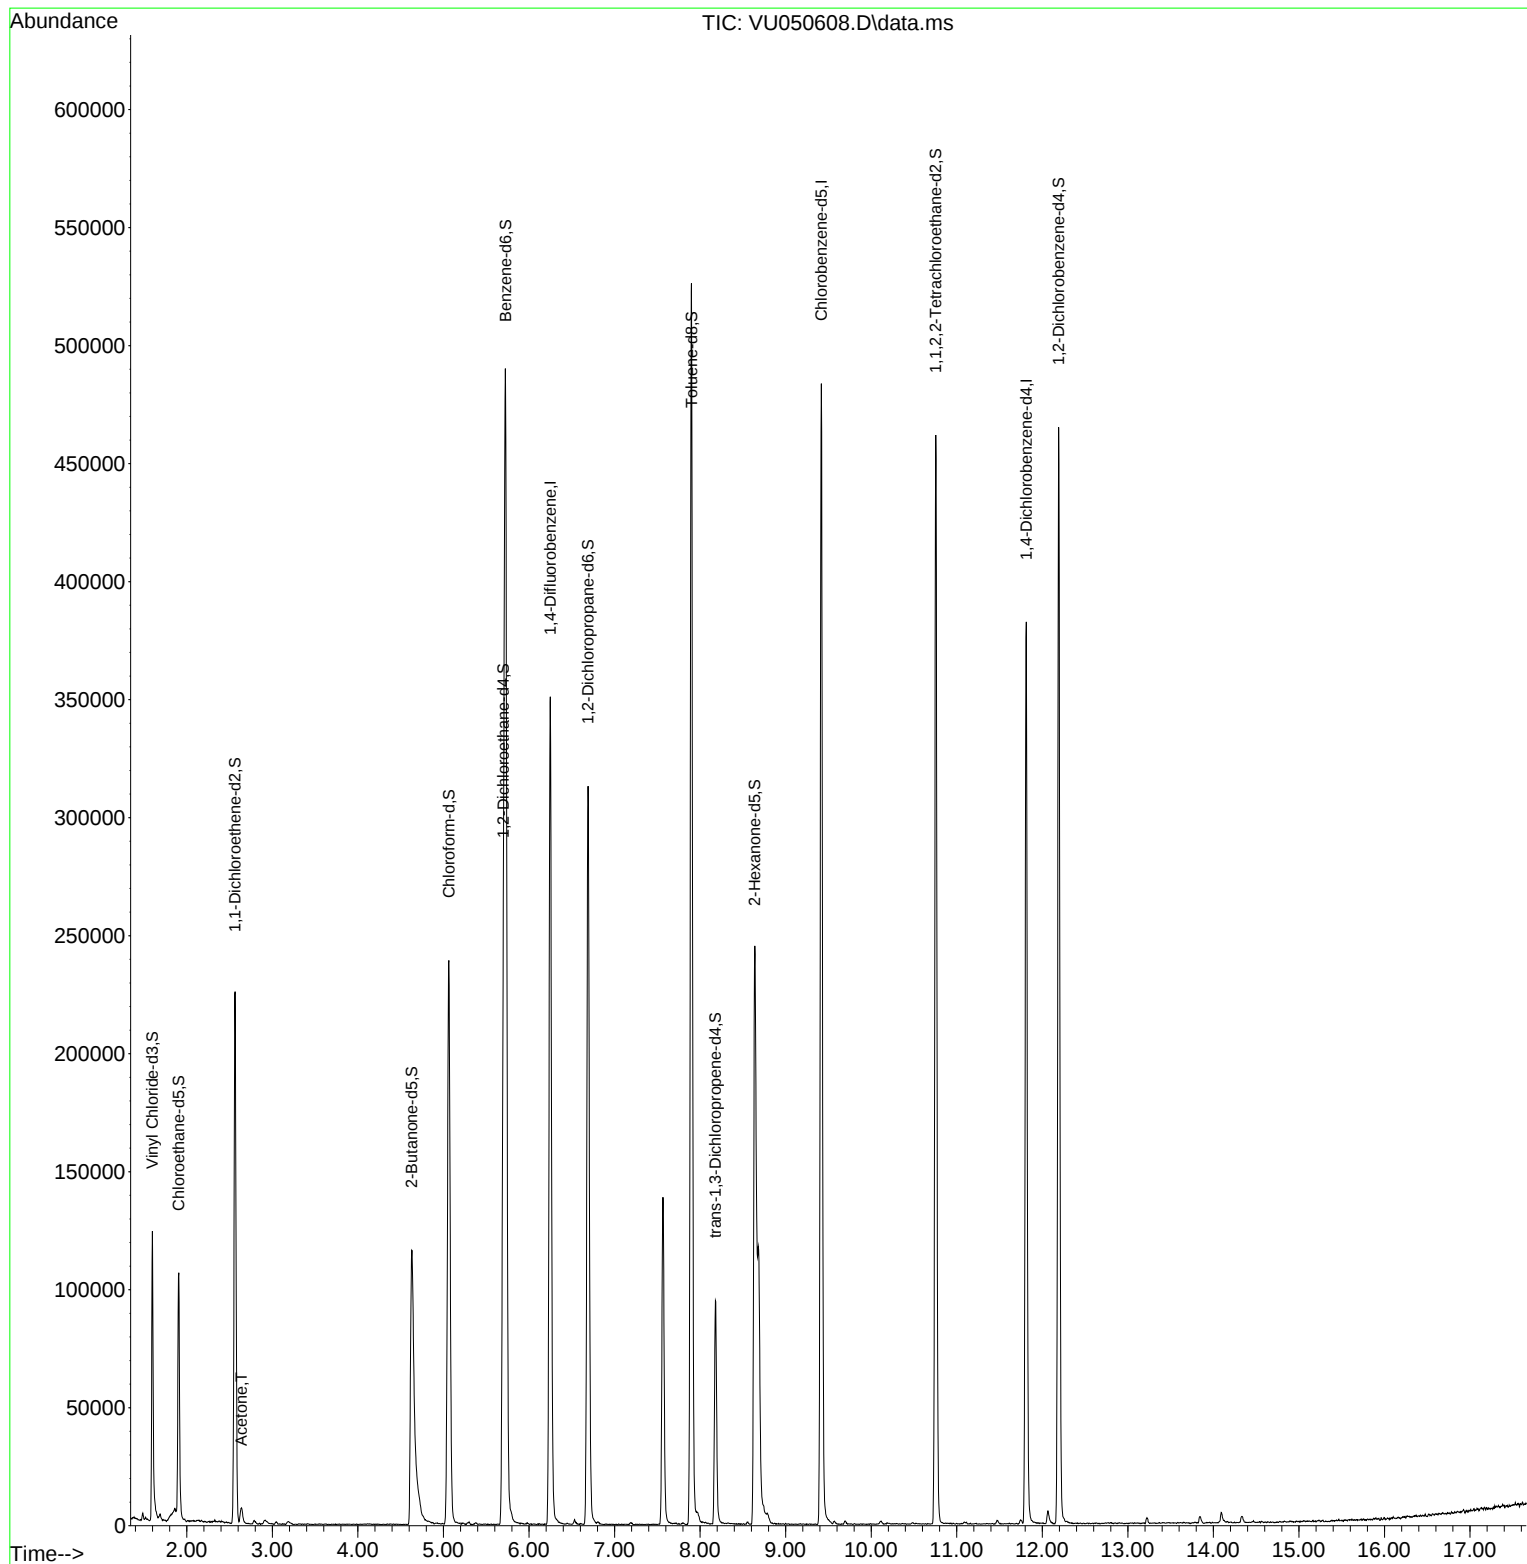

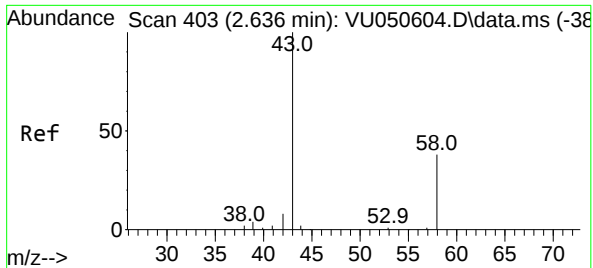

#13
 Acetone
 Concen: 6.436 ug/L
 RT: 2.639 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU050608.D
 Acq: 03 Sep 2022 13:39

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVJ6

Tgt Ion: 43 Resp: 8849
 Ion Ratio Lower Upper
 43 100
 58 38.6 0.0 76.2

