

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050606.D
 Acq On : 03 Sep 2022 12:52
 Operator : SY/MD
 Sample : VU0903WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK180

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050606.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	105	rBV	131142	164167	12.97%	1.878%
2	1.906	168	176	194	rVB	105787	139558	11.02%	1.596%
3	2.565	369	381	397	rBV	251596	403659	31.89%	4.618%
4	2.899	482	485	487	rBV2	219	170	0.01%	0.002%
5	3.002	514	517	519	rVB	133	63	0.00%	0.001%
6	3.044	519	530	539	rBV3	1947	3513	0.28%	0.040%
7	3.182	559	573	588	rBV3	4953	11747	0.93%	0.134%
8	3.259	594	597	602	rVB2	173	144	0.01%	0.002%
9	3.292	605	607	610	rVB2	255	136	0.01%	0.002%
10	3.472	660	663	666	rBV	184	131	0.01%	0.001%
11	3.639	713	715	718	rBV	175	122	0.01%	0.001%
12	3.729	736	743	745	rBV	240	285	0.02%	0.003%
13	3.822	766	772	776	rBV2	273	334	0.03%	0.004%
14	4.070	846	849	851	rBV2	103	48	0.00%	0.001%
15	4.112	858	862	865	rBV2	160	135	0.01%	0.002%
16	4.128	865	867	874	rVB2	219	205	0.02%	0.002%
17	4.185	883	885	887	rBV	144	85	0.01%	0.001%
18	4.227	892	898	902	rBV2	210	198	0.02%	0.002%
19	4.259	902	908	913	rBV2	272	389	0.03%	0.004%
20	4.285	913	916	919	rVB2	201	120	0.01%	0.001%
21	4.404	950	953	954	rBV	155	89	0.01%	0.001%
22	4.558	995	1001	1002	rBV	223	206	0.02%	0.002%
23	4.629	1010	1023	1070	rBV	107303	344497	27.21%	3.941%
24	5.063	1141	1158	1179	rBV	225267	495744	39.16%	5.671%
25	5.211	1202	1204	1206	rBV2	213	113	0.01%	0.001%
26	5.227	1206	1209	1211	rVV3	443	234	0.02%	0.003%
27	5.275	1219	1224	1226	rBV2	657	624	0.05%	0.007%
28	5.340	1242	1244	1247	rBV2	196	150	0.01%	0.002%
29	5.369	1250	1253	1257	rVV3	409	332	0.03%	0.004%
30	5.391	1258	1260	1262	rVB2	206	84	0.01%	0.001%
31	5.436	1270	1274	1278	rBV2	187	184	0.01%	0.002%
32	5.459	1278	1281	1285	rVB2	149	88	0.01%	0.001%
33	5.484	1285	1289	1291	rBV2	124	99	0.01%	0.001%
34	5.539	1303	1306	1310	rVB	271	177	0.01%	0.002%
35	5.562	1310	1313	1317	rBV2	170	152	0.01%	0.002%
36	5.616	1325	1330	1332	rBV	267	203	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050606.D
 Acq On : 03 Sep 2022 12:52
 Operator : SY/MD
 Sample : VU0903WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK180

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	5.726	1342	1364	1397	rBV2	466815	1265927	100.00%	14.482%
38	6.021	1454	1456	1460	rVB2	244	182	0.01%	0.002%
39	6.044	1460	1463	1465	rBV2	277	225	0.02%	0.003%
40	6.076	1470	1473	1478	rVV3	198	152	0.01%	0.002%
41	6.105	1480	1482	1483	rBV3	156	43	0.00%	0.000%
42	6.176	1499	1504	1505	rBV	154	126	0.01%	0.001%
43	6.250	1511	1527	1546	rBV	334833	645971	51.03%	7.390%
44	6.536	1606	1616	1626	rVB6	1895	3320	0.26%	0.038%
45	6.578	1626	1629	1632	rBV2	274	176	0.01%	0.002%
46	6.690	1650	1664	1688	rBV	288915	570290	45.05%	6.524%
47	6.941	1738	1742	1746	rVB2	136	125	0.01%	0.001%
48	6.980	1746	1754	1757	rBV2	192	213	0.02%	0.002%
49	6.996	1757	1759	1764	rVB2	177	133	0.01%	0.002%
50	7.021	1764	1767	1769	rBV	191	142	0.01%	0.002%
51	7.054	1773	1777	1779	rBV2	112	94	0.01%	0.001%
52	7.092	1787	1789	1792	rVB2	119	61	0.00%	0.001%
53	7.111	1792	1795	1800	rVB	187	160	0.01%	0.002%
54	7.144	1800	1805	1808	rBV2	122	101	0.01%	0.001%
55	7.185	1813	1818	1819	rBV2	523	431	0.03%	0.005%
56	7.243	1834	1836	1840	rBV2	217	121	0.01%	0.001%
57	7.343	1863	1867	1872	rVB2	277	252	0.02%	0.003%
58	7.372	1872	1876	1879	rBV2	167	156	0.01%	0.002%
59	7.423	1889	1892	1893	rBV	177	84	0.01%	0.001%
60	7.565	1917	1936	1954	rBV	127222	228366	18.04%	2.612%
61	7.799	2001	2009	2018	rBV4	1182	1599	0.13%	0.018%
62	7.899	2025	2040	2072	rBV	545645	956734	75.58%	10.945%
63	8.121	2107	2109	2114	rBV	227	126	0.01%	0.001%
64	8.179	2116	2127	2145	rVV	84993	147689	11.67%	1.689%
65	8.439	2205	2208	2211	rBV	169	116	0.01%	0.001%
66	8.481	2215	2221	2222	rBV2	275	206	0.02%	0.002%
67	8.574	2247	2250	2251	rBV	127	63	0.00%	0.001%
68	8.587	2251	2254	2256	rBV2	159	89	0.01%	0.001%
69	8.639	2258	2270	2280	rBV3	212980	468145	36.98%	5.355%
70	8.870	2340	2342	2346	rBV3	282	149	0.01%	0.002%
71	9.044	2393	2396	2399	rVB	127	89	0.01%	0.001%
72	9.063	2399	2402	2405	rBV2	208	161	0.01%	0.002%
73	9.417	2498	2512	2537	rBV	461115	784546	61.97%	8.975%
74	9.693	2594	2598	2601	rBV2	353	311	0.02%	0.004%
75	9.832	2638	2641	2642	rBV	158	105	0.01%	0.001%
76	9.912	2664	2666	2669	rVB	171	83	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050606.D
 Acq On : 03 Sep 2022 12:52
 Operator : SY/MD
 Sample : VU0903WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK180

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M

Title : VOC Analysis

77	9.931	2669	2672	2674	rBV	175	135	0.01%	0.002%
78	10.053	2706	2710	2712	rBV2	210	152	0.01%	0.002%
79	10.069	2712	2715	2718	rVV2	219	151	0.01%	0.002%
80	10.118	2727	2730	2737	rVB3	805	780	0.06%	0.009%
81	10.185	2748	2751	2753	rBV2	176	92	0.01%	0.001%
82	10.430	2824	2827	2829	rBV	194	127	0.01%	0.001%
83	10.484	2839	2844	2849	rBV4	494	684	0.05%	0.008%
84	10.754	2915	2928	2955	rBV	415026	669728	52.90%	7.661%
85	11.076	3025	3028	3030	rBV	275	203	0.02%	0.002%
86	11.195	3062	3065	3069	rBV2	367	307	0.02%	0.004%
87	11.340	3106	3110	3111	rBV	145	120	0.01%	0.001%
88	11.404	3127	3130	3133	rBV	229	172	0.01%	0.002%
89	11.812	3244	3257	3284	rBV	390949	633386	50.03%	7.246%
90	12.192	3363	3375	3410	rBV	467022	765321	60.46%	8.755%
91	12.500	3468	3471	3473	rBV	336	203	0.02%	0.002%
92	12.722	3537	3540	3543	rBV2	446	258	0.02%	0.003%
93	14.092	3958	3966	3980	rBV	8725	15937	1.26%	0.182%
94	14.333	4034	4041	4053	rVB6	5486	8673	0.69%	0.099%




Sum of corrected areas: 8741676

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050606.D
Acq On : 03 Sep 2022 12:52
Operator : SY/MD
Sample : VU0903WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK180

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

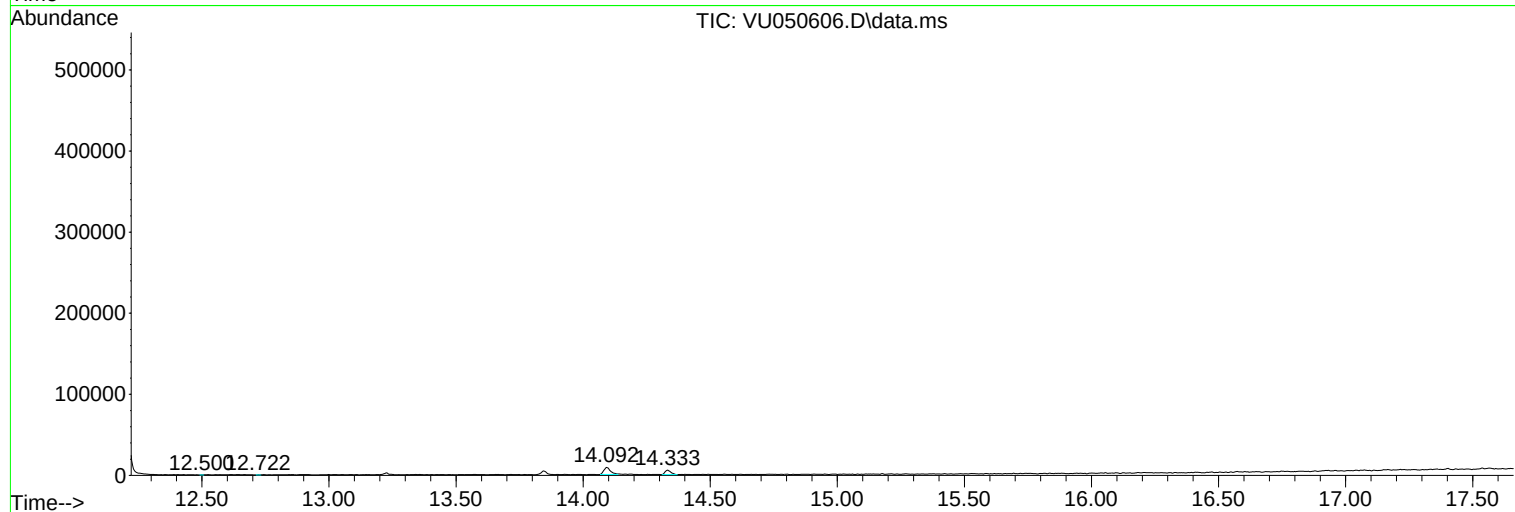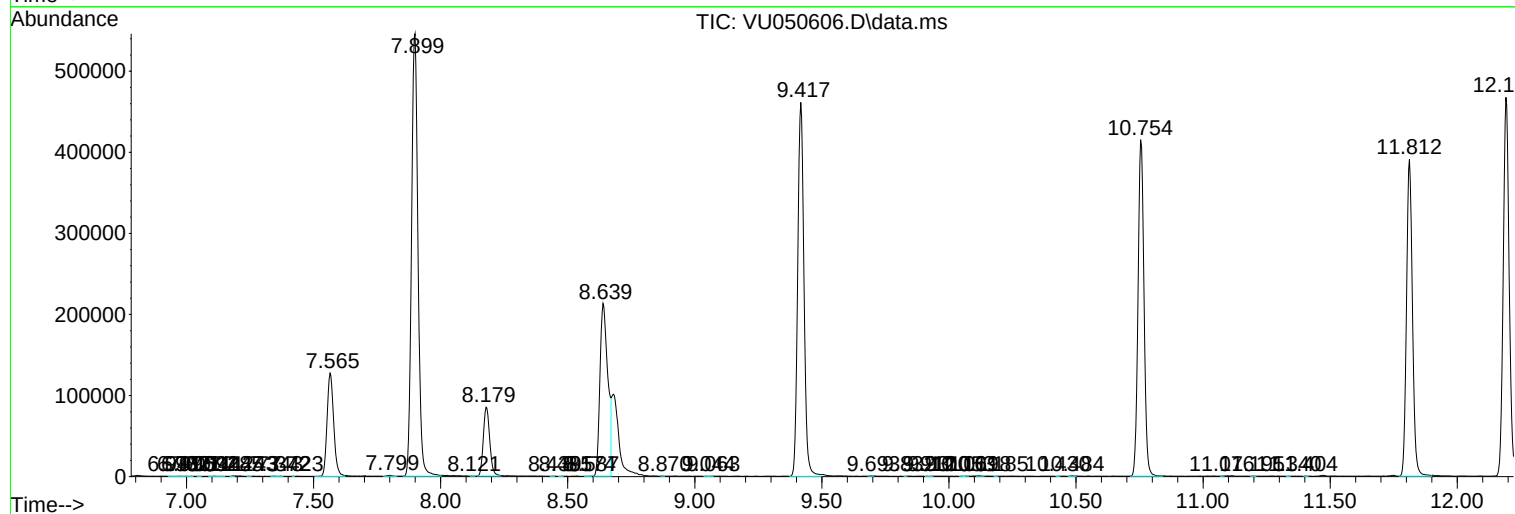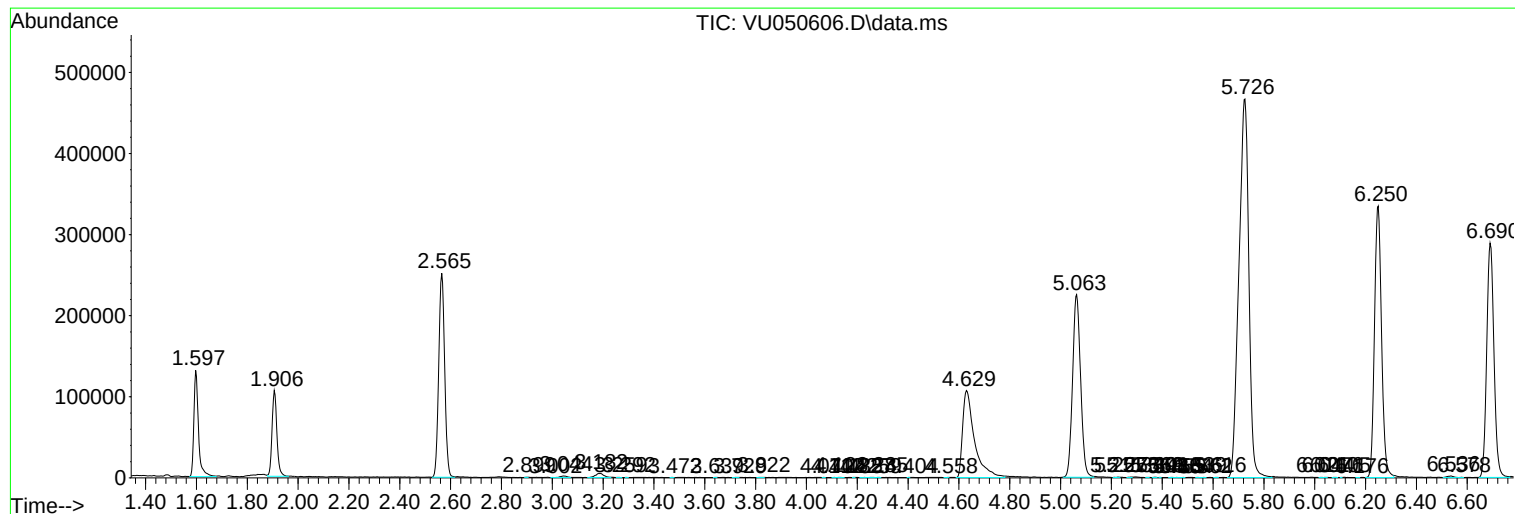

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050606.D
Acq On : 03 Sep 2022 12:52
Operator : SY/MD
Sample : VU0903WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK180

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050606.D
Acq On : 03 Sep 2022 12:52
Operator : SY/MD
Sample : VU0903WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK180

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc