

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050608.D
 Acq On : 03 Sep 2022 13:39
 Operator : SY/MD
 Sample : N4399-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050608.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	51	rVB2	2694	2477	0.18%	0.027%
2	1.597	72	80	101	rBV	122497	152384	11.36%	1.659%
3	1.906	168	176	192	rVB	104412	141687	10.56%	1.543%
4	2.282	291	293	297	rVB3	539	363	0.03%	0.004%
5	2.301	297	299	304	rBV3	560	546	0.04%	0.006%
6	2.565	367	381	395	rBV	225317	367539	27.40%	4.001%
7	2.639	395	404	421	rVB	6683	14313	1.07%	0.156%
8	2.787	444	450	454	rBV4	1357	1722	0.13%	0.019%
9	2.851	468	470	473	rVB	456	278	0.02%	0.003%
10	2.877	473	478	479	rBV	262	191	0.01%	0.002%
11	2.916	479	490	497	rBV3	1672	3543	0.26%	0.039%
12	3.047	523	531	537	rBV3	1061	1680	0.13%	0.018%
13	3.118	549	553	556	rBV2	274	191	0.01%	0.002%
14	3.137	556	559	563	rVB	293	180	0.01%	0.002%
15	3.186	565	574	586	rBV4	1210	3029	0.23%	0.033%
16	3.308	608	612	617	rBV	245	301	0.02%	0.003%
17	3.407	640	643	646	rBV	293	217	0.02%	0.002%
18	3.498	664	671	674	rBV2	268	268	0.02%	0.003%
19	3.944	805	810	813	rBV2	245	225	0.02%	0.002%
20	4.063	843	847	850	rBV2	185	195	0.01%	0.002%
21	4.115	857	863	867	rBV2	212	277	0.02%	0.003%
22	4.629	1010	1023	1071	rBV2	116117	384160	28.64%	4.182%
23	4.909	1104	1110	1111	rBV3	374	336	0.03%	0.004%
24	4.986	1130	1134	1137	rBV2	287	225	0.02%	0.002%
25	5.063	1142	1158	1182	rBV	238808	528120	39.38%	5.750%
26	5.218	1202	1206	1207	rBV2	635	356	0.03%	0.004%
27	5.282	1221	1226	1228	rBV3	676	669	0.05%	0.007%
28	5.356	1244	1249	1250	rBV	288	224	0.02%	0.002%
29	5.382	1250	1257	1263	rVB4	722	1133	0.08%	0.012%
30	5.423	1263	1270	1273	rBV2	230	281	0.02%	0.003%
31	5.494	1289	1292	1297	rVB2	301	244	0.02%	0.003%
32	5.517	1297	1299	1304	rVB2	259	189	0.01%	0.002%
33	5.632	1331	1335	1342	rBV2	186	256	0.02%	0.003%
34	5.723	1342	1363	1399	rBV2	489725	1341182	100.00%	14.602%
35	5.980	1440	1443	1445	rVV2	454	258	0.02%	0.003%
36	6.047	1460	1464	1468	rBV3	216	244	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050608.D
 Acq On : 03 Sep 2022 13:39
 Operator : SY/MD
 Sample : N4399-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	6.121	1484	1487	1490	rVB	317	211	0.02%	0.002%
38	6.160	1496	1499	1503	rVB2	299	294	0.02%	0.003%
39	6.182	1503	1506	1507	rBV	385	187	0.01%	0.002%
40	6.250	1511	1527	1549	rBV	350693	674085	50.26%	7.339%
41	6.446	1585	1588	1594	rVB2	368	316	0.02%	0.003%
42	6.533	1605	1615	1619	rBV5	1951	2337	0.17%	0.025%
43	6.690	1649	1664	1691	rBV	312738	619581	46.20%	6.746%
44	6.803	1695	1699	1700	rBV3	575	431	0.03%	0.005%
45	7.018	1763	1766	1771	rVB2	300	267	0.02%	0.003%
46	7.047	1771	1775	1781	rBV2	350	420	0.03%	0.005%
47	7.115	1792	1796	1798	rBV2	230	239	0.02%	0.003%
48	7.192	1812	1820	1823	rBV5	926	1226	0.09%	0.013%
49	7.523	1916	1923	1924	rBV2	202	214	0.02%	0.002%
50	7.565	1924	1936	1958	rBV	138538	252679	18.84%	2.751%
51	7.790	2001	2006	2007	rBV	411	297	0.02%	0.003%
52	7.803	2007	2010	2013	rVB	388	240	0.02%	0.003%
53	7.899	2026	2040	2057	rBV	525703	940012	70.09%	10.234%
54	8.028	2078	2080	2088	rVB3	499	527	0.04%	0.006%
55	8.179	2116	2127	2147	rBV	94624	163705	12.21%	1.782%
56	8.324	2168	2172	2173	rBV2	283	188	0.01%	0.002%
57	8.420	2200	2202	2205	rVB2	335	201	0.01%	0.002%
58	8.478	2217	2220	2224	rBV2	361	269	0.02%	0.003%
59	8.510	2224	2230	2232	rVB3	308	252	0.02%	0.003%
60	8.549	2239	2242	2243	rBV2	835	471	0.04%	0.005%
61	8.639	2257	2270	2280	rBV4	245074	546802	40.77%	5.953%
62	8.870	2340	2342	2346	rVB3	395	251	0.02%	0.003%
63	8.999	2378	2382	2387	rBV2	473	378	0.03%	0.004%
64	9.250	2457	2460	2465	rVB	208	188	0.01%	0.002%
65	9.282	2465	2470	2473	rBV2	239	237	0.02%	0.003%
66	9.417	2498	2512	2537	rBV	483328	829398	61.84%	9.030%
67	9.568	2553	2559	2565	rBV5	1122	1559	0.12%	0.017%
68	9.690	2592	2597	2598	rBV	1231	860	0.06%	0.009%
69	9.806	2627	2633	2638	rBV2	295	317	0.02%	0.003%
70	9.880	2651	2656	2660	rVB2	248	248	0.02%	0.003%
71	9.906	2660	2664	2666	rBV2	277	187	0.01%	0.002%
72	9.992	2687	2691	2694	rBV	347	272	0.02%	0.003%
73	10.118	2718	2730	2737	rVB6	1216	2290	0.17%	0.025%
74	10.185	2748	2751	2754	rBV	578	464	0.03%	0.005%
75	10.298	2783	2786	2793	rVB2	264	270	0.02%	0.003%
76	10.478	2836	2842	2843	rBV2	563	446	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050608.D
 Acq On : 03 Sep 2022 13:39
 Operator : SY/MD
 Sample : N4399-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

77	10.661	2896	2899	2904	rBV2	260	233	0.02%	0.003%
78	10.754	2915	2928	2951	rBV	461322	754142	56.23%	8.211%
79	10.957	2989	2991	3000	rVB	340	336	0.03%	0.004%
80	10.999	3000	3004	3007	rBV	270	228	0.02%	0.002%
81	11.089	3028	3032	3035	rBV	549	502	0.04%	0.005%
82	11.160	3051	3054	3057	rVB	409	251	0.02%	0.003%
83	11.471	3143	3151	3162	rVV5	1621	2903	0.22%	0.032%
84	11.748	3227	3237	3244	rBV6	1882	3271	0.24%	0.036%
85	11.812	3244	3257	3282	rVV	381948	626853	46.74%	6.825%
86	12.066	3328	3336	3348	rBV4	5369	9351	0.70%	0.102%
87	12.137	3355	3358	3361	rVB2	308	187	0.01%	0.002%
88	12.192	3361	3375	3400	rBV	464630	773139	57.65%	8.417%
89	12.552	3484	3487	3491	rVB	287	210	0.02%	0.002%
90	12.848	3575	3579	3582	rBV2	398	431	0.03%	0.005%
91	13.079	3648	3651	3655	rBV2	372	294	0.02%	0.003%
92	13.224	3689	3696	3702	rBV4	2563	3875	0.29%	0.042%
93	13.738	3853	3856	3857	rBV2	337	197	0.01%	0.002%
94	13.812	3877	3879	3882	rBV	323	183	0.01%	0.002%
95	13.844	3882	3889	3903	rVB5	2945	5462	0.41%	0.059%
96	13.986	3931	3933	3936	rBV2	358	237	0.02%	0.003%
97	14.092	3961	3966	3974	rBV2	3637	4883	0.36%	0.053%
98	14.330	4034	4040	4054	rVB4	2591	4833	0.36%	0.053%
99	15.021	4252	4255	4256	rBV2	550	286	0.02%	0.003%
100	15.529	4410	4413	4415	rBV3	714	484	0.04%	0.005%




Sum of corrected areas: 9185070

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050608.D
Acq On : 03 Sep 2022 13:39
Operator : SY/MD
Sample : N4399-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

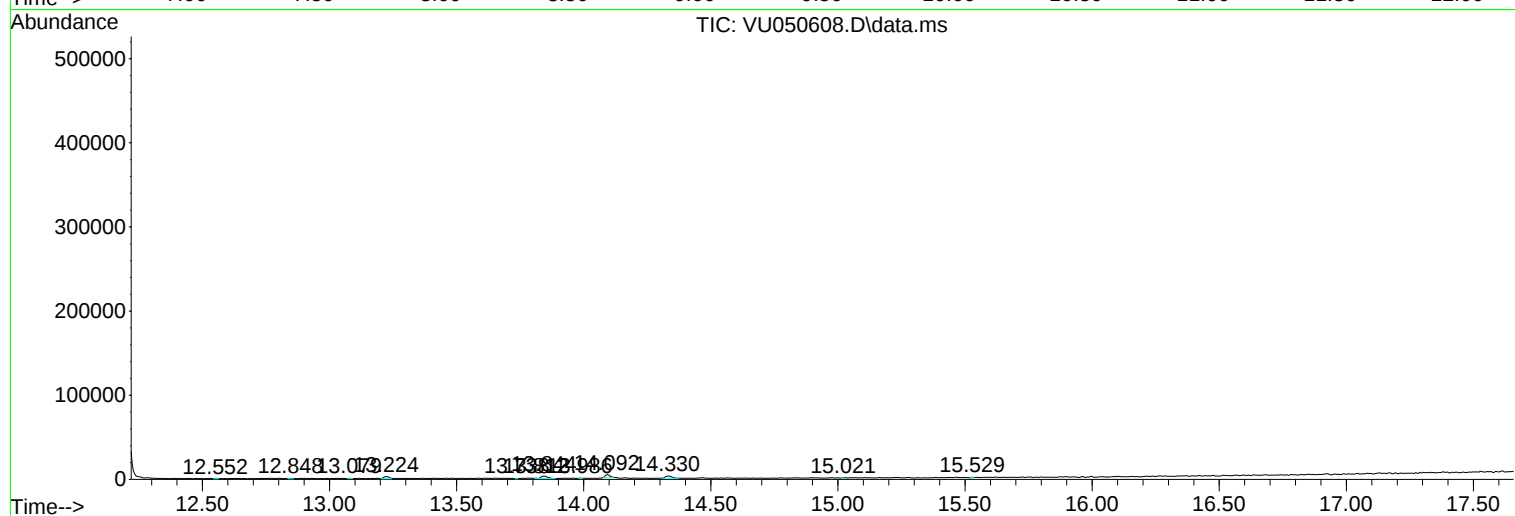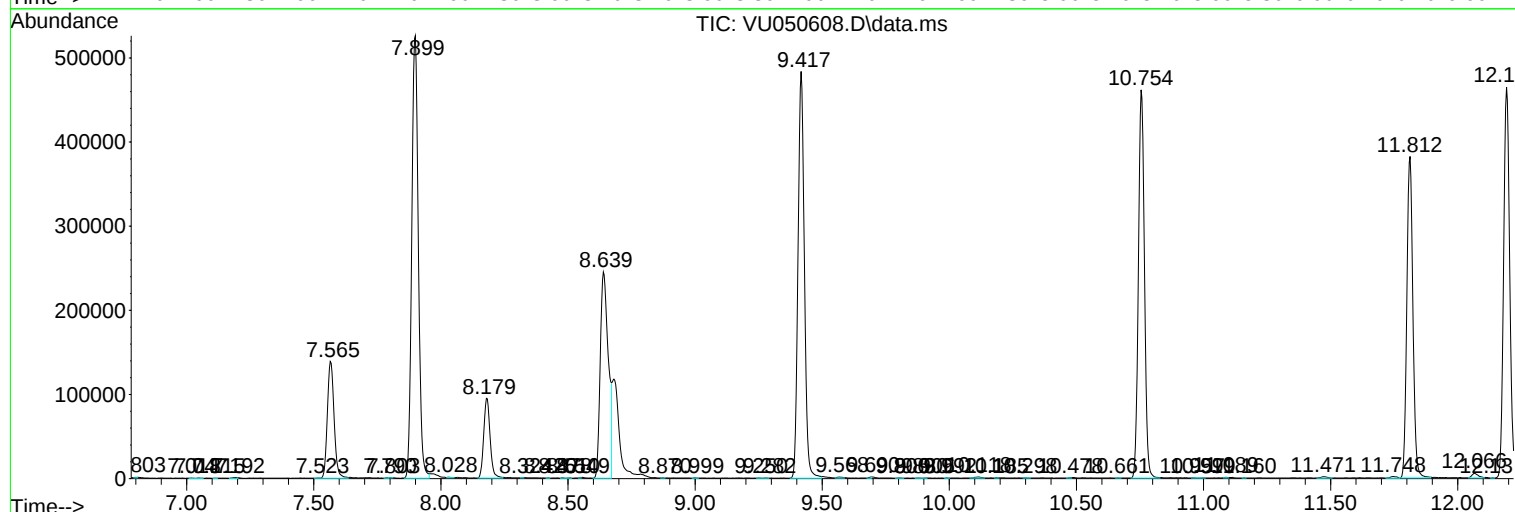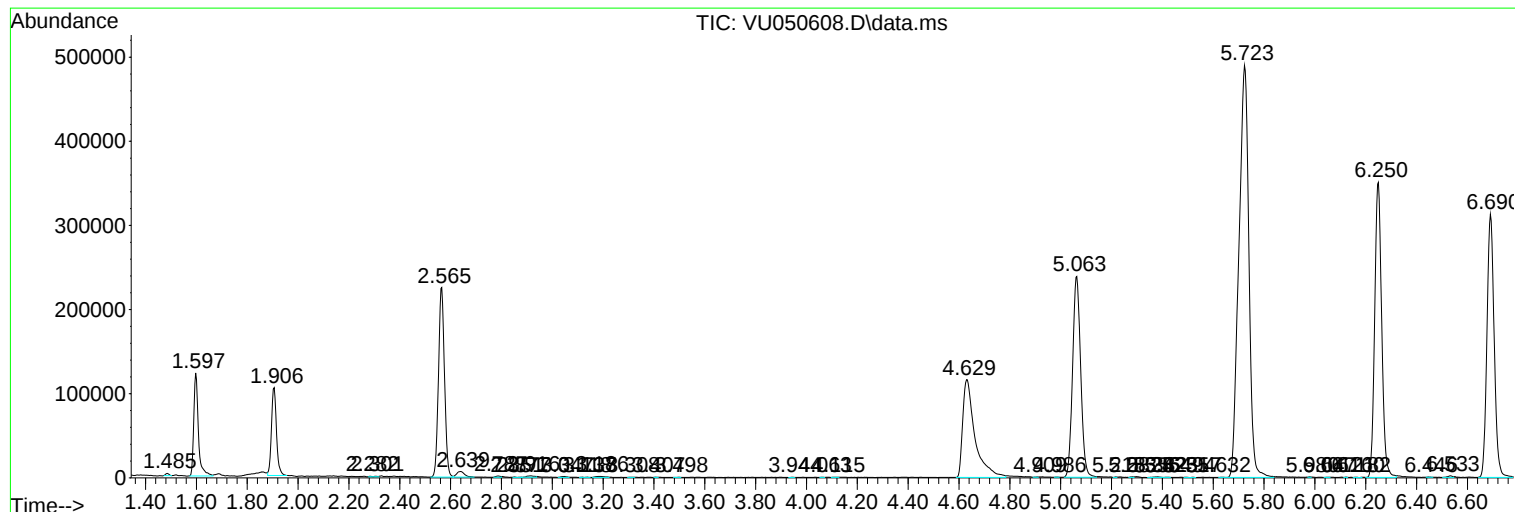

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050608.D
Acq On : 03 Sep 2022 13:39
Operator : SY/MD
Sample : N4399-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050608.D
Acq On : 03 Sep 2022 13:39
Operator : SY/MD
Sample : N4399-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------