

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050609.D
 Acq On : 03 Sep 2022 14:02
 Operator : SY/MD
 Sample : N4458-02DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050609.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	40	44	50	rBV5	2313	2669	0.20%	0.027%
2	1.597	72	80	103	rBV	114629	147415	11.02%	1.501%
3	1.732	117	122	132	rVB3	3240	3765	0.28%	0.038%
4	1.903	167	175	191	rVB	101047	136371	10.19%	1.388%
5	2.189	261	264	268	rBV2	635	472	0.04%	0.005%
6	2.375	320	322	330	rVB5	444	329	0.02%	0.003%
7	2.562	368	380	398	rBV	221425	359343	26.86%	3.659%
8	2.703	421	424	427	rBV2	345	268	0.02%	0.003%
9	2.787	445	450	457	rBV2	1084	1414	0.11%	0.014%
10	2.832	460	464	467	rBV	303	267	0.02%	0.003%
11	3.041	520	529	541	rBV2	6463	11589	0.87%	0.118%
12	3.186	559	574	596	rBV	13453	32764	2.45%	0.334%
13	3.353	624	626	629	rVV2	309	203	0.02%	0.002%
14	3.417	639	646	652	rVV2	220	307	0.02%	0.003%
15	3.491	663	669	674	rBV	301	266	0.02%	0.003%
16	3.645	710	717	721	rVV2	279	358	0.03%	0.004%
17	3.681	721	728	733	rVB2	257	273	0.02%	0.003%
18	3.903	791	797	801	rBV2	226	304	0.02%	0.003%
19	3.945	807	810	817	rVB2	262	284	0.02%	0.003%
20	4.205	888	891	893	rBV2	280	211	0.02%	0.002%
21	4.629	1010	1023	1076	rBV2	128097	419063	31.32%	4.267%
22	5.060	1142	1157	1183	rVV	236074	520860	38.93%	5.303%
23	5.189	1193	1197	1200	rBV3	310	250	0.02%	0.003%
24	5.253	1212	1217	1220	rBV3	560	550	0.04%	0.006%
25	5.285	1220	1227	1236	rVV5	902	1914	0.14%	0.019%
26	5.340	1241	1244	1248	rVV	290	242	0.02%	0.002%
27	5.359	1248	1250	1253	rVV2	506	424	0.03%	0.004%
28	5.382	1253	1257	1265	rVV5	1023	1444	0.11%	0.015%
29	5.433	1269	1273	1280	rVB2	285	302	0.02%	0.003%
30	5.530	1295	1303	1309	rBV3	693	846	0.06%	0.009%
31	5.723	1342	1363	1376	rBV2	482036	1337921	100.00%	13.622%
32	5.986	1441	1445	1449	rBV3	381	328	0.02%	0.003%
33	6.247	1511	1526	1558	rBV	337384	651290	48.68%	6.631%
34	6.433	1581	1584	1588	rBV2	255	222	0.02%	0.002%
35	6.536	1606	1616	1623	rVB7	1926	3609	0.27%	0.037%
36	6.571	1623	1627	1628	rBV3	452	296	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050609.D
 Acq On : 03 Sep 2022 14:02
 Operator : SY/MD
 Sample : N4458-02DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	6.690	1649	1664	1685	rBV	317359	617183	46.13%	6.284%
38	6.806	1697	1700	1703	rVB3	539	411	0.03%	0.004%
39	6.887	1722	1725	1733	rBV2	185	209	0.02%	0.002%
40	6.932	1736	1739	1748	rVB2	248	317	0.02%	0.003%
41	7.012	1757	1764	1768	rVB2	264	334	0.02%	0.003%
42	7.195	1811	1821	1829	rBV3	918	1528	0.11%	0.016%
43	7.488	1909	1912	1920	rVB	318	309	0.02%	0.003%
44	7.565	1920	1936	1964	rBV	138153	248236	18.55%	2.527%
45	7.694	1970	1976	1980	rBV4	642	673	0.05%	0.007%
46	7.800	2003	2009	2011	rBV	627	640	0.05%	0.007%
47	7.896	2025	2039	2075	rBV	525941	925872	69.20%	9.427%
48	8.134	2110	2113	2116	rBV2	349	281	0.02%	0.003%
49	8.179	2116	2127	2143	rBV	92410	158615	11.86%	1.615%
50	8.443	2206	2209	2216	rVB2	473	424	0.03%	0.004%
51	8.497	2224	2226	2232	rVB	395	288	0.02%	0.003%
52	8.552	2237	2243	2245	rBV6	883	863	0.06%	0.009%
53	8.639	2257	2270	2280	rBV3	254830	558572	41.75%	5.687%
54	8.838	2330	2332	2335	rVB2	410	201	0.02%	0.002%
55	8.870	2339	2342	2345	rBV3	320	246	0.02%	0.003%
56	8.899	2349	2351	2356	rVB2	343	237	0.02%	0.002%
57	9.028	2384	2391	2394	rBV2	413	373	0.03%	0.004%
58	9.112	2414	2417	2419	rBV2	311	224	0.02%	0.002%
59	9.256	2456	2462	2464	rBV2	288	301	0.02%	0.003%
60	9.417	2498	2512	2516	rBV	485682	768598	57.45%	7.826%
61	9.642	2580	2582	2589	rVB2	301	234	0.02%	0.002%
62	9.700	2589	2600	2605	rBV3	1096	1683	0.13%	0.017%
63	9.729	2605	2609	2613	rVB2	238	223	0.02%	0.002%
64	9.829	2634	2640	2646	rVB2	335	383	0.03%	0.004%
65	9.915	2659	2667	2673	rBV2	267	381	0.03%	0.004%
66	10.047	2702	2708	2711	rBV	357	323	0.02%	0.003%
67	10.111	2718	2728	2731	rBV5	1297	2038	0.15%	0.021%
68	10.481	2839	2843	2844	rBV	290	213	0.02%	0.002%
69	10.587	2873	2876	2879	rBV2	279	209	0.02%	0.002%
70	10.755	2915	2928	2948	rBV	465945	748115	55.92%	7.617%
71	10.938	2982	2985	2989	rVB3	426	300	0.02%	0.003%
72	10.964	2989	2993	2996	rBV	383	322	0.02%	0.003%
73	11.092	3027	3033	3036	rBV3	756	878	0.07%	0.009%
74	11.246	3078	3081	3084	rBV	277	233	0.02%	0.002%
75	11.330	3103	3107	3115	rVB2	259	307	0.02%	0.003%
76	11.459	3144	3147	3148	rBV2	711	415	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050609.D
 Acq On : 03 Sep 2022 14:02
 Operator : SY/MD
 Sample : N4458-02DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

77	11.520	3161	3166	3169	rBV2	319	320	0.02%	0.003%
78	11.697	3218	3221	3227	rVB2	292	310	0.02%	0.003%
79	11.745	3227	3236	3245	rBV3	21930	34243	2.56%	0.349%
80	11.812	3245	3257	3283	rVB2	398298	871809	65.16%	8.876%
81	11.928	3291	3293	3296	rVB4	637	388	0.03%	0.004%
82	11.970	3303	3306	3310	rBV2	396	274	0.02%	0.003%
83	12.070	3334	3337	3339	rBV3	854	486	0.04%	0.005%
84	12.195	3362	3376	3408	rVV2	529497	1159233	86.64%	11.803%
85	12.404	3439	3441	3447	rBV3	268	246	0.02%	0.003%
86	12.513	3470	3475	3480	rBV3	530	634	0.05%	0.006%
87	12.664	3519	3522	3527	rVB3	436	415	0.03%	0.004%
88	12.748	3546	3548	3553	rVB2	489	411	0.03%	0.004%
89	12.941	3606	3608	3614	rVB2	369	287	0.02%	0.003%
90	12.973	3614	3618	3620	rBV2	473	358	0.03%	0.004%
91	13.044	3637	3640	3647	rBV3	315	346	0.03%	0.004%
92	13.224	3688	3696	3703	rBV3	2225	3346	0.25%	0.034%
93	13.465	3768	3771	3774	rBV2	452	365	0.03%	0.004%
94	13.571	3800	3804	3807	rBV2	396	418	0.03%	0.004%
95	13.841	3878	3888	3901	rBV3	27926	46342	3.46%	0.472%
96	14.015	3939	3942	3945	rBV2	368	286	0.02%	0.003%
97	14.095	3960	3967	3975	rBV	3434	5737	0.43%	0.058%
98	14.333	4032	4041	4054	rVB5	9442	14728	1.10%	0.150%
99	14.986	4242	4244	4248	rVB	674	302	0.02%	0.003%
100	15.729	4472	4475	4478	rBV2	1054	673	0.05%	0.007%




Sum of corrected areas: 9821582

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050609.D
Acq On : 03 Sep 2022 14:02
Operator : SY/MD
Sample : N4458-02DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

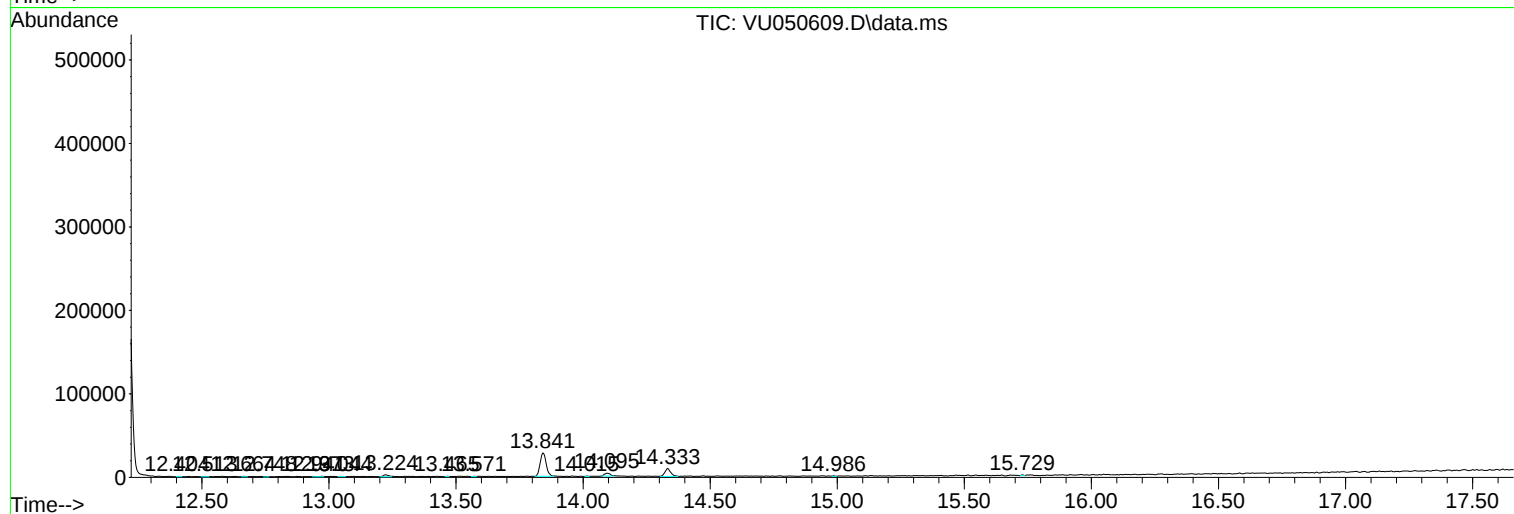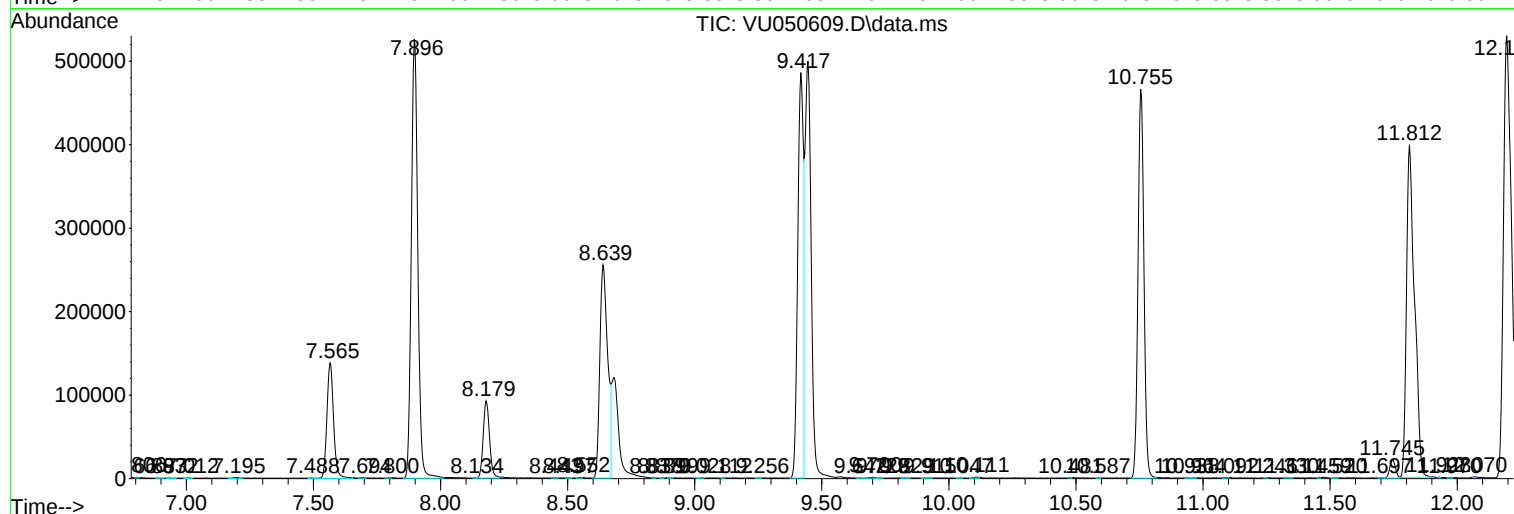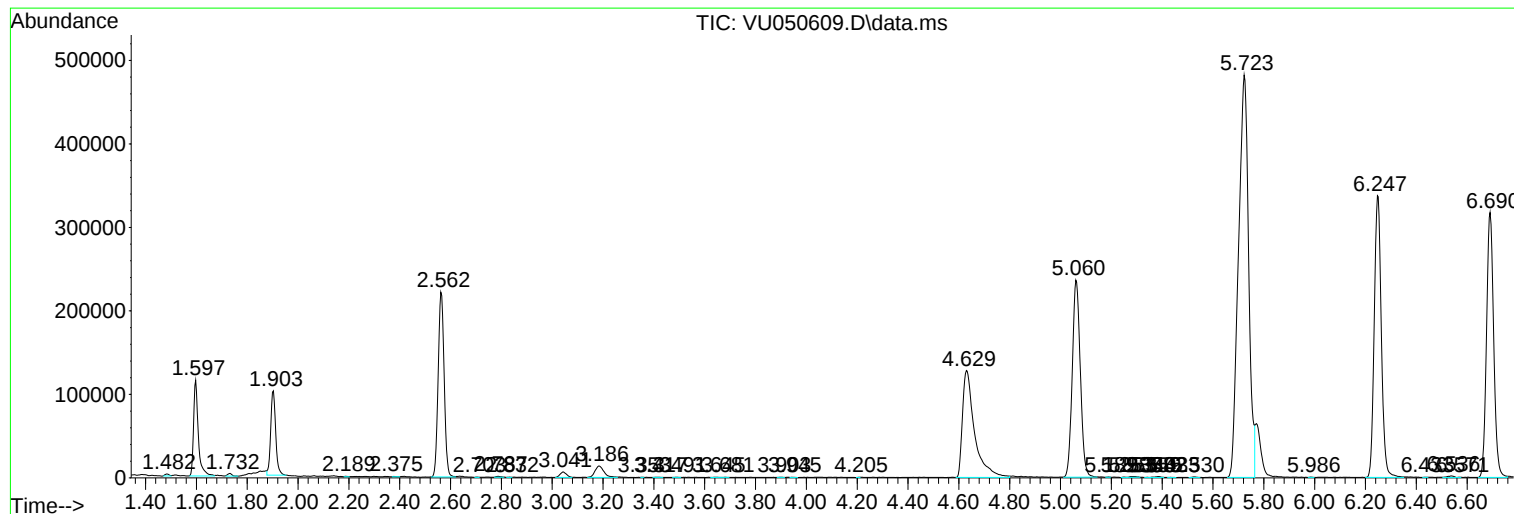

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050609.D
Acq On : 03 Sep 2022 14:02
Operator : SY/MD
Sample : N4458-02DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050609.D
Acq On : 03 Sep 2022 14:02
Operator : SY/MD
Sample : N4458-02DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------