

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050610.D
 Acq On : 03 Sep 2022 14:26
 Operator : SY/MD
 Sample : N4458-02 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M

Title : VOC Analysis

Signal : TIC: VU050610.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	51	rBV2	2798	3163	0.06%	0.017%
2	1.597	72	80	103	rBV	135190	170091	3.06%	0.889%
3	1.729	118	121	129	rVB3	2114	2277	0.04%	0.012%
4	1.903	167	175	192	rVB	105542	142770	2.57%	0.746%
5	2.157	251	254	257	rVB2	504	319	0.01%	0.002%
6	2.436	338	341	343	rBV2	512	344	0.01%	0.002%
7	2.562	368	380	396	rVV	249241	403084	7.24%	2.106%
8	2.623	396	399	401	rBV4	434	304	0.01%	0.002%
9	2.758	435	441	444	rBV	304	305	0.01%	0.002%
10	2.784	444	449	452	rBV	1018	1078	0.02%	0.006%
11	2.964	502	505	508	rVB2	374	254	0.00%	0.001%
12	3.044	520	530	541	rBV5	4035	7825	0.14%	0.041%
13	3.186	559	574	597	rBV	10431	24422	0.44%	0.128%
14	3.272	597	601	602	rBV	392	253	0.00%	0.001%
15	3.350	616	625	628	rBV3	417	462	0.01%	0.002%
16	3.970	813	818	827	rVB2	211	336	0.01%	0.002%
17	4.018	827	833	837	rBV2	352	393	0.01%	0.002%
18	4.379	936	945	947	rBV2	224	285	0.01%	0.001%
19	4.533	990	993	996	rBV3	521	369	0.01%	0.002%
20	4.629	1010	1023	1071	rBV2	127937	409556	7.36%	2.140%
21	4.919	1110	1113	1115	rBV2	384	229	0.00%	0.001%
22	5.060	1141	1157	1184	rBV	261953	582915	10.47%	3.046%
23	5.247	1213	1215	1221	rVB2	335	299	0.01%	0.002%
24	5.276	1221	1224	1225	rBV	390	238	0.00%	0.001%
25	5.292	1226	1229	1233	rVB2	496	443	0.01%	0.002%
26	5.378	1250	1256	1258	rVV4	404	411	0.01%	0.002%
27	5.388	1258	1259	1267	rVB4	722	635	0.01%	0.003%
28	5.523	1291	1301	1311	rVB4	1888	3376	0.06%	0.018%
29	5.591	1318	1322	1326	rBV	229	227	0.00%	0.001%
30	5.723	1342	1363	1372	rBV2	551043	1464862	26.32%	7.654%
31	5.980	1438	1443	1446	rBV4	484	448	0.01%	0.002%
32	6.034	1457	1460	1466	rVB3	397	334	0.01%	0.002%
33	6.247	1512	1526	1548	rBV	390503	746322	13.41%	3.900%
34	6.513	1601	1609	1610	rBV	1036	646	0.01%	0.003%
35	6.530	1610	1614	1617	rBV3	914	788	0.01%	0.004%
36	6.620	1635	1642	1647	rVB3	307	386	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050610.D
 Acq On : 03 Sep 2022 14:26
 Operator : SY/MD
 Sample : N4458-02 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	6.690	1649	1664	1686	rBV	345327	672160	12.08%	3.512%
38	6.938	1739	1741	1747	rVB2	324	266	0.00%	0.001%
39	7.189	1813	1819	1823	rBV4	1018	1187	0.02%	0.006%
40	7.266	1835	1843	1846	rBV2	688	789	0.01%	0.004%
41	7.565	1921	1936	1956	rBV	153637	271885	4.89%	1.421%
42	7.700	1974	1978	1984	rVB4	555	623	0.01%	0.003%
43	7.793	2002	2007	2010	rBV4	602	592	0.01%	0.003%
44	7.896	2023	2039	2070	rBV	616761	1077650	19.36%	5.631%
45	8.179	2115	2127	2149	rBV	100606	174438	3.13%	0.911%
46	8.555	2238	2244	2248	rVB4	867	895	0.02%	0.005%
47	8.639	2257	2270	2279	rBV3	271575	571345	10.27%	2.985%
48	8.835	2329	2331	2340	rVB4	679	761	0.01%	0.004%
49	8.906	2351	2353	2360	rVB3	322	223	0.00%	0.001%
50	8.980	2369	2376	2378	rBV2	329	396	0.01%	0.002%
51	8.999	2379	2382	2386	rVB3	505	378	0.01%	0.002%
52	9.028	2386	2391	2394	rBV2	355	244	0.00%	0.001%
53	9.166	2429	2434	2435	rBV2	337	262	0.00%	0.001%
54	9.256	2459	2462	2469	rVB2	340	379	0.01%	0.002%
55	9.292	2469	2473	2476	rBV2	295	282	0.01%	0.001%
56	9.446	2499	2521	2556	rBV2	2833668	5565188	100.00%	29.079%
57	9.661	2585	2588	2592	rBV4	600	480	0.01%	0.003%
58	9.687	2594	2596	2597	rBV	626	292	0.01%	0.002%
59	9.796	2627	2630	2635	rVB2	455	284	0.01%	0.001%
60	9.864	2649	2651	2658	rVB3	359	220	0.00%	0.001%
61	9.983	2685	2688	2692	rVB2	408	292	0.01%	0.002%
62	10.050	2702	2709	2712	rBV2	227	288	0.01%	0.002%
63	10.105	2720	2726	2729	rBV3	717	843	0.02%	0.004%
64	10.491	2841	2846	2852	rVB3	786	940	0.02%	0.005%
65	10.529	2852	2858	2861	rBV2	317	381	0.01%	0.002%
66	10.655	2891	2897	2900	rBV2	308	388	0.01%	0.002%
67	10.703	2908	2912	2915	rBV	362	351	0.01%	0.002%
68	10.754	2916	2928	2948	rVV	488108	788578	14.17%	4.120%
69	10.864	2960	2962	2970	rVB4	418	398	0.01%	0.002%
70	10.899	2970	2973	2977	rBV2	341	219	0.00%	0.001%
71	10.938	2981	2985	2989	rVB2	367	279	0.01%	0.001%
72	10.989	2998	3001	3006	rVB2	321	265	0.00%	0.001%
73	11.092	3026	3033	3036	rBV3	1008	1025	0.02%	0.005%
74	11.230	3073	3076	3081	rVB	303	241	0.00%	0.001%
75	11.372	3117	3120	3126	rVB2	383	275	0.00%	0.001%
76	11.404	3127	3130	3133	rBV2	312	213	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050610.D
 Acq On : 03 Sep 2022 14:26
 Operator : SY/MD
 Sample : N4458-02 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

77	11.471	3147	3151	3156	rVB3	906	892	0.02%	0.005%
78	11.745	3222	3236	3246	rBV	126247	196708	3.53%	1.028%
79	11.835	3246	3264	3299	rVB2	1033016	2275111	40.88%	11.888%
80	11.999	3310	3315	3318	rBV3	675	552	0.01%	0.003%
81	12.060	3330	3334	3335	rBV	361	237	0.00%	0.001%
82	12.208	3361	3380	3419	rBV2	1527928	3167914	56.92%	16.553%
83	12.410	3442	3443	3445	rBV2	429	210	0.00%	0.001%
84	12.761	3548	3552	3554	rBV	502	366	0.01%	0.002%
85	12.780	3554	3558	3562	rVB	454	349	0.01%	0.002%
86	12.851	3575	3580	3583	rBV2	408	441	0.01%	0.002%
87	12.912	3596	3599	3601	rVV2	381	228	0.00%	0.001%
88	12.983	3613	3621	3630	rVB5	1169	1870	0.03%	0.010%
89	13.018	3630	3632	3634	rBV2	362	244	0.00%	0.001%
90	13.115	3658	3662	3669	rBV3	583	741	0.01%	0.004%
91	13.169	3676	3679	3682	rBV2	308	253	0.00%	0.001%
92	13.330	3727	3729	3736	rVB3	522	440	0.01%	0.002%
93	13.645	3824	3827	3831	rVB2	708	532	0.01%	0.003%
94	13.748	3856	3859	3862	rBV3	386	344	0.01%	0.002%
95	13.841	3876	3888	3909	rBV	181512	301147	5.41%	1.574%
96	14.092	3958	3966	3977	rBV2	4649	7328	0.13%	0.038%
97	14.330	4030	4040	4053	rBV	45480	74667	1.34%	0.390%
98	14.539	4103	4105	4108	rBV2	364	262	0.00%	0.001%
99	15.172	4300	4302	4303	rBV2	591	259	0.00%	0.001%
100	15.198	4307	4310	4313	rVV3	791	443	0.01%	0.002%




Sum of corrected areas: 19138182

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050610.D
Acq On : 03 Sep 2022 14:26
Operator : SY/MD
Sample : N4458-02 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

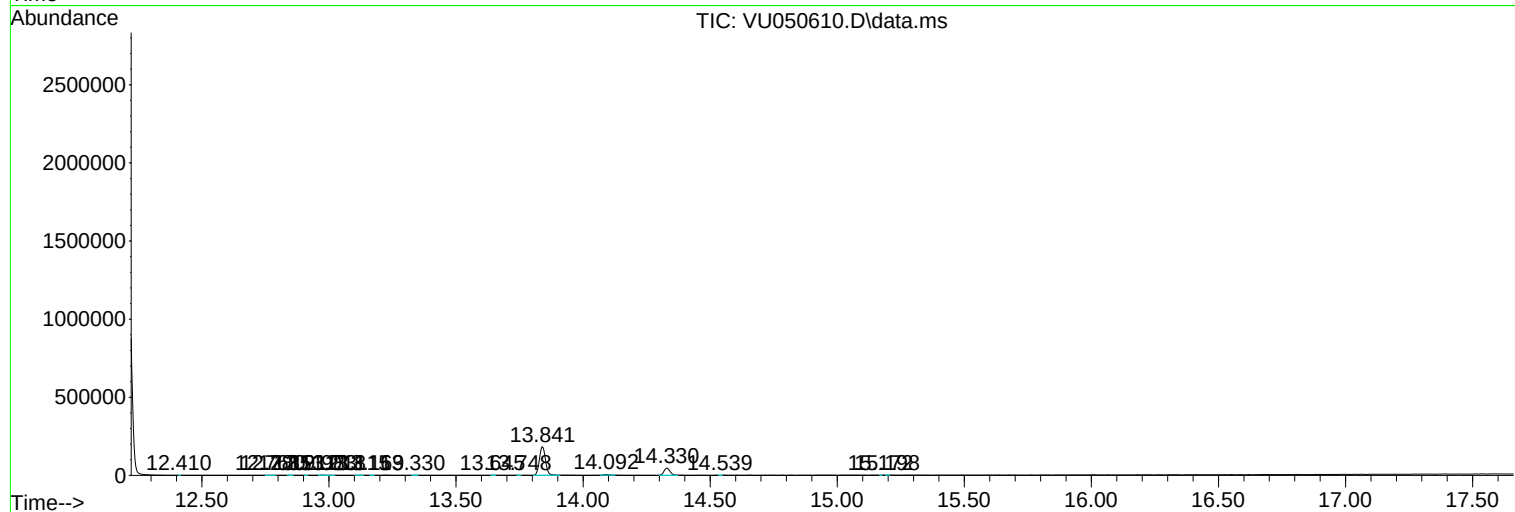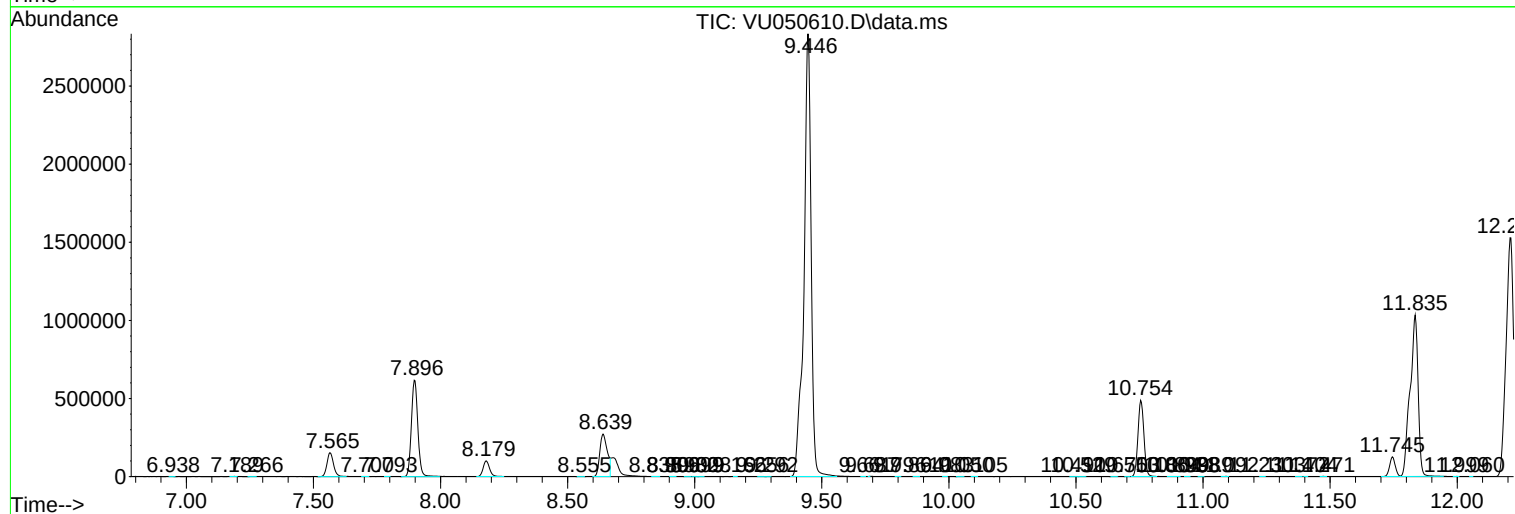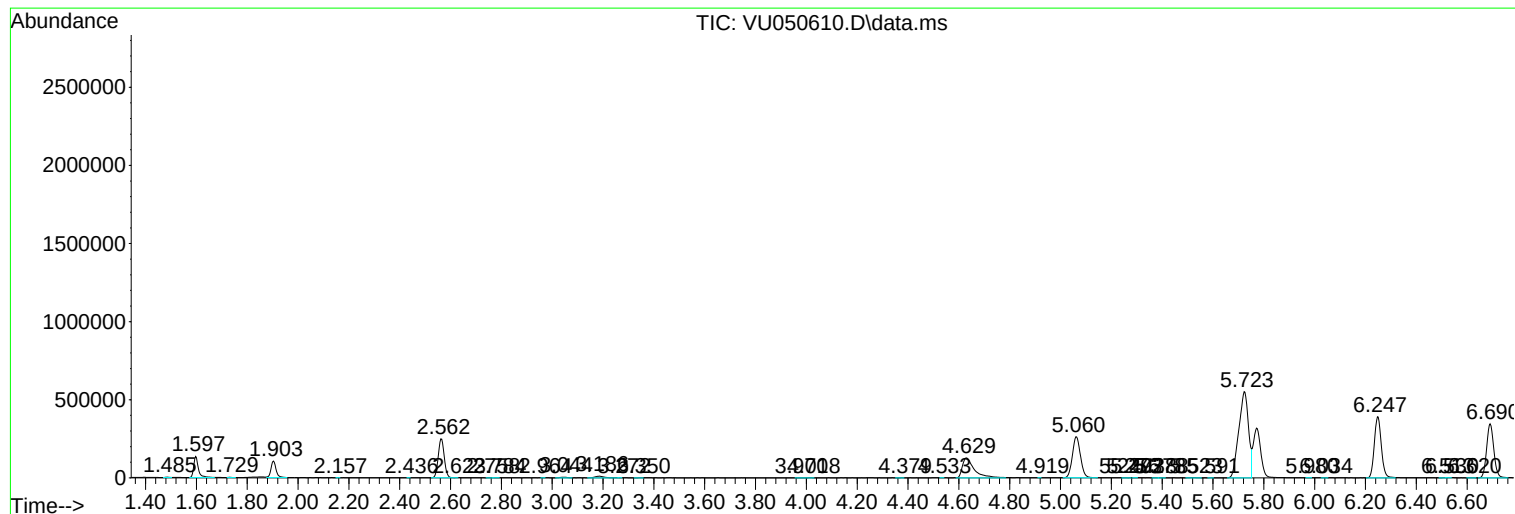

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050610.D
Acq On : 03 Sep 2022 14:26
Operator : SY/MD
Sample : N4458-02 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050610.D
Acq On : 03 Sep 2022 14:26
Operator : SY/MD
Sample : N4458-02 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc