

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050611.D
 Acq On : 03 Sep 2022 14:49
 Operator : SY/MD
 Sample : N4399-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050611.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	51	rVB4	3033	3360	0.26%	0.037%
2	1.597	72	80	100	rBV	138770	168917	13.23%	1.841%
3	1.906	168	176	196	rVB	107716	143261	11.22%	1.561%
4	2.160	253	255	257	rBV	385	203	0.02%	0.002%
5	2.253	282	284	286	rBV2	393	190	0.01%	0.002%
6	2.385	322	325	328	rVB2	598	392	0.03%	0.004%
7	2.411	330	333	337	rBV3	467	477	0.04%	0.005%
8	2.449	343	345	350	rVB2	469	324	0.03%	0.004%
9	2.565	369	381	401	rBV	247979	398452	31.21%	4.342%
10	2.681	415	417	421	rVB3	345	225	0.02%	0.002%
11	2.790	445	451	454	rBV2	773	802	0.06%	0.009%
12	3.044	519	530	537	rBV4	2013	3418	0.27%	0.037%
13	3.092	539	545	553	rVB2	428	400	0.03%	0.004%
14	3.186	561	574	591	rBV	8812	20317	1.59%	0.221%
15	3.314	609	614	617	rBV2	226	181	0.01%	0.002%
16	3.343	617	623	628	rVV2	351	435	0.03%	0.005%
17	3.395	636	639	641	rVV3	394	268	0.02%	0.003%
18	3.440	645	653	657	rVV2	276	424	0.03%	0.005%
19	3.475	661	664	666	rVV	261	192	0.02%	0.002%
20	3.539	681	684	690	rVB2	244	232	0.02%	0.003%
21	3.584	693	698	703	rVB	375	328	0.03%	0.004%
22	4.147	865	873	875	rBV2	218	218	0.02%	0.002%
23	4.260	901	908	913	rVB2	266	316	0.02%	0.003%
24	4.285	913	916	921	rBV2	257	189	0.01%	0.002%
25	4.311	921	924	931	rBV2	341	349	0.03%	0.004%
26	4.375	939	944	947	rBV2	186	195	0.02%	0.002%
27	4.629	1006	1023	1071	rBV	116529	377235	29.54%	4.111%
28	4.961	1124	1126	1130	rVB	474	187	0.01%	0.002%
29	4.983	1130	1133	1140	rBV2	322	260	0.02%	0.003%
30	5.063	1141	1158	1182	rBV	225554	497306	38.95%	5.419%
31	5.288	1222	1228	1232	rBV2	651	940	0.07%	0.010%
32	5.555	1307	1311	1315	rBV2	360	263	0.02%	0.003%
33	5.594	1320	1323	1329	rVB2	250	217	0.02%	0.002%
34	5.726	1341	1364	1395	rBV2	473498	1276881	100.00%	13.914%
35	6.047	1461	1464	1468	rBV	293	249	0.02%	0.003%
36	6.067	1468	1470	1476	rVB3	400	329	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050611.D
 Acq On : 03 Sep 2022 14:49
 Operator : SY/MD
 Sample : N4399-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	6.247	1513	1526	1555	rBV	332428	646344	50.62%	7.043%
38	6.401	1571	1574	1575	rBV2	328	193	0.02%	0.002%
39	6.530	1607	1614	1620	rBV5	1798	2852	0.22%	0.031%
40	6.690	1645	1664	1689	rBV	297064	588249	46.07%	6.410%
41	6.793	1694	1696	1698	rVV2	496	302	0.02%	0.003%
42	6.813	1699	1702	1706	rVB4	757	563	0.04%	0.006%
43	6.941	1738	1742	1746	rBV2	307	244	0.02%	0.003%
44	7.034	1766	1771	1774	rBV	175	182	0.01%	0.002%
45	7.192	1812	1820	1829	rVB5	693	1265	0.10%	0.014%
46	7.378	1873	1878	1883	rVB2	295	327	0.03%	0.004%
47	7.565	1917	1936	1956	rBV	131534	237071	18.57%	2.583%
48	7.751	1990	1994	1998	rBV	341	333	0.03%	0.004%
49	7.796	2004	2008	2010	rBV2	550	460	0.04%	0.005%
50	7.896	2026	2039	2068	rBV	542905	941062	73.70%	10.254%
51	8.018	2074	2077	2079	rBV2	483	302	0.02%	0.003%
52	8.179	2113	2127	2147	rBV	86417	153922	12.05%	1.677%
53	8.485	2216	2222	2225	rBV2	277	305	0.02%	0.003%
54	8.552	2237	2243	2246	rBV3	362	315	0.02%	0.003%
55	8.639	2257	2270	2280	rBV4	227319	509927	39.94%	5.556%
56	9.320	2479	2482	2486	rBV2	288	206	0.02%	0.002%
57	9.417	2499	2512	2534	rBV	470567	821760	64.36%	8.954%
58	9.690	2593	2597	2600	rBV3	374	319	0.02%	0.003%
59	9.732	2606	2610	2613	rVB	270	205	0.02%	0.002%
60	9.755	2613	2617	2621	rBV	338	253	0.02%	0.003%
61	9.877	2651	2655	2659	rBV2	229	212	0.02%	0.002%
62	9.902	2660	2663	2667	rVB	334	245	0.02%	0.003%
63	10.095	2720	2723	2727	rVB2	568	423	0.03%	0.005%
64	10.118	2727	2730	2736	rBV2	468	573	0.04%	0.006%
65	10.246	2767	2770	2774	rVB	284	178	0.01%	0.002%
66	10.308	2783	2789	2792	rBV	295	291	0.02%	0.003%
67	10.388	2811	2814	2819	rBV	255	178	0.01%	0.002%
68	10.439	2827	2830	2834	rBV2	260	238	0.02%	0.003%
69	10.478	2840	2842	2850	rVB2	366	404	0.03%	0.004%
70	10.565	2866	2869	2872	rBV	245	225	0.02%	0.002%
71	10.674	2897	2903	2907	rBV2	364	436	0.03%	0.005%
72	10.755	2915	2928	2951	rVV	454177	750527	58.78%	8.178%
73	10.883	2964	2968	2971	rBV2	446	367	0.03%	0.004%
74	11.092	3028	3033	3035	rBV3	506	445	0.03%	0.005%
75	11.160	3048	3054	3058	rBV2	338	471	0.04%	0.005%
76	11.298	3092	3097	3101	rBV2	327	320	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050611.D
 Acq On : 03 Sep 2022 14:49
 Operator : SY/MD
 Sample : N4399-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

77	11.401	3125	3129	3135	rBV2	276	300	0.02%	0.003%
78	11.430	3135	3138	3142	rBV2	232	222	0.02%	0.002%
79	11.465	3145	3149	3150	rBV	626	426	0.03%	0.005%
80	11.597	3186	3190	3193	rBV2	377	319	0.02%	0.003%
81	11.748	3230	3237	3245	rBV3	3451	4736	0.37%	0.052%
82	11.812	3245	3257	3281	rBV	404299	702147	54.99%	7.651%
83	11.951	3295	3300	3303	rBV3	334	343	0.03%	0.004%
84	11.986	3309	3311	3317	rVB3	600	503	0.04%	0.005%
85	12.031	3322	3325	3327	rBV2	286	196	0.02%	0.002%
86	12.192	3361	3375	3407	rBV	498904	866867	67.89%	9.446%
87	12.333	3415	3419	3423	rVB3	664	516	0.04%	0.006%
88	12.500	3467	3471	3474	rBV2	423	354	0.03%	0.004%
89	12.539	3481	3483	3486	rVV	383	252	0.02%	0.003%
90	12.783	3555	3559	3565	rBV2	398	503	0.04%	0.005%
91	12.880	3586	3589	3592	rBV	409	244	0.02%	0.003%
92	12.963	3610	3615	3621	rVB3	368	500	0.04%	0.005%
93	12.996	3621	3625	3628	rBV	358	297	0.02%	0.003%
94	13.224	3692	3696	3703	rVB3	753	887	0.07%	0.010%
95	13.330	3726	3729	3731	rBV	317	185	0.01%	0.002%
96	13.481	3772	3776	3779	rBV3	357	316	0.02%	0.003%
97	13.619	3816	3819	3821	rBV2	420	264	0.02%	0.003%
98	13.844	3879	3889	3905	rBV3	15360	25956	2.03%	0.283%
99	13.963	3921	3926	3930	rBV2	523	648	0.05%	0.007%
100	14.336	4033	4042	4059	rVB7	5707	9727	0.76%	0.106%




Sum of corrected areas: 9177134

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050611.D
Acq On : 03 Sep 2022 14:49
Operator : SY/MD
Sample : N4399-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

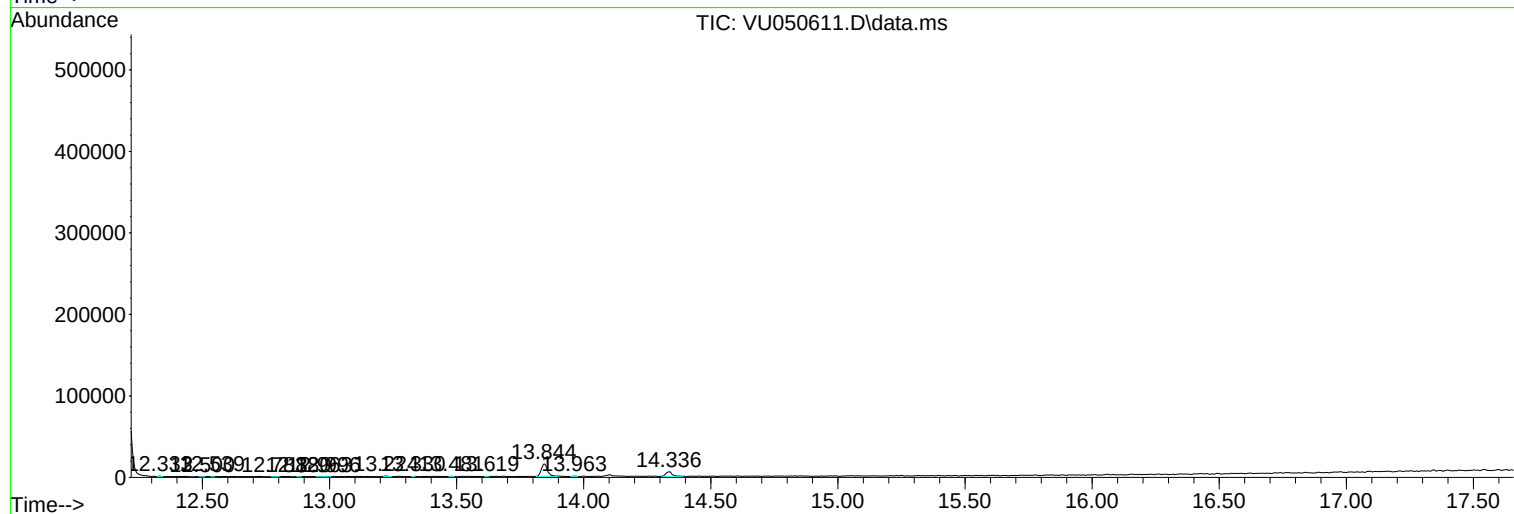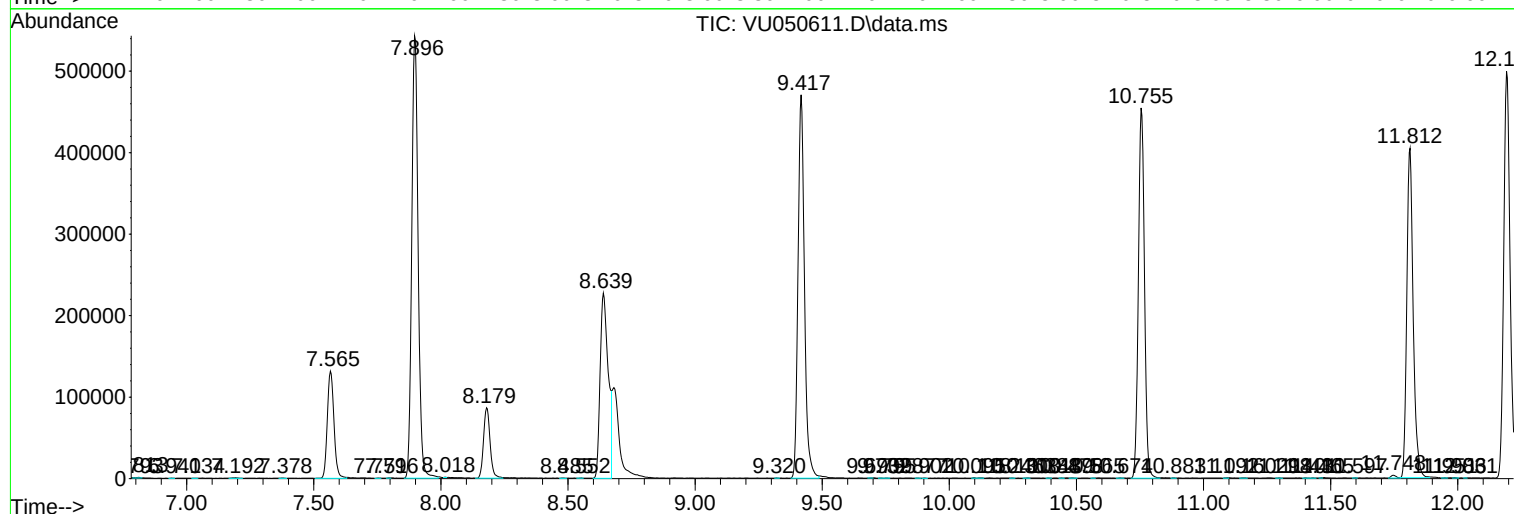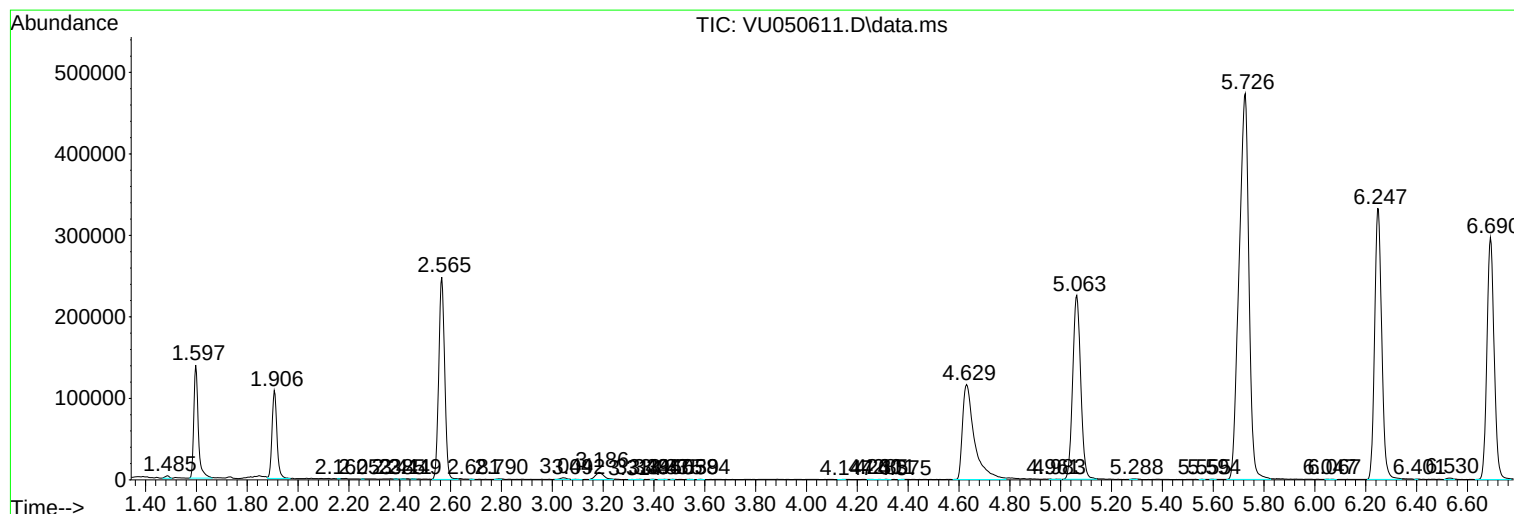

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050611.D
Acq On : 03 Sep 2022 14:49
Operator : SY/MD
Sample : N4399-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050611.D
Acq On : 03 Sep 2022 14:49
Operator : SY/MD
Sample : N4399-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------