

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050612.D
 Acq On : 03 Sep 2022 15:13
 Operator : SY/MD
 Sample : N4458-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050612.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	97	rBV	154044	191294	13.36%	1.946%
2	1.729	117	121	131	rVB2	2840	3503	0.24%	0.036%
3	1.906	168	176	196	rVB	128196	174185	12.16%	1.772%
4	2.237	276	279	285	rBV4	614	533	0.04%	0.005%
5	2.295	295	297	299	rBV2	470	314	0.02%	0.003%
6	2.565	367	381	398	rBV	277374	452573	31.60%	4.603%
7	2.726	427	431	438	rVB3	353	361	0.03%	0.004%
8	2.793	446	452	456	rBV4	659	823	0.06%	0.008%
9	2.909	486	488	494	rVB2	389	291	0.02%	0.003%
10	3.041	523	529	539	rVB3	2730	4407	0.31%	0.045%
11	3.186	561	574	592	rVV3	10917	25108	1.75%	0.255%
12	3.353	623	626	629	rVB	321	193	0.01%	0.002%
13	3.379	630	634	638	rBV2	182	199	0.01%	0.002%
14	3.449	650	656	660	rVV2	195	202	0.01%	0.002%
15	3.478	660	665	668	rVV2	177	212	0.01%	0.002%
16	3.662	719	722	729	rBV2	190	236	0.02%	0.002%
17	3.813	765	769	771	rBV2	281	197	0.01%	0.002%
18	3.874	781	788	792	rVB2	299	377	0.03%	0.004%
19	3.906	792	798	803	rBV2	334	381	0.03%	0.004%
20	4.025	830	835	839	rBV	620	743	0.05%	0.008%
21	4.253	903	906	912	rVB2	267	256	0.02%	0.003%
22	4.285	912	916	920	rBV2	219	218	0.02%	0.002%
23	4.340	930	933	937	rBV2	186	196	0.01%	0.002%
24	4.533	987	993	998	rBB2	219	306	0.02%	0.003%
25	4.572	998	1005	1007	rBV2	191	202	0.01%	0.002%
26	4.633	1010	1024	1072	rBV2	134813	441226	30.81%	4.488%
27	4.932	1114	1117	1119	rBV3	407	238	0.02%	0.002%
28	4.977	1129	1131	1137	rVB4	486	368	0.03%	0.004%
29	5.063	1141	1158	1183	rBV	256169	564658	39.42%	5.743%
30	5.289	1219	1228	1229	rBV4	860	856	0.06%	0.009%
31	5.330	1237	1241	1245	rBV	180	190	0.01%	0.002%
32	5.723	1342	1363	1394	rBV2	528487	1432292	100.00%	14.568%
33	5.890	1412	1415	1421	rVB3	435	375	0.03%	0.004%
34	5.977	1438	1442	1449	rBV3	511	541	0.04%	0.006%
35	6.054	1463	1466	1469	rVB	435	287	0.02%	0.003%
36	6.112	1480	1484	1490	rBV3	316	322	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050612.D
 Acq On : 03 Sep 2022 15:13
 Operator : SY/MD
 Sample : N4458-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	6.144	1490	1494	1496	rBV2	341	249	0.02%	0.003%
38	6.250	1509	1527	1553	rBV	369305	716439	50.02%	7.287%
39	6.526	1607	1613	1626	rBV4	2186	3771	0.26%	0.038%
40	6.626	1640	1644	1647	rVB2	313	229	0.02%	0.002%
41	6.690	1647	1664	1694	rBV	335273	661634	46.19%	6.730%
42	6.858	1714	1716	1721	rVB3	309	207	0.01%	0.002%
43	7.099	1788	1791	1797	rVB2	290	247	0.02%	0.003%
44	7.179	1810	1816	1817	rBV3	582	454	0.03%	0.005%
45	7.395	1878	1883	1888	rVB	451	421	0.03%	0.004%
46	7.565	1923	1936	1961	rBV	146019	259436	18.11%	2.639%
47	7.700	1974	1978	1983	rVB3	686	779	0.05%	0.008%
48	7.761	1994	1997	2000	rVB2	312	215	0.02%	0.002%
49	7.790	2000	2006	2007	rBV3	310	324	0.02%	0.003%
50	7.896	2025	2039	2059	rBV	571686	1018771	71.13%	10.362%
51	8.121	2107	2109	2114	rVB	473	386	0.03%	0.004%
52	8.179	2114	2127	2146	rBV	96095	169281	11.82%	1.722%
53	8.404	2194	2197	2202	rVB3	305	317	0.02%	0.003%
54	8.494	2223	2225	2230	rVB2	321	203	0.01%	0.002%
55	8.639	2257	2270	2280	rBV3	262300	583774	40.76%	5.938%
56	8.864	2337	2340	2343	rVB2	327	249	0.02%	0.003%
57	8.896	2343	2350	2355	rBV4	422	616	0.04%	0.006%
58	9.147	2422	2428	2429	rBV2	306	213	0.01%	0.002%
59	9.237	2454	2456	2462	rVB2	319	247	0.02%	0.003%
60	9.417	2499	2512	2535	rBV	500050	851385	59.44%	8.660%
61	9.562	2554	2557	2560	rBV4	344	255	0.02%	0.003%
62	9.594	2565	2567	2570	rVB2	388	236	0.02%	0.002%
63	9.616	2570	2574	2579	rBV2	304	294	0.02%	0.003%
64	9.925	2665	2670	2673	rBV	254	252	0.02%	0.003%
65	10.205	2753	2757	2760	rBV2	247	208	0.01%	0.002%
66	10.359	2800	2805	2808	rBV2	281	274	0.02%	0.003%
67	10.456	2830	2835	2839	rBV2	285	286	0.02%	0.003%
68	10.478	2839	2842	2845	rBV2	444	361	0.03%	0.004%
69	10.526	2852	2857	2862	rBV2	224	312	0.02%	0.003%
70	10.755	2915	2928	2953	rBV	481079	784148	54.75%	7.976%
71	10.890	2967	2970	2973	rVB2	305	192	0.01%	0.002%
72	10.931	2981	2983	2987	rVB2	297	186	0.01%	0.002%
73	10.986	2996	3000	3005	rBV2	277	295	0.02%	0.003%
74	11.089	3029	3032	3035	rVB2	445	301	0.02%	0.003%
75	11.121	3035	3042	3047	rVB4	832	1065	0.07%	0.011%
76	11.150	3047	3051	3056	rBV2	204	283	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050612.D
 Acq On : 03 Sep 2022 15:13
 Operator : SY/MD
 Sample : N4458-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

77	11.472	3144	3151	3154	rBV3	562	598	0.04%	0.006%
78	11.755	3230	3239	3245	rBV3	924	1482	0.10%	0.015%
79	11.812	3245	3257	3275	rBV	386360	643831	44.95%	6.549%
80	12.192	3362	3375	3403	rBV	480002	811465	56.65%	8.254%
81	12.340	3418	3421	3422	rBV2	322	199	0.01%	0.002%
82	12.391	3435	3437	3441	rVB	318	224	0.02%	0.002%
83	12.452	3453	3456	3459	rBV	261	193	0.01%	0.002%
84	12.478	3462	3464	3471	rVB3	241	255	0.02%	0.003%
85	12.539	3480	3483	3485	rBV2	285	222	0.02%	0.002%
86	12.574	3491	3494	3496	rBV	431	294	0.02%	0.003%
87	12.610	3502	3505	3508	rVB2	328	186	0.01%	0.002%
88	12.816	3566	3569	3572	rBV	364	297	0.02%	0.003%
89	13.144	3667	3671	3679	rVB3	474	609	0.04%	0.006%
90	13.185	3682	3684	3687	rBV	451	273	0.02%	0.003%
91	13.221	3692	3695	3703	rVB3	750	721	0.05%	0.007%
92	13.314	3721	3724	3728	rVB2	421	329	0.02%	0.003%
93	13.468	3767	3772	3774	rBV2	397	363	0.03%	0.004%
94	13.597	3809	3812	3817	rBV	313	234	0.02%	0.002%
95	13.751	3858	3860	3863	rBV2	311	190	0.01%	0.002%
96	13.844	3882	3889	3898	rBV4	4480	7140	0.50%	0.073%
97	14.205	3999	4001	4005	rBV2	345	238	0.02%	0.002%
98	14.230	4006	4009	4014	rVV3	442	305	0.02%	0.003%
99	14.333	4034	4041	4051	rVB5	2471	3970	0.28%	0.040%
100	15.060	4264	4267	4271	rBV3	734	541	0.04%	0.006%




Sum of corrected areas: 9831617

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050612.D
Acq On : 03 Sep 2022 15:13
Operator : SY/MD
Sample : N4458-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

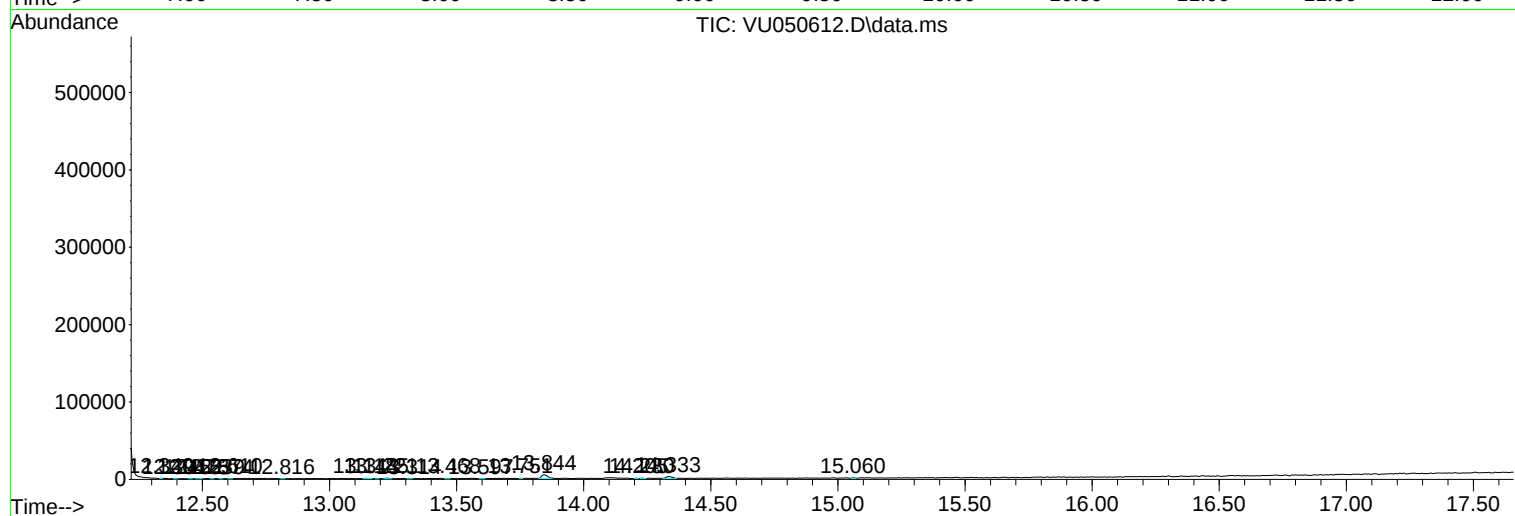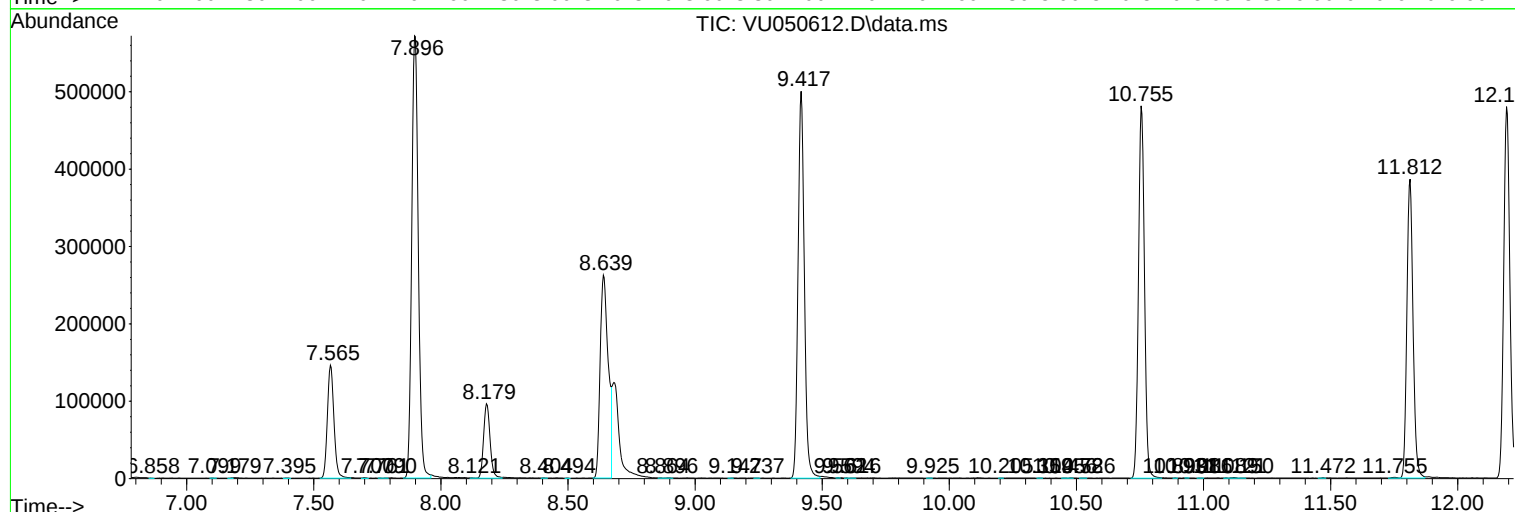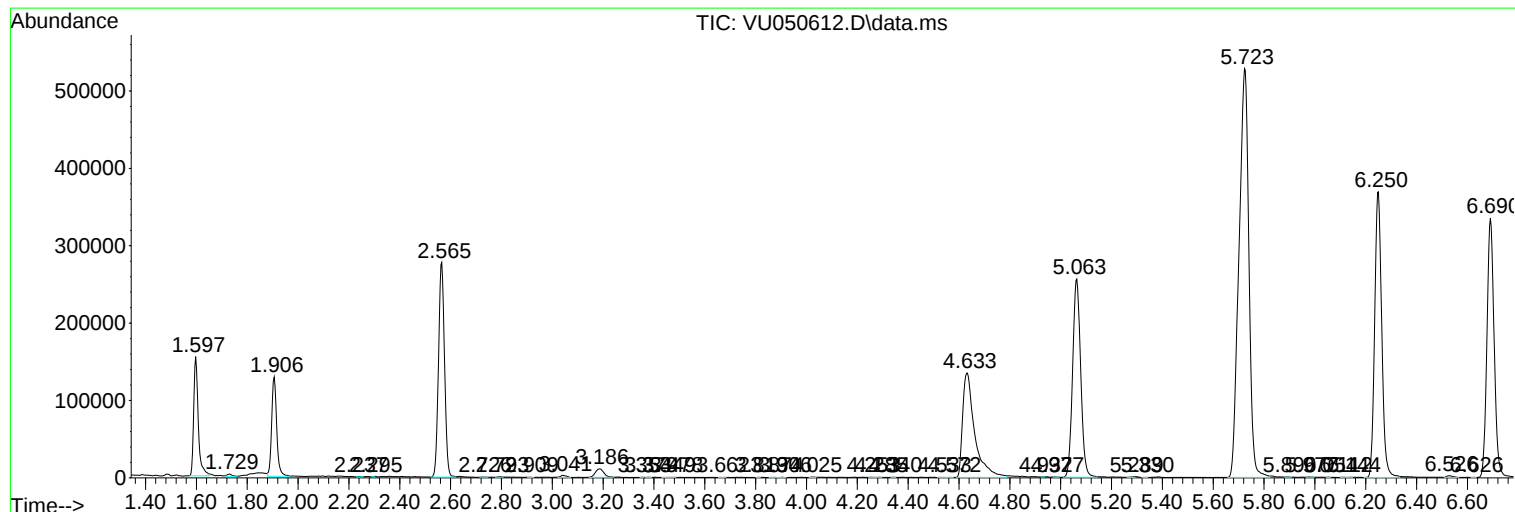

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050612.D
Acq On : 03 Sep 2022 15:13
Operator : SY/MD
Sample : N4458-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050612.D
Acq On : 03 Sep 2022 15:13
Operator : SY/MD
Sample : N4458-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------