

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050614.D
 Acq On : 03 Sep 2022 16:00
 Operator : SY/MD
 Sample : N4481-01 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050614.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	105	rBV	160485	205139	14.46%	2.005%
2	1.900	167	174	198	rVB	119988	169804	11.97%	1.659%
3	2.372	318	321	325	rBV2	464	466	0.03%	0.005%
4	2.478	351	354	356	rBV2	366	261	0.02%	0.003%
5	2.562	368	380	396	rBV	261137	421084	29.68%	4.115%
6	2.755	436	440	443	rBV3	348	288	0.02%	0.003%
7	2.787	443	450	451	rBV3	1081	1045	0.07%	0.010%
8	2.848	464	469	473	rVB3	328	340	0.02%	0.003%
9	2.919	483	491	507	rVV2	2388	5163	0.36%	0.050%
10	3.009	517	519	521	rBV2	297	192	0.01%	0.002%
11	3.044	521	530	541	rVB3	4241	7467	0.53%	0.073%
12	3.109	546	550	554	rVB	410	341	0.02%	0.003%
13	3.186	560	574	596	rBV	9145	21771	1.53%	0.213%
14	3.298	606	609	615	rVB2	185	183	0.01%	0.002%
15	3.359	619	628	632	rBV4	949	1214	0.09%	0.012%
16	3.453	654	657	660	rBV	290	181	0.01%	0.002%
17	3.491	665	669	677	rVV2	235	270	0.02%	0.003%
18	3.655	717	720	725	rVB	284	224	0.02%	0.002%
19	3.681	725	728	734	rBV	294	331	0.02%	0.003%
20	3.964	810	816	823	rBV2	298	393	0.03%	0.004%
21	4.099	856	858	862	rVB2	305	195	0.01%	0.002%
22	4.308	919	923	926	rBV	285	201	0.01%	0.002%
23	4.629	1009	1023	1066	rBV	119638	373332	26.32%	3.648%
24	5.063	1138	1158	1183	rBV	252758	557283	39.28%	5.446%
25	5.260	1215	1219	1220	rBV	269	210	0.01%	0.002%
26	5.433	1270	1273	1278	rVB	301	226	0.02%	0.002%
27	5.723	1342	1363	1399	rBV2	533078	1418600	100.00%	13.863%
28	5.877	1408	1411	1413	rBV	306	194	0.01%	0.002%
29	5.967	1437	1439	1442	rVB2	384	219	0.02%	0.002%
30	5.983	1442	1444	1448	rVB2	491	273	0.02%	0.003%
31	6.018	1453	1455	1462	rBV3	351	291	0.02%	0.003%
32	6.108	1480	1483	1486	rBV3	380	179	0.01%	0.002%
33	6.247	1511	1526	1555	rBV	379802	738583	52.06%	7.218%
34	6.388	1568	1570	1573	rVB2	506	277	0.02%	0.003%
35	6.411	1573	1577	1580	rBV4	620	558	0.04%	0.005%
36	6.465	1591	1594	1598	rBV3	241	270	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050614.D
 Acq On : 03 Sep 2022 16:00
 Operator : SY/MD
 Sample : N4481-01 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	6.526	1607	1613	1615	rBV4	1608	1850	0.13%	0.018%
38	6.578	1625	1629	1631	rBV	236	178	0.01%	0.002%
39	6.613	1637	1640	1643	rVB3	513	306	0.02%	0.003%
40	6.690	1648	1664	1686	rBV	342305	675637	47.63%	6.603%
41	6.922	1733	1736	1742	rVB2	229	244	0.02%	0.002%
42	6.977	1749	1753	1756	rBV2	204	187	0.01%	0.002%
43	7.047	1771	1775	1780	rBV3	496	490	0.03%	0.005%
44	7.182	1811	1817	1819	rBV4	991	996	0.07%	0.010%
45	7.565	1920	1936	1958	rBV	150129	269491	19.00%	2.634%
46	7.687	1971	1974	1982	rVB4	703	873	0.06%	0.009%
47	7.780	1999	2003	2005	rBV3	387	299	0.02%	0.003%
48	7.899	2025	2040	2069	rBV	625082	1095877	77.25%	10.709%
49	8.128	2109	2111	2114	rVB3	380	203	0.01%	0.002%
50	8.179	2114	2127	2145	rBV	98814	173342	12.22%	1.694%
51	8.301	2163	2165	2172	rVB4	388	363	0.03%	0.004%
52	8.346	2176	2179	2182	rBV2	375	215	0.02%	0.002%
53	8.382	2187	2190	2192	rBV2	277	214	0.02%	0.002%
54	8.510	2226	2230	2234	rVB2	272	213	0.02%	0.002%
55	8.533	2234	2237	2239	rBV	244	181	0.01%	0.002%
56	8.639	2255	2270	2311	rBV5	271998	797058	56.19%	7.789%
57	8.864	2337	2340	2350	rVB5	657	837	0.06%	0.008%
58	8.912	2353	2355	2359	rVB3	535	319	0.02%	0.003%
59	9.028	2386	2391	2396	rBV2	197	217	0.02%	0.002%
60	9.169	2432	2435	2438	rBV2	309	184	0.01%	0.002%
61	9.214	2443	2449	2457	rVB5	1619	2271	0.16%	0.022%
62	9.263	2457	2464	2467	rBV2	184	205	0.01%	0.002%
63	9.333	2481	2486	2489	rBV2	276	231	0.02%	0.002%
64	9.417	2498	2512	2539	rBV	547038	917615	64.68%	8.967%
65	9.558	2552	2556	2559	rBV2	241	248	0.02%	0.002%
66	9.578	2559	2562	2566	rVB2	793	642	0.05%	0.006%
67	9.703	2599	2601	2605	rVB2	416	250	0.02%	0.002%
68	9.848	2643	2646	2652	rVB2	221	226	0.02%	0.002%
69	9.880	2652	2656	2659	rBV2	336	223	0.02%	0.002%
70	9.922	2666	2669	2673	rVB2	317	203	0.01%	0.002%
71	10.099	2719	2724	2727	rBV2	533	610	0.04%	0.006%
72	10.247	2767	2770	2773	rBV	272	224	0.02%	0.002%
73	10.340	2795	2799	2802	rVB	363	242	0.02%	0.002%
74	10.365	2802	2807	2810	rBV2	255	319	0.02%	0.003%
75	10.385	2810	2813	2818	rVB2	235	219	0.02%	0.002%
76	10.430	2824	2827	2832	rVB2	314	251	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050614.D
 Acq On : 03 Sep 2022 16:00
 Operator : SY/MD
 Sample : N4481-01 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

77	10.626	2884	2888	2891	rBV2	331	316	0.02%	0.003%
78	10.677	2902	2904	2911	rVB	303	251	0.02%	0.002%
79	10.755	2916	2928	2949	rBV	490282	802035	56.54%	7.838%
80	10.854	2956	2959	2962	rBV3	372	243	0.02%	0.002%
81	11.092	3031	3033	3037	rVB2	383	251	0.02%	0.002%
82	11.246	3077	3081	3083	rBV2	232	205	0.01%	0.002%
83	11.459	3143	3147	3150	rBV3	393	398	0.03%	0.004%
84	11.481	3151	3154	3160	rVB2	512	541	0.04%	0.005%
85	11.748	3234	3237	3244	rBV3	777	657	0.05%	0.006%
86	11.812	3244	3257	3276	rBV	425296	693620	48.89%	6.778%
87	12.025	3319	3323	3325	rBV3	452	312	0.02%	0.003%
88	12.192	3362	3375	3398	rBV	520797	857048	60.42%	8.375%
89	12.449	3453	3455	3458	rVB2	420	211	0.01%	0.002%
90	12.812	3565	3568	3573	rBV2	469	351	0.02%	0.003%
91	13.012	3627	3630	3634	rVB2	373	317	0.02%	0.003%
92	13.201	3686	3689	3692	rVB	676	476	0.03%	0.005%
93	13.221	3692	3695	3697	rBV2	536	356	0.03%	0.003%
94	13.234	3697	3699	3701	rVB	515	270	0.02%	0.003%
95	13.336	3728	3731	3733	rBV2	464	290	0.02%	0.003%
96	13.388	3744	3747	3749	rBV	391	221	0.02%	0.002%
97	13.539	3791	3794	3795	rBV2	338	207	0.01%	0.002%
98	13.626	3817	3821	3824	rBV	560	447	0.03%	0.004%
99	13.854	3883	3892	3896	rBV5	1800	2618	0.18%	0.026%
100	15.552	4417	4420	4421	rBV	614	380	0.03%	0.004%




Sum of corrected areas: 10232822

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050614.D
Acq On : 03 Sep 2022 16:00
Operator : SY/MD
Sample : N4481-01 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

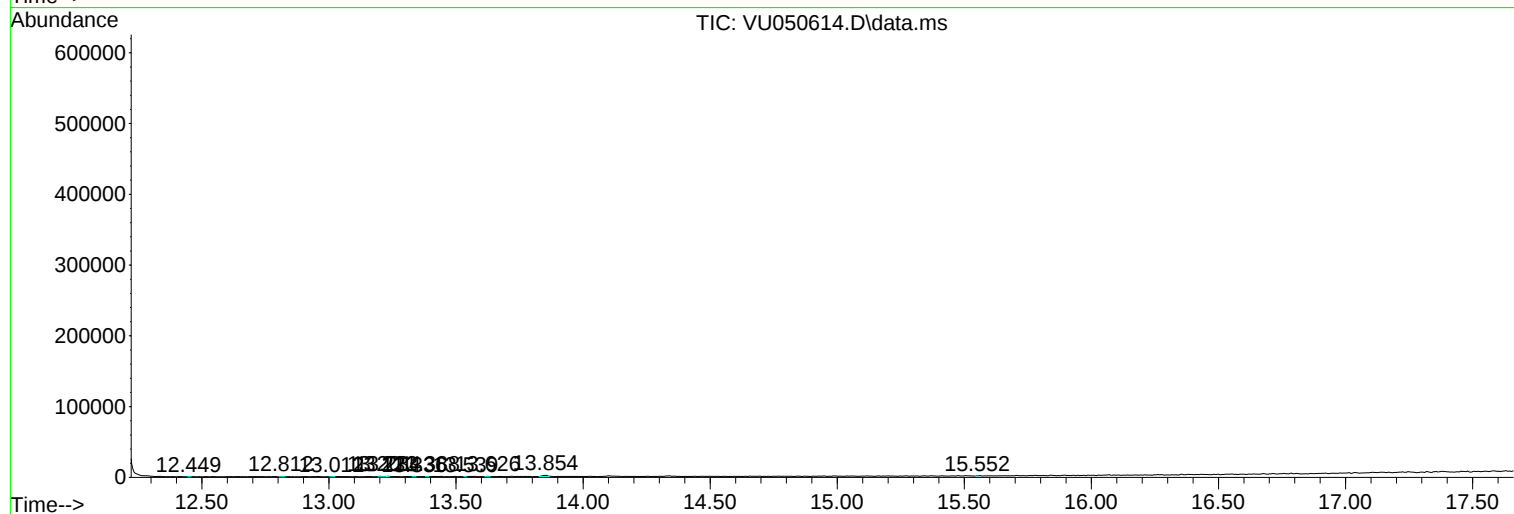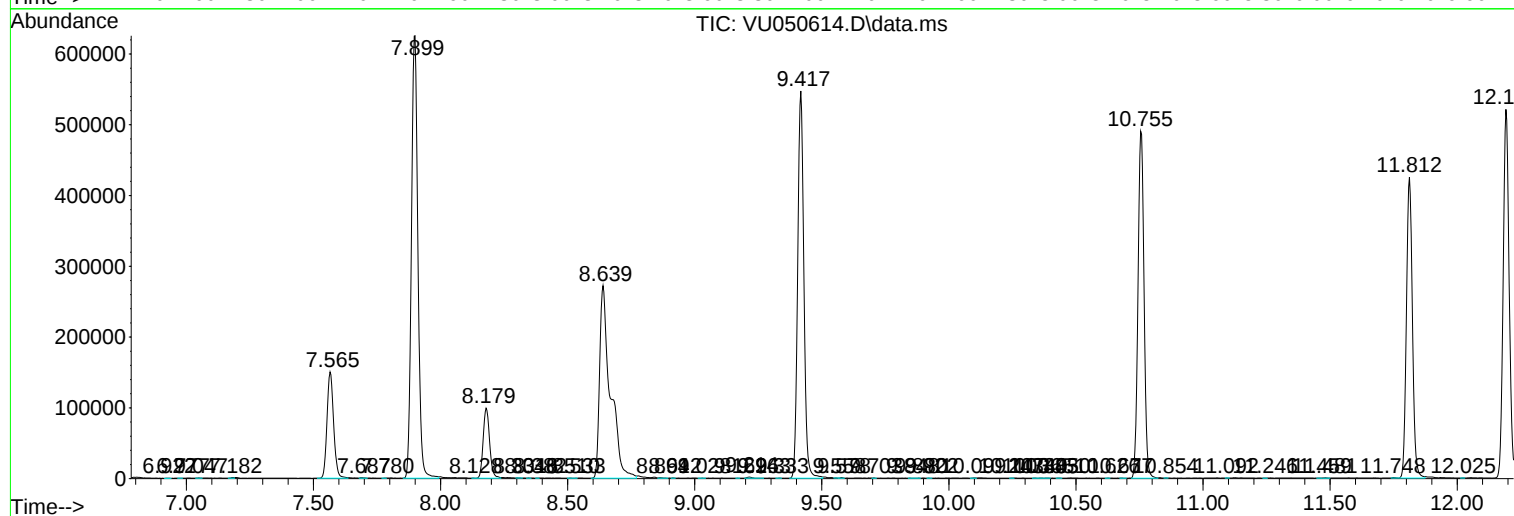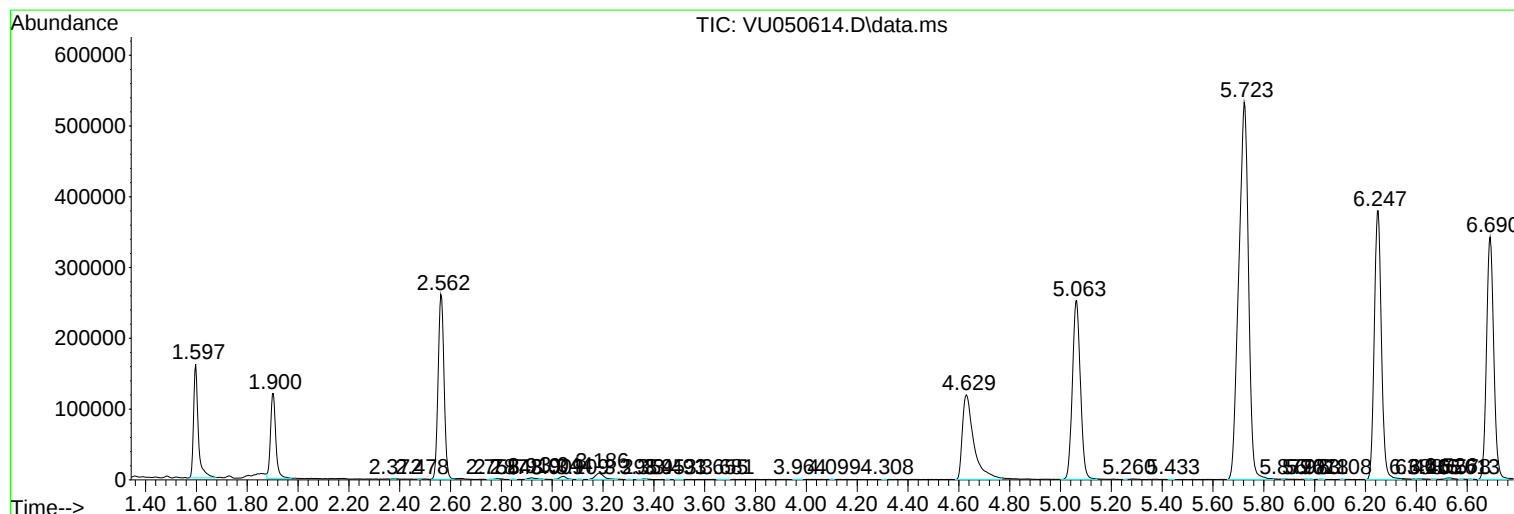

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050614.D
Acq On : 03 Sep 2022 16:00
Operator : SY/MD
Sample : N4481-01 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050614.D
Acq On : 03 Sep 2022 16:00
Operator : SY/MD
Sample : N4481-01 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------