

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050615.D
 Acq On : 03 Sep 2022 16:23
 Operator : SY/MD
 Sample : N4481-02 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050615.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	51	rBV3	2939	3455	0.23%	0.031%
2	1.597	72	80	102	rBV	150837	187786	12.27%	1.700%
3	1.906	168	176	190	rVB	132048	174879	11.43%	1.583%
4	2.565	368	381	395	rBV	293929	475384	31.07%	4.304%
5	2.636	395	403	424	rVB	10704	20849	1.36%	0.189%
6	2.742	433	436	440	rVB3	415	305	0.02%	0.003%
7	2.784	444	449	450	rBV	1303	974	0.06%	0.009%
8	2.954	498	502	504	rBV2	303	230	0.02%	0.002%
9	3.041	521	529	530	rBV2	4036	3781	0.25%	0.034%
10	3.186	560	574	587	rBV	7068	15797	1.03%	0.143%
11	3.340	619	622	627	rVB2	196	195	0.01%	0.002%
12	3.366	627	630	634	rBV3	249	195	0.01%	0.002%
13	3.407	638	643	647	rBV2	199	214	0.01%	0.002%
14	3.475	660	664	667	rBV2	291	227	0.01%	0.002%
15	3.510	671	675	683	rVB2	324	403	0.03%	0.004%
16	3.565	688	692	696	rBV	351	291	0.02%	0.003%
17	3.597	696	702	706	rBV2	220	230	0.02%	0.002%
18	3.877	785	789	792	rVB	273	207	0.01%	0.002%
19	3.954	809	813	820	rVV2	290	323	0.02%	0.003%
20	4.009	827	830	835	rVV	285	264	0.02%	0.002%
21	4.102	846	859	863	rBV3	9970	22695	1.48%	0.205%
22	4.375	940	944	947	rVB	307	258	0.02%	0.002%
23	4.433	955	962	964	rBV	240	244	0.02%	0.002%
24	4.494	978	981	987	rVB2	207	217	0.01%	0.002%
25	4.629	1009	1023	1065	rBV	137982	435976	28.50%	3.947%
26	5.063	1140	1158	1181	rBV	270373	598569	39.13%	5.419%
27	5.276	1220	1224	1225	rBV2	529	337	0.02%	0.003%
28	5.288	1225	1228	1231	rVV	469	366	0.02%	0.003%
29	5.375	1249	1255	1256	rVV3	512	521	0.03%	0.005%
30	5.497	1288	1293	1300	rBV2	178	230	0.02%	0.002%
31	5.568	1313	1315	1321	rVB	297	207	0.01%	0.002%
32	5.726	1342	1364	1391	rBV2	569172	1529887	100.00%	13.850%
33	5.886	1412	1414	1417	rVB3	681	346	0.02%	0.003%
34	5.970	1437	1440	1443	rBV2	283	185	0.01%	0.002%
35	5.999	1447	1449	1453	rVB2	461	263	0.02%	0.002%
36	6.022	1453	1456	1457	rBV2	289	186	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050615.D
 Acq On : 03 Sep 2022 16:23
 Operator : SY/MD
 Sample : N4481-02 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	6.128	1483	1489	1492	rVB4	466	474	0.03%	0.004%
38	6.250	1511	1527	1554	rBV	416415	807022	52.75%	7.306%
39	6.404	1573	1575	1579	rVB3	587	318	0.02%	0.003%
40	6.501	1602	1605	1606	rBV2	495	315	0.02%	0.003%
41	6.533	1607	1615	1627	rVB7	2605	4886	0.32%	0.044%
42	6.623	1640	1643	1649	rVB5	607	525	0.03%	0.005%
43	6.690	1649	1664	1690	rBV	372851	733063	47.92%	6.636%
44	7.128	1794	1800	1803	rBV2	224	201	0.01%	0.002%
45	7.173	1811	1814	1816	rBV2	592	437	0.03%	0.004%
46	7.301	1851	1854	1862	rVB	454	446	0.03%	0.004%
47	7.365	1867	1874	1878	rBV	319	348	0.02%	0.003%
48	7.388	1878	1881	1887	rVB2	225	211	0.01%	0.002%
49	7.510	1915	1919	1922	rBV2	304	237	0.02%	0.002%
50	7.565	1923	1936	1961	rBV	154032	280152	18.31%	2.536%
51	7.851	2021	2025	2026	rBV2	337	193	0.01%	0.002%
52	7.899	2026	2040	2062	rBV	699472	1219789	79.73%	11.043%
53	8.179	2116	2127	2147	rVV	97195	167243	10.93%	1.514%
54	8.250	2147	2149	2151	rVB2	547	208	0.01%	0.002%
55	8.317	2166	2170	2175	rVB4	494	488	0.03%	0.004%
56	8.414	2194	2200	2202	rBV3	481	447	0.03%	0.004%
57	8.552	2237	2243	2245	rBV4	627	579	0.04%	0.005%
58	8.639	2257	2270	2280	rBV4	309280	684393	44.73%	6.196%
59	8.851	2334	2336	2340	rVB2	867	542	0.04%	0.005%
60	8.870	2340	2342	2348	rVB4	474	487	0.03%	0.004%
61	8.902	2349	2352	2360	rVB3	519	549	0.04%	0.005%
62	9.256	2459	2462	2466	rVB2	427	349	0.02%	0.003%
63	9.288	2466	2472	2473	rBV2	239	229	0.01%	0.002%
64	9.417	2499	2512	2545	rBV	638504	1077554	70.43%	9.755%
65	9.619	2572	2575	2577	rBV3	352	197	0.01%	0.002%
66	9.636	2577	2580	2585	rVB2	836	679	0.04%	0.006%
67	9.658	2585	2587	2590	rBV3	618	453	0.03%	0.004%
68	9.799	2628	2631	2637	rVB2	261	245	0.02%	0.002%
69	9.918	2665	2668	2675	rBV2	199	248	0.02%	0.002%
70	9.989	2685	2690	2693	rBV	483	388	0.03%	0.004%
71	10.102	2719	2725	2732	rVB3	765	997	0.07%	0.009%
72	10.246	2766	2770	2775	rBV2	226	190	0.01%	0.002%
73	10.333	2794	2797	2801	rVB2	292	192	0.01%	0.002%
74	10.754	2914	2928	2949	rBV	535668	882090	57.66%	7.985%
75	11.008	3004	3007	3008	rBV	278	200	0.01%	0.002%
76	11.410	3129	3132	3138	rVB2	509	391	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050615.D
 Acq On : 03 Sep 2022 16:23
 Operator : SY/MD
 Sample : N4481-02 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

77	11.468	3146	3150	3156	rVB3	502	574	0.04%	0.005%
78	11.751	3233	3238	3244	rVB2	864	835	0.05%	0.008%
79	11.812	3244	3257	3284	rBV	487002	803561	52.52%	7.274%
80	11.973	3305	3307	3313	rVB3	429	382	0.02%	0.003%
81	12.192	3363	3375	3392	rBV	534523	885927	57.91%	8.020%
82	12.346	3421	3423	3425	rBV2	297	190	0.01%	0.002%
83	12.433	3448	3450	3457	rVB3	391	339	0.02%	0.003%
84	12.523	3475	3478	3485	rVB3	591	587	0.04%	0.005%
85	12.905	3593	3597	3601	rBV4	299	255	0.02%	0.002%
86	12.970	3613	3617	3620	rBV2	411	323	0.02%	0.003%
87	12.999	3623	3626	3627	rBV2	446	245	0.02%	0.002%
88	13.063	3643	3646	3648	rBV2	400	221	0.01%	0.002%
89	13.513	3781	3786	3788	rBV3	415	452	0.03%	0.004%
90	13.655	3828	3830	3835	rVB2	668	481	0.03%	0.004%
91	13.844	3885	3889	3902	rVB6	1388	2132	0.14%	0.019%
92	14.098	3961	3968	3969	rBV3	1225	1225	0.08%	0.011%
93	14.333	4036	4041	4046	rBV3	810	950	0.06%	0.009%
94	14.420	4065	4068	4070	rBV2	295	202	0.01%	0.002%
95	14.503	4090	4094	4098	rBV2	475	553	0.04%	0.005%
96	14.577	4114	4117	4124	rVB2	383	364	0.02%	0.003%
97	14.616	4124	4129	4133	rBV2	422	568	0.04%	0.005%
98	14.764	4171	4175	4179	rBV3	691	571	0.04%	0.005%
99	15.015	4250	4253	4256	rBV2	634	334	0.02%	0.003%
100	15.822	4501	4504	4506	rBV3	797	609	0.04%	0.006%




Sum of corrected areas: 11046311

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050615.D
Acq On : 03 Sep 2022 16:23
Operator : SY/MD
Sample : N4481-02 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

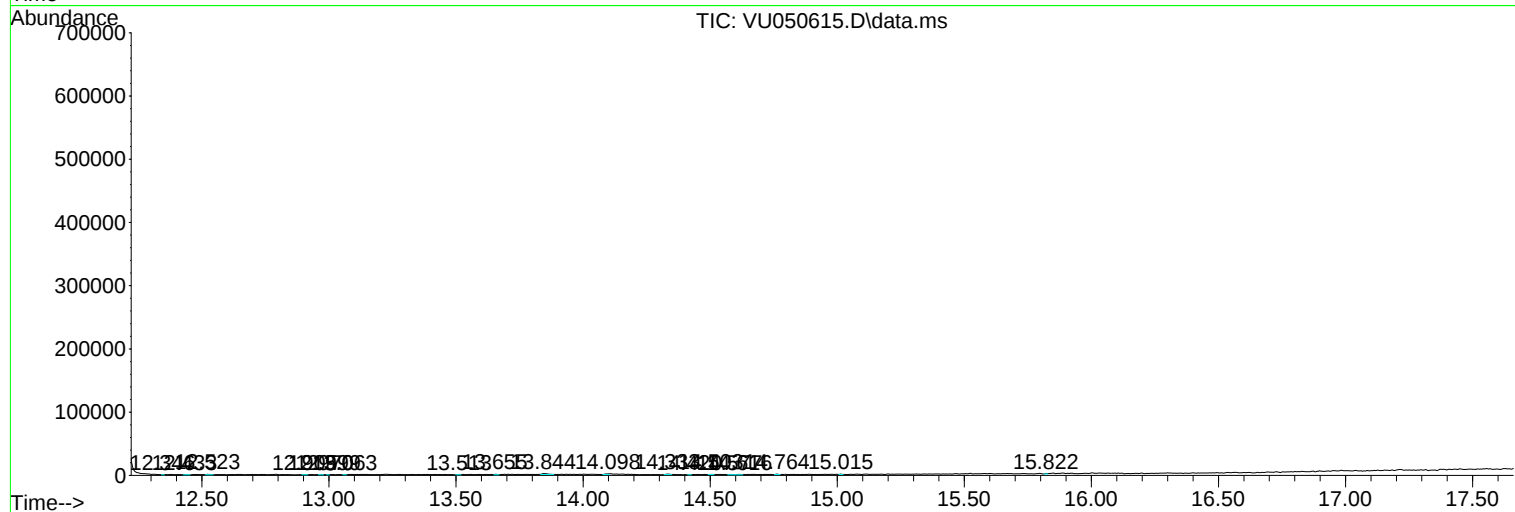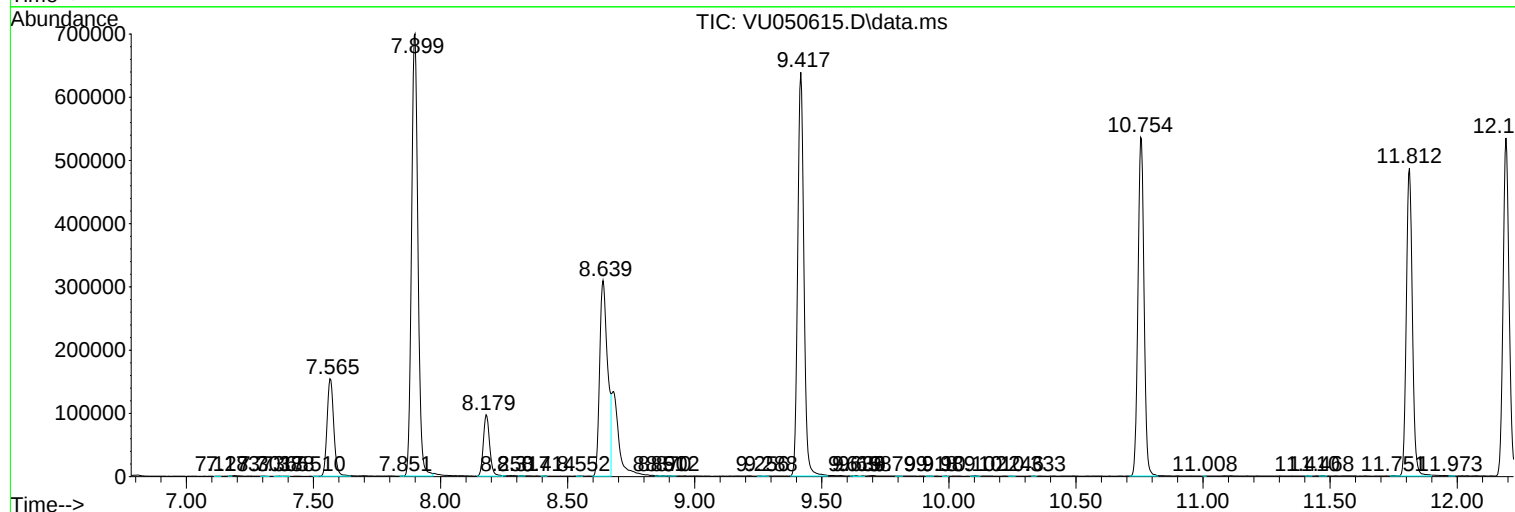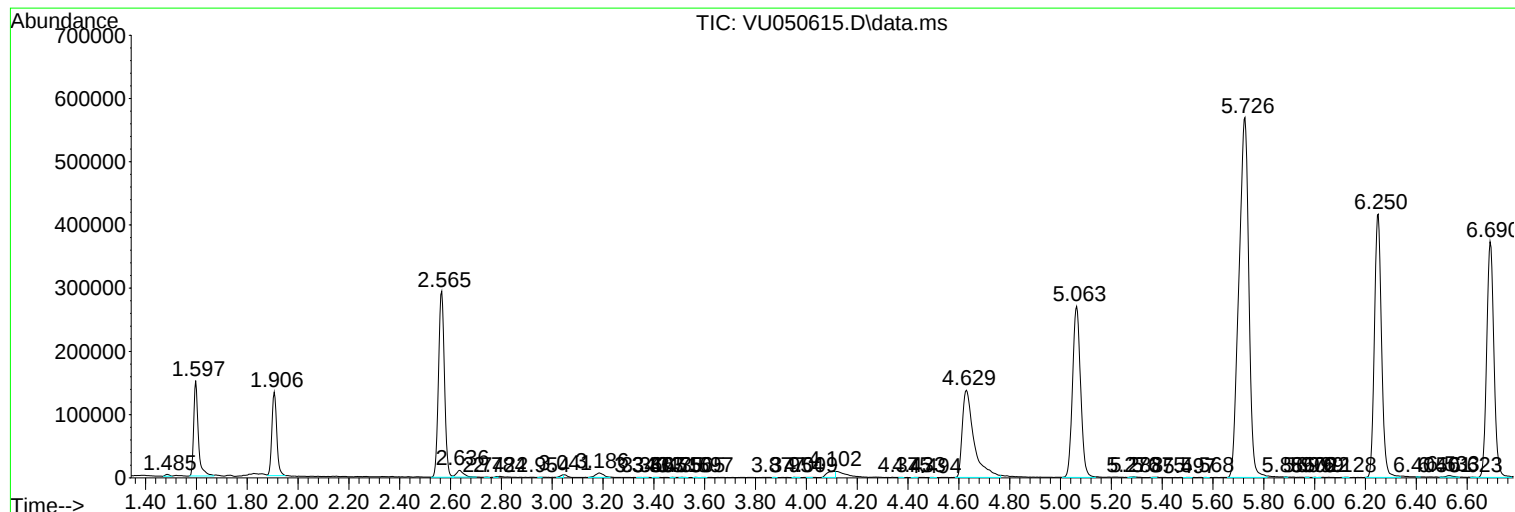

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050615.D
Acq On : 03 Sep 2022 16:23
Operator : SY/MD
Sample : N4481-02 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050615.D
Acq On : 03 Sep 2022 16:23
Operator : SY/MD
Sample : N4481-02 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc