

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050616.D
 Acq On : 03 Sep 2022 16:46
 Operator : SY/MD
 Sample : N4481-03 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050616.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	50	rBV2	2576	2653	0.21%	0.028%
2	1.597	72	80	105	rBV	231658	293829	22.73%	3.058%
3	1.903	167	175	205	rVB	202258	281866	21.81%	2.933%
4	2.562	368	380	396	rBV	387468	628558	48.63%	6.541%
5	2.919	487	491	493	rBV2	600	409	0.03%	0.004%
6	3.044	520	530	543	rVB	6125	11218	0.87%	0.117%
7	3.186	561	574	593	rBV	7209	17110	1.32%	0.178%
8	3.398	637	640	650	rVB2	506	515	0.04%	0.005%
9	3.446	652	655	659	rVB2	338	257	0.02%	0.003%
10	3.523	674	679	681	rBV2	368	275	0.02%	0.003%
11	3.546	682	686	693	rVB2	462	548	0.04%	0.006%
12	3.581	693	697	699	rBV2	298	223	0.02%	0.002%
13	3.665	721	723	727	rBV	360	299	0.02%	0.003%
14	3.806	764	767	772	rVB2	361	249	0.02%	0.003%
15	4.012	828	831	837	rVB2	369	317	0.02%	0.003%
16	4.044	838	841	845	rBV	399	278	0.02%	0.003%
17	4.317	924	926	930	rVB	365	223	0.02%	0.002%
18	4.385	944	947	949	rBV	241	188	0.01%	0.002%
19	4.440	962	964	975	rVB	190	217	0.02%	0.002%
20	4.629	1009	1023	1069	rBV	160554	516979	40.00%	5.380%
21	4.932	1112	1117	1122	rVB	701	686	0.05%	0.007%
22	4.954	1122	1124	1126	rBV2	461	230	0.02%	0.002%
23	5.060	1141	1157	1188	rBV2	326691	737139	57.03%	7.671%
24	5.276	1221	1224	1225	rBV	533	252	0.02%	0.003%
25	5.427	1265	1271	1276	rVB2	262	287	0.02%	0.003%
26	5.501	1292	1294	1300	rVB2	281	203	0.02%	0.002%
27	5.555	1306	1311	1314	rBV	287	225	0.02%	0.002%
28	5.723	1337	1363	1396	rBV2	478106	1292443	100.00%	13.450%
29	5.870	1406	1409	1414	rBV3	474	324	0.03%	0.003%
30	5.983	1440	1444	1447	rVB3	602	594	0.05%	0.006%
31	6.070	1467	1471	1474	rBV	273	245	0.02%	0.003%
32	6.108	1479	1483	1487	rBV2	331	272	0.02%	0.003%
33	6.137	1490	1492	1495	rVB	442	240	0.02%	0.002%
34	6.247	1510	1526	1545	rBV	342950	652840	50.51%	6.794%
35	6.533	1605	1615	1619	rBV7	2231	3520	0.27%	0.037%
36	6.690	1649	1664	1685	rBV	299045	587917	45.49%	6.118%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050616.D
 Acq On : 03 Sep 2022 16:46
 Operator : SY/MD
 Sample : N4481-03 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	6.912	1730	1733	1737	rVV2	217	172	0.01%	0.002%
38	6.944	1741	1743	1746	rVV2	378	182	0.01%	0.002%
39	6.964	1746	1749	1753	rVB2	206	171	0.01%	0.002%
40	7.060	1775	1779	1783	rVB2	351	278	0.02%	0.003%
41	7.186	1815	1818	1819	rBV2	619	373	0.03%	0.004%
42	7.420	1886	1891	1893	rBV	177	177	0.01%	0.002%
43	7.565	1923	1936	1955	rBV	124540	223047	17.26%	2.321%
44	7.838	2015	2021	2024	rBV2	213	238	0.02%	0.002%
45	7.899	2025	2040	2068	rBV	529906	937737	72.56%	9.759%
46	8.179	2114	2127	2145	rBV2	86019	146933	11.37%	1.529%
47	8.285	2155	2160	2163	rBV4	331	411	0.03%	0.004%
48	8.327	2168	2173	2177	rBV3	459	469	0.04%	0.005%
49	8.446	2208	2210	2216	rVB2	273	206	0.02%	0.002%
50	8.494	2221	2225	2227	rBV2	266	185	0.01%	0.002%
51	8.552	2234	2243	2252	rBV5	5628	9360	0.72%	0.097%
52	8.639	2257	2270	2280	rBV4	214060	468301	36.23%	4.873%
53	9.005	2381	2384	2389	rBV2	321	262	0.02%	0.003%
54	9.150	2423	2429	2435	rBV2	260	400	0.03%	0.004%
55	9.417	2499	2512	2551	rVV	462174	789195	61.06%	8.213%
56	9.565	2555	2558	2560	rVV2	352	182	0.01%	0.002%
57	9.693	2594	2598	2605	rVB3	704	779	0.06%	0.008%
58	9.812	2628	2635	2638	rBV	298	406	0.03%	0.004%
59	10.099	2720	2724	2727	rBV2	339	294	0.02%	0.003%
60	10.118	2727	2730	2733	rVV	261	168	0.01%	0.002%
61	10.182	2742	2750	2752	rBV	379	420	0.03%	0.004%
62	10.526	2854	2857	2860	rVB2	291	173	0.01%	0.002%
63	10.591	2875	2877	2882	rVV	233	183	0.01%	0.002%
64	10.652	2892	2896	2901	rBV2	258	239	0.02%	0.002%
65	10.755	2916	2928	2955	rVV	421006	680572	52.66%	7.082%
66	11.070	3020	3026	3028	rBV	162	170	0.01%	0.002%
67	11.095	3029	3034	3038	rVV3	438	431	0.03%	0.004%
68	11.118	3038	3041	3045	rVB3	489	359	0.03%	0.004%
69	11.272	3084	3089	3092	rBV2	255	244	0.02%	0.003%
70	11.455	3143	3146	3148	rBV2	322	208	0.02%	0.002%
71	11.510	3160	3163	3168	rVB	342	292	0.02%	0.003%
72	11.542	3168	3173	3177	rBV2	245	332	0.03%	0.003%
73	11.748	3233	3237	3241	rVB3	583	459	0.04%	0.005%
74	11.812	3244	3257	3280	rBV	361066	577738	44.70%	6.012%
75	11.999	3312	3315	3319	rVB2	481	306	0.02%	0.003%
76	12.086	3340	3342	3346	rBV2	236	174	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050616.D
 Acq On : 03 Sep 2022 16:46
 Operator : SY/MD
 Sample : N4481-03 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

77	12.108	3347	3349	3353	rVB2	356	232	0.02%	0.002%
78	12.192	3362	3375	3398	rBV	442013	727409	56.28%	7.570%
79	12.356	3424	3426	3431	rBV2	411	344	0.03%	0.004%
80	12.394	3433	3438	3439	rBV2	305	237	0.02%	0.002%
81	12.423	3445	3447	3456	rVB2	168	190	0.01%	0.002%
82	12.523	3476	3478	3482	rVB	286	197	0.02%	0.002%
83	12.562	3488	3490	3495	rBV2	364	283	0.02%	0.003%
84	12.642	3513	3515	3519	rVB3	351	206	0.02%	0.002%
85	12.697	3528	3532	3535	rBV	267	267	0.02%	0.003%
86	12.790	3558	3561	3565	rBV	317	257	0.02%	0.003%
87	13.031	3633	3636	3639	rBV	313	179	0.01%	0.002%
88	13.102	3655	3658	3663	rVV	264	273	0.02%	0.003%
89	13.153	3671	3674	3676	rBV2	342	236	0.02%	0.002%
90	13.221	3693	3695	3698	rBV	345	250	0.02%	0.003%
91	13.385	3741	3746	3749	rBV2	400	395	0.03%	0.004%
92	13.433	3758	3761	3764	rBV2	434	274	0.02%	0.003%
93	13.571	3800	3804	3807	rBV2	325	288	0.02%	0.003%
94	13.613	3814	3817	3820	rBV2	352	288	0.02%	0.003%
95	13.655	3827	3830	3833	rBV2	259	193	0.01%	0.002%
96	13.754	3858	3861	3863	rBV2	419	300	0.02%	0.003%
97	14.066	3955	3958	3961	rBV	346	206	0.02%	0.002%
98	15.076	4270	4272	4275	rBV2	449	267	0.02%	0.003%
99	15.349	4355	4357	4361	rBV3	412	235	0.02%	0.002%
100	15.893	4524	4526	4528	rBV2	804	398	0.03%	0.004%




Sum of corrected areas: 9609258

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050616.D
Acq On : 03 Sep 2022 16:46
Operator : SY/MD
Sample : N4481-03 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

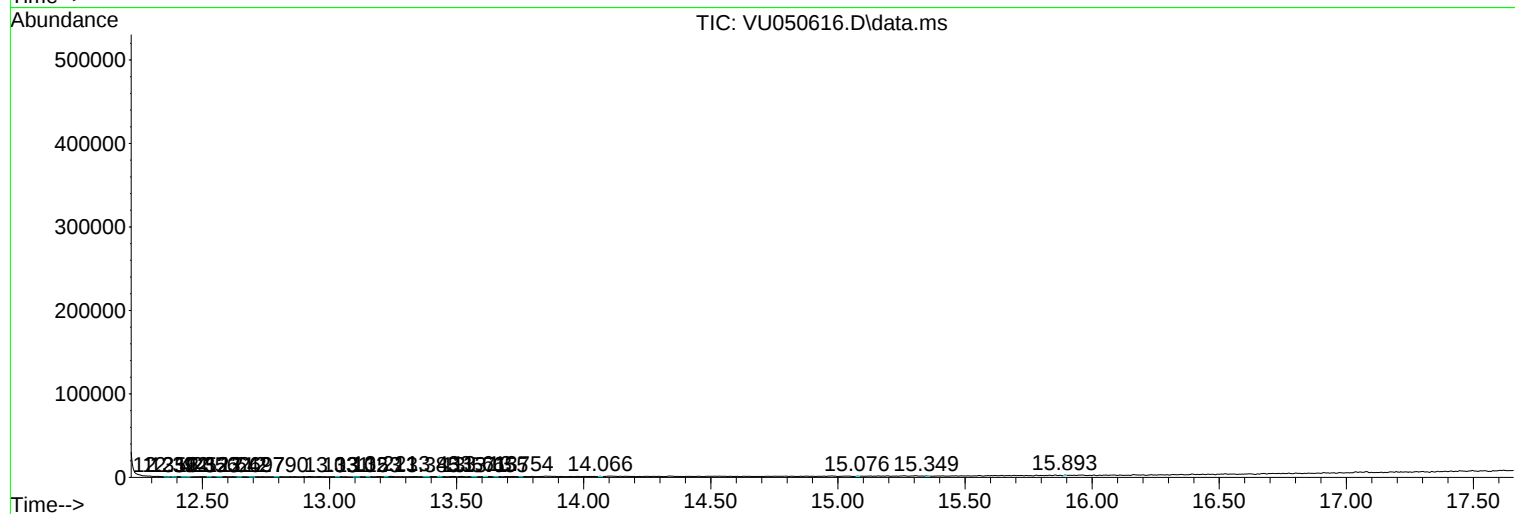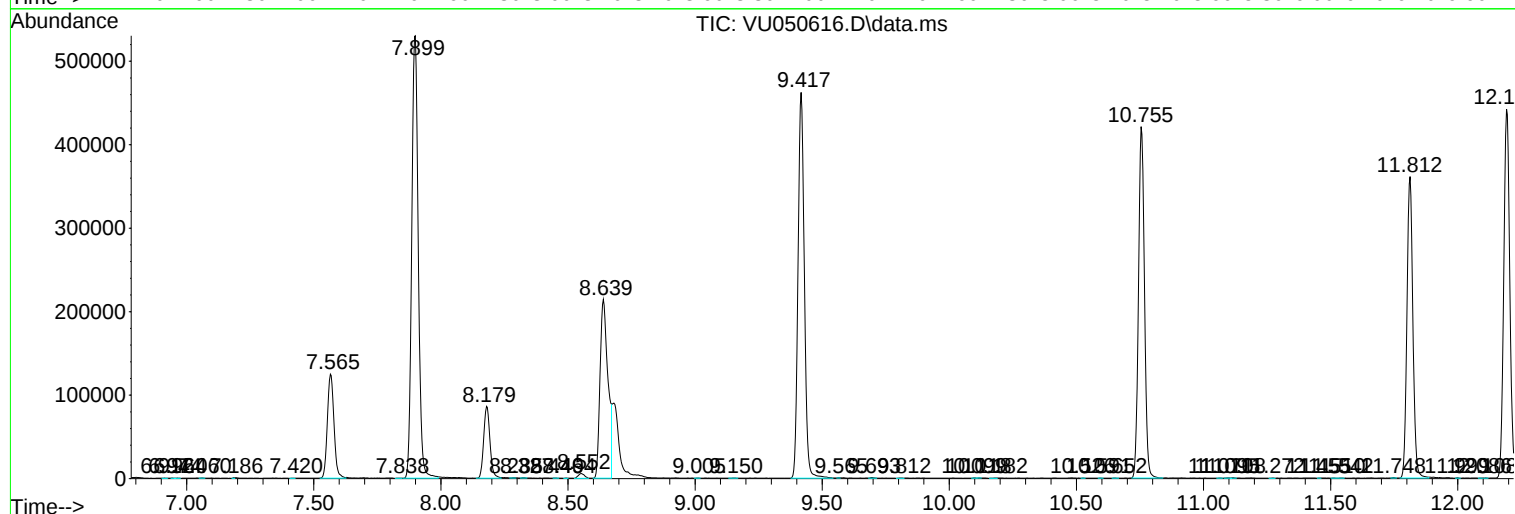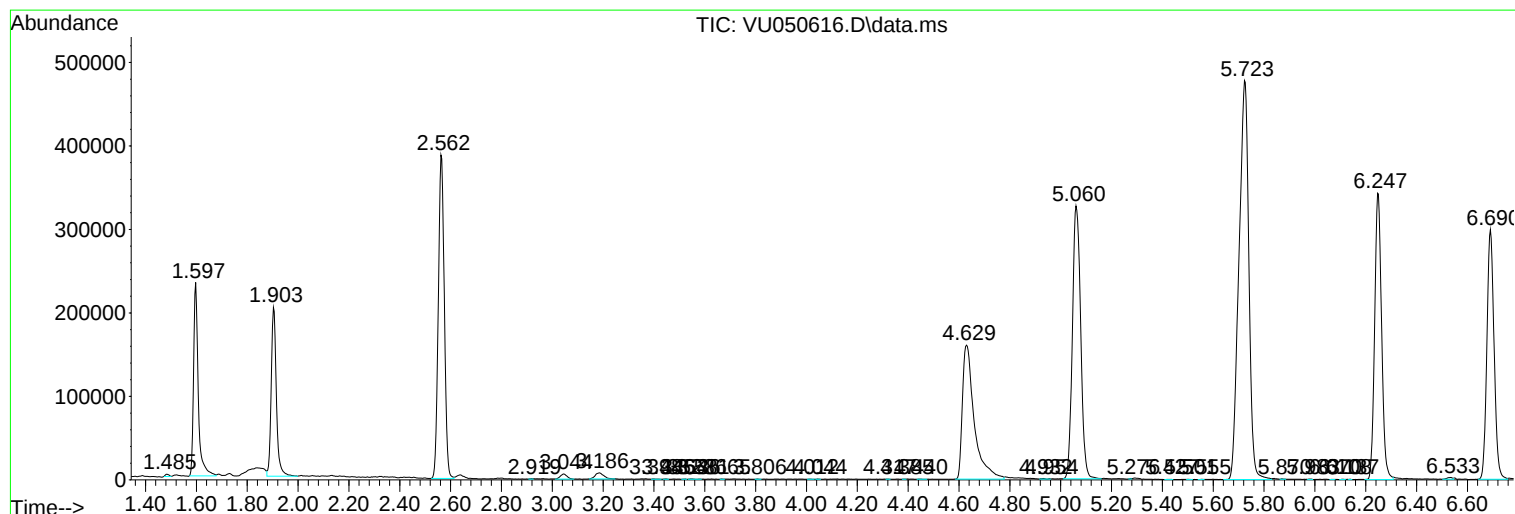

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050616.D
Acq On : 03 Sep 2022 16:46
Operator : SY/MD
Sample : N4481-03 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050616.D
Acq On : 03 Sep 2022 16:46
Operator : SY/MD
Sample : N4481-03 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------