

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050617.D
 Acq On : 03 Sep 2022 17:10
 Operator : SY/MD
 Sample : N4481-04 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050617.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	51	rVB3	2937	3129	0.23%	0.033%
2	1.597	71	80	102	rBV	139632	174159	12.89%	1.838%
3	1.729	117	121	130	rVB3	3101	3701	0.27%	0.039%
4	1.906	167	176	195	rVB	114185	153929	11.39%	1.625%
5	2.099	234	236	238	rBV2	525	286	0.02%	0.003%
6	2.356	312	316	319	rBV3	565	502	0.04%	0.005%
7	2.562	368	380	396	rBV	260173	424796	31.43%	4.484%
8	2.787	443	450	454	rBV2	806	898	0.07%	0.009%
9	2.851	467	470	475	rBV	370	277	0.02%	0.003%
10	2.922	488	492	496	rBV2	341	333	0.02%	0.004%
11	3.006	516	518	521	rVV	260	147	0.01%	0.002%
12	3.041	521	529	541	rVV3	3710	6938	0.51%	0.073%
13	3.186	560	574	588	rBV	9717	21556	1.59%	0.228%
14	3.330	613	619	621	rBV	169	186	0.01%	0.002%
15	3.356	621	627	632	rVV2	190	266	0.02%	0.003%
16	3.536	679	683	688	rVB2	330	318	0.02%	0.003%
17	3.562	688	691	695	rBV	246	205	0.02%	0.002%
18	3.684	727	729	731	rBV2	403	169	0.01%	0.002%
19	3.726	738	742	747	rBV	459	423	0.03%	0.004%
20	3.916	795	801	804	rBV2	236	242	0.02%	0.003%
21	3.964	813	816	820	rBV2	202	181	0.01%	0.002%
22	4.128	863	867	871	rBV2	223	223	0.02%	0.002%
23	4.626	1009	1022	1075	rBV2	119721	378800	28.03%	3.998%
24	4.916	1110	1112	1116	rVB4	306	173	0.01%	0.002%
25	5.063	1142	1158	1185	rVB	244084	535866	39.65%	5.656%
26	5.160	1185	1188	1192	rBV3	325	308	0.02%	0.003%
27	5.205	1200	1202	1204	rBV	291	174	0.01%	0.002%
28	5.289	1219	1228	1237	rBV4	898	1724	0.13%	0.018%
29	5.356	1243	1249	1251	rBV2	214	209	0.02%	0.002%
30	5.456	1277	1280	1284	rVB	284	168	0.01%	0.002%
31	5.523	1299	1301	1305	rVB	427	232	0.02%	0.002%
32	5.565	1311	1314	1317	rBV	277	262	0.02%	0.003%
33	5.639	1334	1337	1340	rBV2	248	227	0.02%	0.002%
34	5.723	1342	1363	1385	rBV2	503779	1351575	100.00%	14.265%
35	5.903	1417	1419	1424	rVB2	542	350	0.03%	0.004%
36	5.977	1436	1442	1445	rBV2	356	389	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050617.D
 Acq On : 03 Sep 2022 17:10
 Operator : SY/MD
 Sample : N4481-04 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	6.057	1465	1467	1473	rVV3	299	292	0.02%	0.003%
38	6.105	1478	1482	1485	rBV2	333	295	0.02%	0.003%
39	6.250	1511	1527	1553	rBV	358774	695270	51.44%	7.338%
40	6.433	1582	1584	1587	rBV3	285	186	0.01%	0.002%
41	6.475	1593	1597	1599	rBV2	374	246	0.02%	0.003%
42	6.539	1606	1617	1622	rBV9	2624	4351	0.32%	0.046%
43	6.597	1631	1635	1638	rBV2	302	309	0.02%	0.003%
44	6.690	1649	1664	1696	rVV	319477	630608	46.66%	6.656%
45	6.854	1713	1715	1719	rVB2	365	206	0.02%	0.002%
46	6.961	1745	1748	1753	rVB2	529	411	0.03%	0.004%
47	6.993	1753	1758	1761	rBV2	295	229	0.02%	0.002%
48	7.028	1761	1769	1774	rBV2	226	347	0.03%	0.004%
49	7.073	1777	1783	1789	rBV2	296	470	0.03%	0.005%
50	7.182	1813	1817	1818	rVV2	224	182	0.01%	0.002%
51	7.195	1818	1821	1826	rVV4	554	562	0.04%	0.006%
52	7.359	1870	1872	1876	rVB	380	249	0.02%	0.003%
53	7.475	1903	1908	1911	rBV2	145	150	0.01%	0.002%
54	7.510	1916	1919	1924	rVB2	272	234	0.02%	0.002%
55	7.565	1924	1936	1955	rBV	135500	240958	17.83%	2.543%
56	7.697	1975	1977	1983	rVB4	700	660	0.05%	0.007%
57	7.800	2004	2009	2015	rBV3	447	555	0.04%	0.006%
58	7.896	2026	2039	2065	rBV	567958	1009524	74.69%	10.655%
59	8.179	2116	2127	2145	rBV	91107	156716	11.60%	1.654%
60	8.346	2176	2179	2182	rBV2	242	202	0.01%	0.002%
61	8.401	2191	2196	2199	rBV	291	291	0.02%	0.003%
62	8.485	2220	2222	2226	rVB2	341	214	0.02%	0.002%
63	8.555	2234	2244	2254	rVB3	7674	11760	0.87%	0.124%
64	8.639	2254	2270	2280	rBV4	237854	531774	39.34%	5.613%
65	8.993	2377	2380	2385	rVB2	332	276	0.02%	0.003%
66	9.079	2402	2407	2408	rBV	344	315	0.02%	0.003%
67	9.269	2463	2466	2469	rVB	381	211	0.02%	0.002%
68	9.417	2497	2512	2536	rBV	497916	843572	62.41%	8.904%
69	9.629	2574	2578	2580	rBV	304	175	0.01%	0.002%
70	9.703	2596	2601	2605	rVB3	615	540	0.04%	0.006%
71	9.903	2660	2663	2667	rBV2	212	155	0.01%	0.002%
72	9.941	2672	2675	2679	rBV2	170	160	0.01%	0.002%
73	9.993	2687	2691	2695	rBV2	254	278	0.02%	0.003%
74	10.176	2743	2748	2750	rBV	319	235	0.02%	0.002%
75	10.195	2751	2754	2757	rVV2	254	197	0.01%	0.002%
76	10.243	2766	2769	2772	rBV	248	152	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050617.D
 Acq On : 03 Sep 2022 17:10
 Operator : SY/MD
 Sample : N4481-04 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

77	10.317	2790	2792	2796	rBV	238	150	0.01%	0.002%
78	10.462	2832	2837	2840	rBV2	258	265	0.02%	0.003%
79	10.485	2840	2844	2847	rBV2	380	416	0.03%	0.004%
80	10.755	2912	2928	2955	rBV	458662	753328	55.74%	7.951%
81	10.851	2956	2958	2964	rVB3	601	498	0.04%	0.005%
82	10.877	2964	2966	2971	rBV2	270	213	0.02%	0.002%
83	11.095	3028	3034	3037	rBV2	336	418	0.03%	0.004%
84	11.263	3084	3086	3090	rVB2	323	196	0.01%	0.002%
85	11.349	3110	3113	3119	rBV2	331	370	0.03%	0.004%
86	11.427	3134	3137	3140	rBV2	221	195	0.01%	0.002%
87	11.697	3218	3221	3226	rBV2	230	250	0.02%	0.003%
88	11.812	3244	3257	3283	rBV	420083	676533	50.06%	7.141%
89	12.028	3320	3324	3327	rBV2	412	329	0.02%	0.003%
90	12.086	3339	3342	3347	rBV	357	304	0.02%	0.003%
91	12.192	3362	3375	3398	rBV	499413	840081	62.16%	8.867%
92	12.504	3469	3472	3477	rBV3	522	550	0.04%	0.006%
93	12.542	3481	3484	3486	rVB2	304	176	0.01%	0.002%
94	12.562	3487	3490	3497	rVV4	467	555	0.04%	0.006%
95	12.780	3556	3558	3561	rBV	227	163	0.01%	0.002%
96	12.870	3583	3586	3595	rVB2	437	522	0.04%	0.006%
97	13.375	3737	3743	3744	rBV2	485	424	0.03%	0.004%
98	13.417	3752	3756	3760	rBV	513	464	0.03%	0.005%
99	13.668	3831	3834	3837	rBV3	516	409	0.03%	0.004%
100	14.336	4038	4042	4045	rBV2	987	852	0.06%	0.009%




Sum of corrected areas: 9474499

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050617.D
Acq On : 03 Sep 2022 17:10
Operator : SY/MD
Sample : N4481-04 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

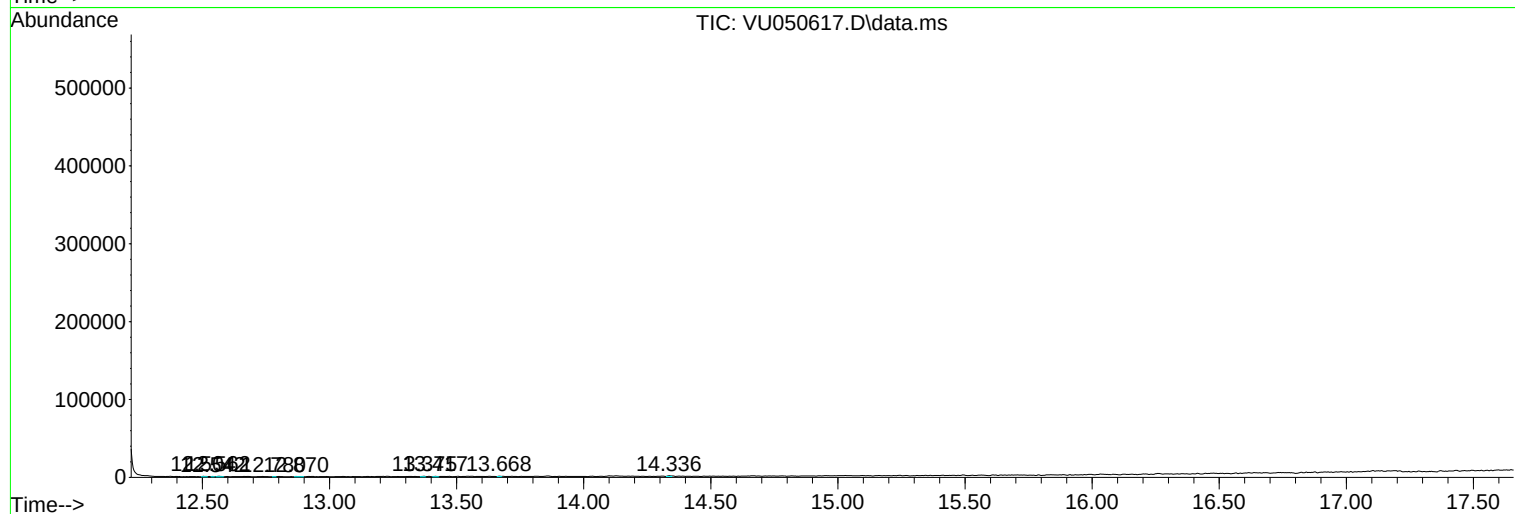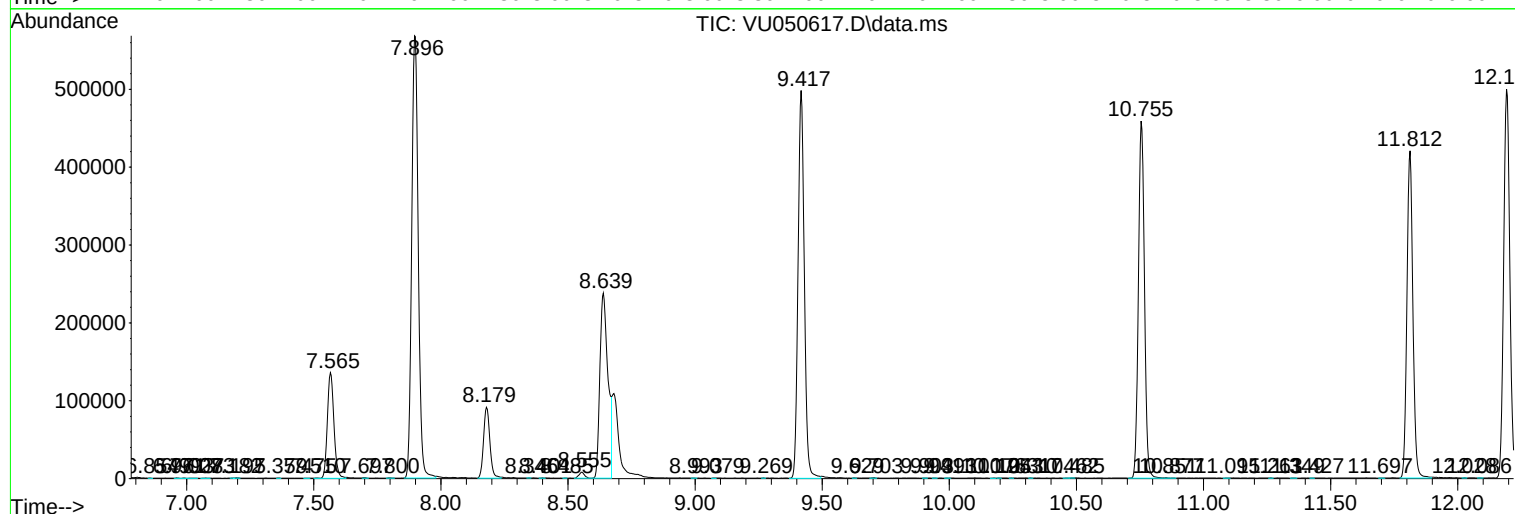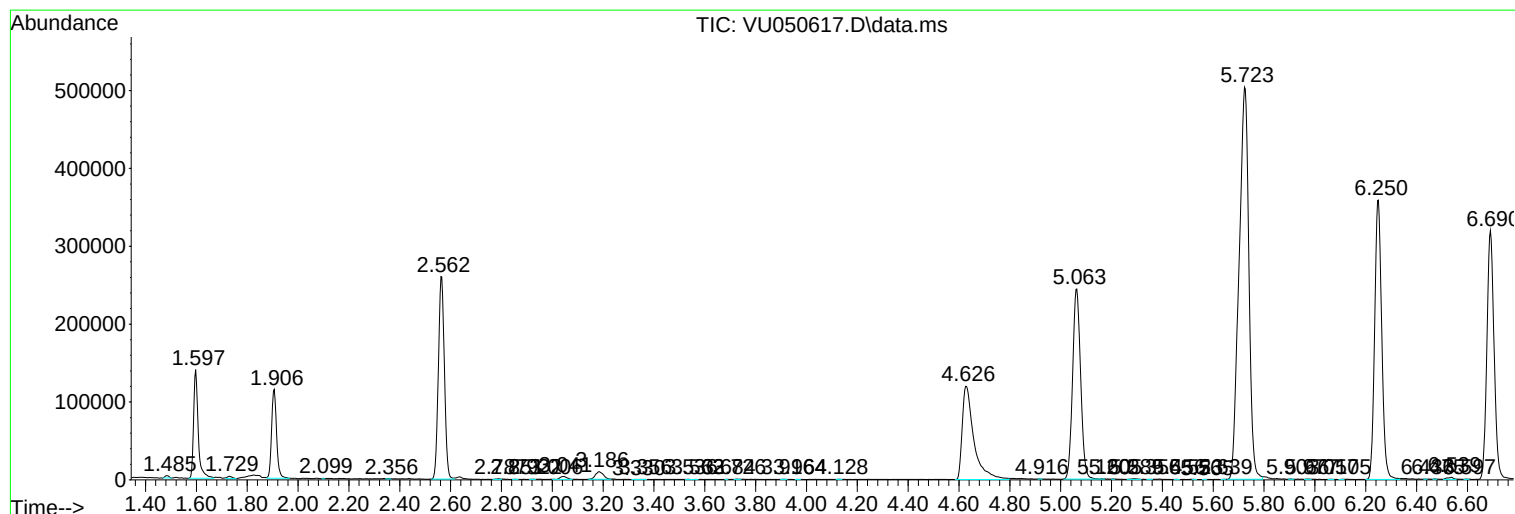

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050617.D
Acq On : 03 Sep 2022 17:10
Operator : SY/MD
Sample : N4481-04 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050617.D
Acq On : 03 Sep 2022 17:10
Operator : SY/MD
Sample : N4481-04 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------