

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050625.D
 Acq On : 03 Sep 2022 20:18
 Operator : SY/MD
 Sample : N4344-23MEDL 40X
 Misc : 5.58g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVS0MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050625.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	50	rBV2	3789	4063	0.23%	0.031%
2	1.520	51	56	64	rVV6	3001	4514	0.26%	0.034%
3	1.597	72	80	104	rBV	188415	248508	14.06%	1.882%
4	1.899	167	174	191	rVB	173998	239968	13.57%	1.818%
5	2.562	367	380	398	rBV	327581	528312	29.88%	4.002%
6	2.677	413	416	421	rVB4	757	717	0.04%	0.005%
7	2.751	436	439	443	rVB2	368	278	0.02%	0.002%
8	2.771	443	445	448	rBV2	429	358	0.02%	0.003%
9	2.825	459	462	466	rVB3	696	455	0.03%	0.003%
10	3.002	514	517	520	rBV2	422	323	0.02%	0.002%
11	3.044	521	530	542	rVB2	5505	9488	0.54%	0.072%
12	3.185	559	574	592	rBV2	31009	78023	4.41%	0.591%
13	3.346	619	624	628	rBV3	414	475	0.03%	0.004%
14	3.375	628	633	638	rVB3	367	477	0.03%	0.004%
15	3.411	638	644	647	rBV2	321	333	0.02%	0.003%
16	3.446	652	655	659	rVV2	430	326	0.02%	0.002%
17	3.517	670	677	685	rVV3	308	526	0.03%	0.004%
18	3.700	729	734	737	rBV2	324	299	0.02%	0.002%
19	3.742	743	747	749	rBV2	382	312	0.02%	0.002%
20	3.915	799	801	807	rVB2	354	266	0.02%	0.002%
21	4.050	838	843	846	rBV	357	335	0.02%	0.003%
22	4.118	860	864	869	rBV2	335	257	0.01%	0.002%
23	4.240	897	902	905	rBV2	273	320	0.02%	0.002%
24	4.330	924	930	934	rVB2	368	383	0.02%	0.003%
25	4.356	934	938	943	rBV2	337	385	0.02%	0.003%
26	4.629	1010	1023	1067	rBV	183493	551656	31.20%	4.179%
27	5.005	1136	1140	1141	rBV3	459	270	0.02%	0.002%
28	5.063	1141	1158	1184	rVV	319134	700979	39.65%	5.310%
29	5.291	1219	1229	1240	rVB8	1673	3155	0.18%	0.024%
30	5.375	1250	1255	1259	rBV4	665	690	0.04%	0.005%
31	5.722	1342	1363	1399	rBV2	652980	1767975	100.00%	13.392%
32	5.973	1435	1441	1445	rBV4	867	1139	0.06%	0.009%
33	6.144	1491	1494	1498	rVB2	315	278	0.02%	0.002%
34	6.250	1511	1527	1551	rBV	480522	935174	52.90%	7.083%
35	6.529	1607	1614	1617	rBV6	2561	3043	0.17%	0.023%
36	6.607	1630	1638	1640	rBV3	640	761	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050625.D
 Acq On : 03 Sep 2022 20:18
 Operator : SY/MD
 Sample : N4344-23MEDL 40X
 Misc : 5.58g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVS0MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	6.690	1650	1664	1688	rBV	417860	821414	46.46%	6.222%
38	6.848	1711	1713	1717	rVB3	818	489	0.03%	0.004%
39	6.925	1734	1737	1742	rVB2	375	286	0.02%	0.002%
40	7.053	1773	1777	1781	rVB	490	427	0.02%	0.003%
41	7.121	1793	1798	1802	rVB2	267	301	0.02%	0.002%
42	7.143	1802	1805	1810	rBV2	349	371	0.02%	0.003%
43	7.189	1813	1819	1833	rVV3	1508	2563	0.14%	0.019%
44	7.288	1845	1850	1853	rBV2	306	316	0.02%	0.002%
45	7.333	1861	1864	1870	rVB2	271	302	0.02%	0.002%
46	7.365	1870	1874	1877	rBV2	413	402	0.02%	0.003%
47	7.565	1921	1936	1958	rBV	162287	295004	16.69%	2.235%
48	7.803	2005	2010	2014	rVB4	539	615	0.03%	0.005%
49	7.896	2026	2039	2063	rBV	689387	1201611	67.97%	9.102%
50	8.179	2116	2127	2147	rBV	110412	192590	10.89%	1.459%
51	8.365	2180	2185	2189	rBV4	505	544	0.03%	0.004%
52	8.414	2196	2200	2204	rVB3	438	323	0.02%	0.002%
53	8.465	2214	2216	2223	rVB3	791	788	0.04%	0.006%
54	8.552	2230	2243	2258	rBV	573874	959116	54.25%	7.265%
55	8.639	2258	2270	2307	rVV3	420412	959439	54.27%	7.267%
56	8.938	2361	2363	2366	rVB2	742	430	0.02%	0.003%
57	8.957	2366	2369	2373	rBV4	496	275	0.02%	0.002%
58	8.976	2373	2375	2380	rVB4	634	399	0.02%	0.003%
59	9.073	2402	2405	2407	rBV2	350	258	0.01%	0.002%
60	9.140	2423	2426	2429	rVB	382	273	0.02%	0.002%
61	9.166	2429	2434	2435	rBV3	472	301	0.02%	0.002%
62	9.365	2492	2496	2499	rBV	362	327	0.02%	0.002%
63	9.417	2499	2512	2530	rBV	649223	1088110	61.55%	8.242%
64	9.594	2564	2567	2572	rVB4	818	670	0.04%	0.005%
65	9.635	2577	2580	2583	rVV2	378	271	0.02%	0.002%
66	9.700	2597	2600	2604	rVB3	767	507	0.03%	0.004%
67	9.819	2634	2637	2642	rBV	361	314	0.02%	0.002%
68	9.944	2673	2676	2680	rBV	410	289	0.02%	0.002%
69	10.037	2700	2705	2709	rBV3	362	324	0.02%	0.002%
70	10.102	2721	2725	2727	rBV	462	368	0.02%	0.003%
71	10.118	2727	2730	2733	rVB2	581	450	0.03%	0.003%
72	10.243	2765	2769	2772	rVB	373	324	0.02%	0.002%
73	10.362	2799	2806	2808	rBV2	288	295	0.02%	0.002%
74	10.484	2840	2844	2846	rBV2	360	331	0.02%	0.003%
75	10.587	2873	2876	2879	rBV	360	268	0.02%	0.002%
76	10.626	2884	2888	2891	rBV2	305	291	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050625.D
 Acq On : 03 Sep 2022 20:18
 Operator : SY/MD
 Sample : N4344-23MEDL 40X
 Misc : 5.58g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVS0MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

77	10.754	2915	2928	2955	rVV	587710	959126	54.25%	7.265%
78	11.114	3036	3040	3045	rVB5	840	887	0.05%	0.007%
79	11.336	3104	3109	3116	rVB2	406	483	0.03%	0.004%
80	11.478	3150	3153	3158	rBV2	375	321	0.02%	0.002%
81	11.812	3244	3257	3274	rBV	478566	761568	43.08%	5.769%
82	12.018	3317	3321	3324	rBV2	494	507	0.03%	0.004%
83	12.098	3341	3346	3352	rVV3	429	567	0.03%	0.004%
84	12.192	3362	3375	3398	rBV	523625	856476	48.44%	6.487%
85	12.375	3429	3432	3434	rVV2	670	321	0.02%	0.002%
86	12.394	3435	3438	3440	rVV2	428	268	0.02%	0.002%
87	12.507	3469	3473	3478	rBV3	534	435	0.02%	0.003%
88	12.735	3542	3544	3549	rVB2	495	304	0.02%	0.002%
89	12.761	3549	3552	3556	rBV3	389	276	0.02%	0.002%
90	12.822	3567	3571	3573	rBV2	445	301	0.02%	0.002%
91	12.970	3614	3617	3620	rBV2	391	285	0.02%	0.002%
92	13.249	3700	3704	3707	rBV3	524	399	0.02%	0.003%
93	13.294	3716	3718	3724	rVB	336	279	0.02%	0.002%
94	13.484	3774	3777	3783	rBV4	388	457	0.03%	0.003%
95	13.597	3810	3812	3818	rVB	601	366	0.02%	0.003%
96	13.629	3818	3822	3823	rBV	327	271	0.02%	0.002%
97	14.037	3946	3949	3951	rBV2	465	335	0.02%	0.003%
98	14.265	4018	4020	4027	rBV2	389	349	0.02%	0.003%
99	14.642	4133	4137	4139	rBV3	717	484	0.03%	0.004%
100	14.712	4156	4159	4160	rBV	509	310	0.02%	0.002%




Sum of corrected areas: 13202172

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050625.D
Acq On : 03 Sep 2022 20:18
Operator : SY/MD
Sample : N4344-23MEDL 40X
Misc : 5.58g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVS0MEDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

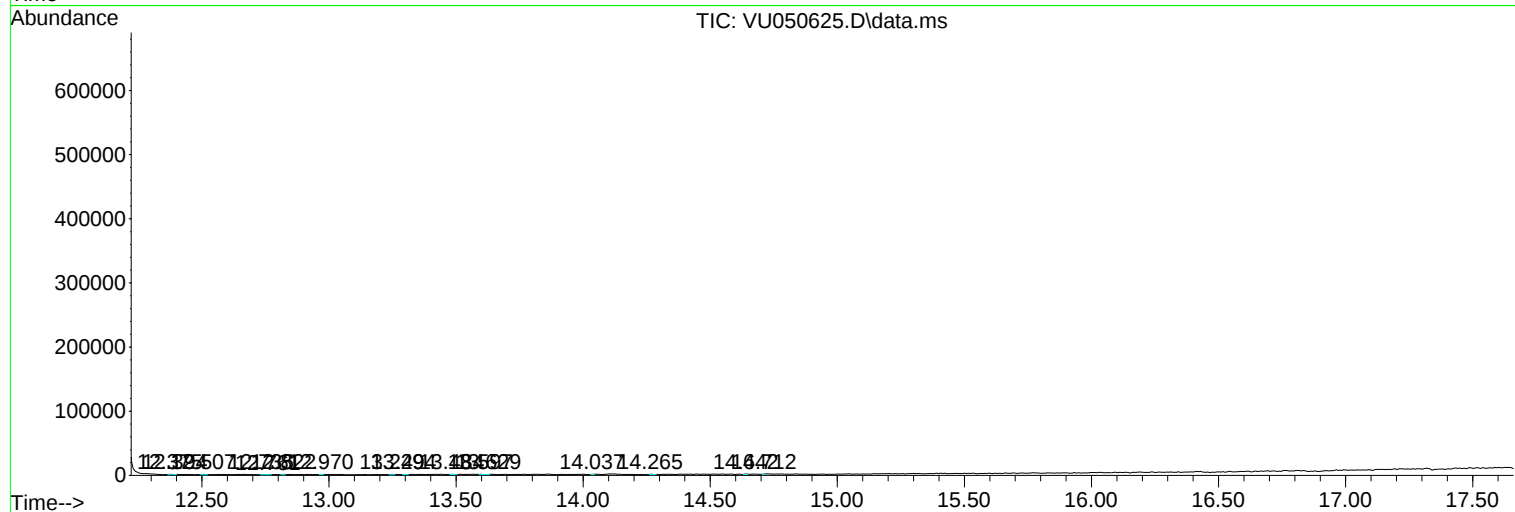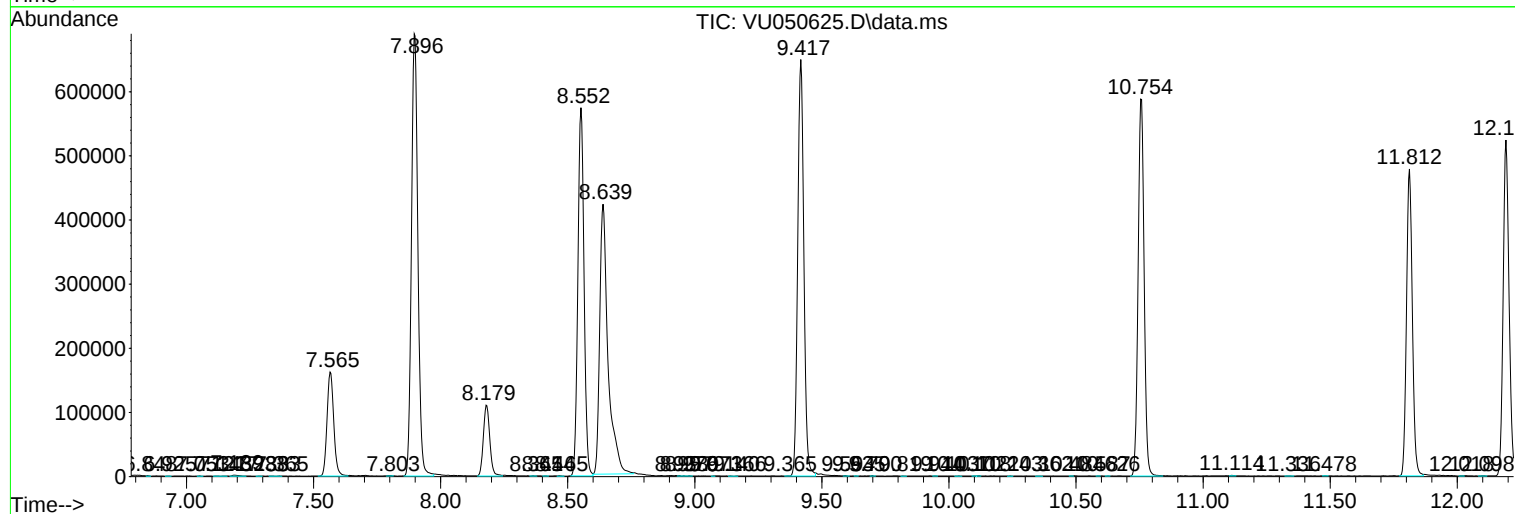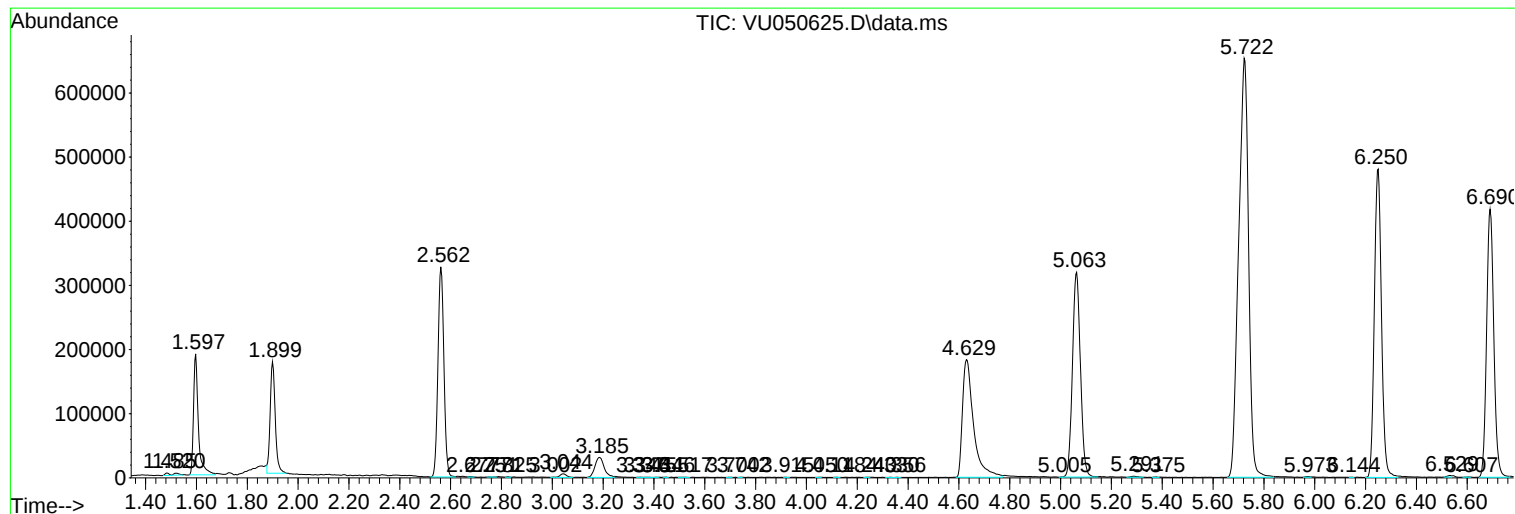

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050625.D
Acq On : 03 Sep 2022 20:18
Operator : SY/MD
Sample : N4344-23MEDL 40X
Misc : 5.58g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVS0MEDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
Data File : VU050625.D
Acq On : 03 Sep 2022 20:18
Operator : SY/MD
Sample : N4344-23MEDL 40X
Misc : 5.58g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVS0MEDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------