


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090322\
 Data File : VU050603.D
 Acq On : 03 Sep 2022 10:02
 Operator : SY/MD
 Sample : BFB119
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB119

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis
 Last Update : Wed Sep 07 01:37:50 2022

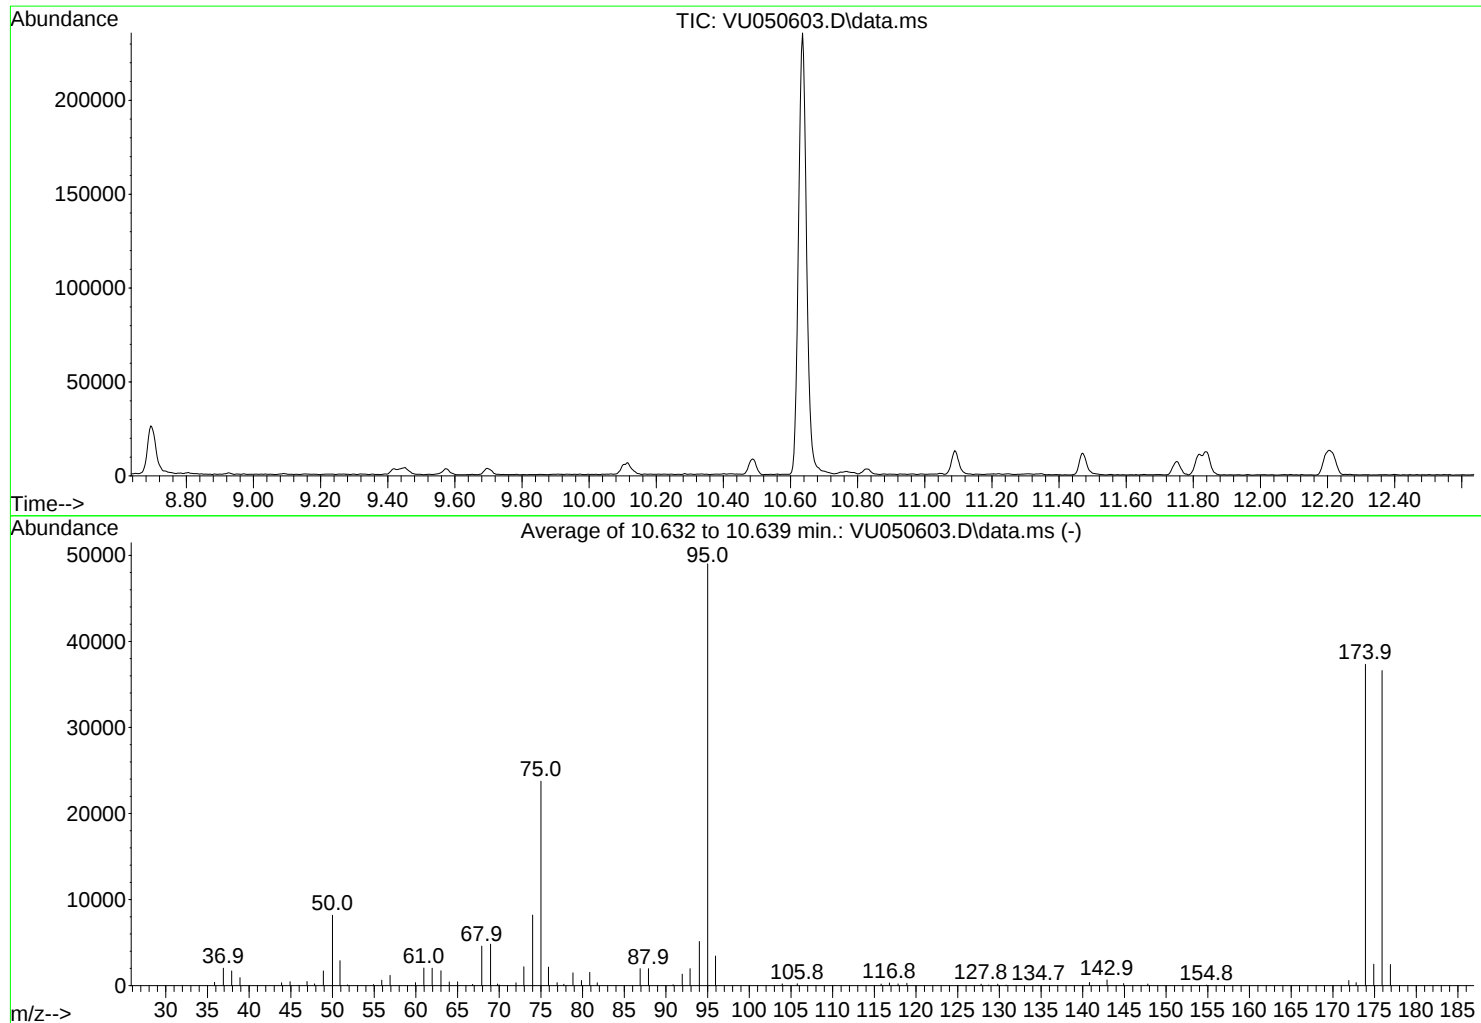

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	8189	PASS
75	95	30	80	48.5	23768	PASS
95	95	100	100	100.0	49011	PASS
96	95	5	9	7.0	3444	PASS
173	174	0.00	2	1.0	362	PASS
174	95	50	120	76.2	37341	PASS
175	174	5	9	6.7	2490	PASS
176	174	95	101	98.0	36611	PASS
177	176	5	9	6.7	2451	PASS

Scan 2878 (10.594 min): VU050603.D\data.ms
BFB119

m/z	Abundance
39.80	493.0
43.90	394.0

Instrument :
MSVOA_U
ClientSampleId :
BFB119

m/z	Abundance
35.90	422.0
36.90	2135.0
37.90	1844.0
38.90	1019.0
39.90	461.0
43.90	811.0
44.90	434.0
46.90	460.0
47.80	210.0
48.90	1763.0
50.00	8104.0
50.90	2758.0
54.90	111.0
55.90	625.0
56.90	1109.0
59.90	373.0
60.90	2033.0
62.00	2017.0
63.00	1744.0
64.00	408.0
65.00	461.0
66.80	188.0
67.90	4558.0
68.90	4916.0
69.80	299.0
72.00	381.0
72.90	2139.0
74.00	8222.0
75.00	23592.0
75.90	2176.0
77.00	374.0
77.80	185.0
78.90	1453.0
79.80	558.0
80.90	1411.0
81.80	313.0
86.90	2098.0
87.90	1876.0
90.80	117.0
92.00	1227.0
92.90	1948.0
94.00	5188.0
95.00	48528.0
95.90	3602.0
103.90	176.0
105.80	177.0
115.80	176.0
116.70	332.0
117.80	203.0
118.90	295.0
127.80	176.0
129.80	150.0
140.80	405.0
142.90	620.0
144.90	289.0
147.80	155.0
154.90	107.0
171.90	600.0
172.80	379.0
173.90	36272.0
174.90	2515.0
175.90	35504.0
176.90	2499.0

Instrument :
MSVOA_U
ClientSampleId :
BFB119

m/z	Abundance
35.80	391.0
36.90	2078.0
37.90	1773.0
38.90	945.0
39.90	418.0
43.90	748.0
44.90	475.0
45.90	101.0
47.00	473.0
47.90	200.0
48.90	1732.0
50.00	8406.0
50.90	2976.0
51.80	117.0
54.90	136.0
55.90	654.0
56.90	1268.0
59.90	346.0
61.00	2112.0
61.90	2103.0
63.00	1746.0
64.00	456.0
65.00	480.0
66.80	160.0
67.90	4744.0
69.00	4962.0
69.80	239.0
72.00	359.0
72.90	2234.0
74.00	8543.0
75.00	24616.0
75.90	2244.0
76.90	365.0
77.70	181.0
78.80	1517.0
79.90	613.0
80.80	1572.0
81.70	359.0
86.90	1984.0
87.90	2076.0
90.90	127.0
91.90	1395.0
92.90	1952.0
94.00	5316.0
95.00	50816.0
96.00	3571.0
103.90	207.0
105.80	226.0
115.80	182.0
116.80	322.0
117.80	208.0
118.90	295.0
127.80	174.0
128.70	111.0
129.80	168.0
130.80	104.0
140.80	398.0
142.90	679.0
144.90	244.0
147.80	204.0
154.80	101.0
171.90	609.0
172.80	375.0
173.90	38360.0
174.90	2550.0
175.90	37728.0
176.90	2480.0

Instrument :
MSVOA_U
ClientSampleId :
BFB119

m/z	Abundance
35.90	355.0
36.90	1852.0
37.90	1535.0
38.90	836.0
39.90	416.0
43.90	657.0
44.90	495.0
46.90	501.0
47.90	205.0
48.90	1658.0
50.00	8056.0
50.90	2945.0
51.80	143.0
54.90	122.0
55.90	618.0
56.90	1213.0
60.00	345.0
61.00	2019.0
61.90	1981.0
63.00	1719.0
64.00	397.0
65.00	419.0
66.90	100.0
67.90	4474.0
69.00	4583.0
70.00	202.0
72.00	259.0
73.00	2187.0
74.00	7836.0
75.00	23096.0
75.90	2066.0
76.90	302.0
77.80	165.0
78.80	1480.0
79.90	599.0
80.80	1626.0
81.80	357.0
86.90	1811.0
87.90	1964.0
90.90	105.0
91.90	1422.0
92.90	2007.0
94.00	4874.0
95.00	47688.0
96.00	3160.0
104.00	221.0
105.70	274.0
115.80	184.0
116.90	321.0
117.90	190.0
118.90	262.0
127.80	143.0
128.70	110.0
129.80	166.0
130.80	100.0
134.70	132.0
140.80	317.0
142.90	702.0
144.90	212.0
147.80	178.0
171.90	607.0
172.80	332.0
173.90	37392.0
174.90	2405.0
175.90	36600.0
176.90	2373.0

Instrument :
MSVOA_U
ClientSampleId :
BFB119