

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090324\
 Data File : VU060584.D
 Acq On : 03 Sep 2024 14:12
 Operator : MD/SY
 Sample : VU0903WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0903WBL01

Quant Time: Sep 04 05:42:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Aug 06 11:07:28 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.113	96	30307	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.631	95	8990	0.871	ug/l	0.00
Spiked Amount 1.000			Recovery	=	87.000%	
68) 1,2-Dichlorobenzene-d4	12.193	152	8703	0.776	ug/l	0.00
Spiked Amount 1.000			Recovery	=	78.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090324\
Data File : VU060584.D
Acq On : 03 Sep 2024 14:12
Operator : MD/SY
Sample : VU0903WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0903WBL01

Quant Time: Sep 04 05:42:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Aug 06 11:07:28 2024
Response via : Initial Calibration

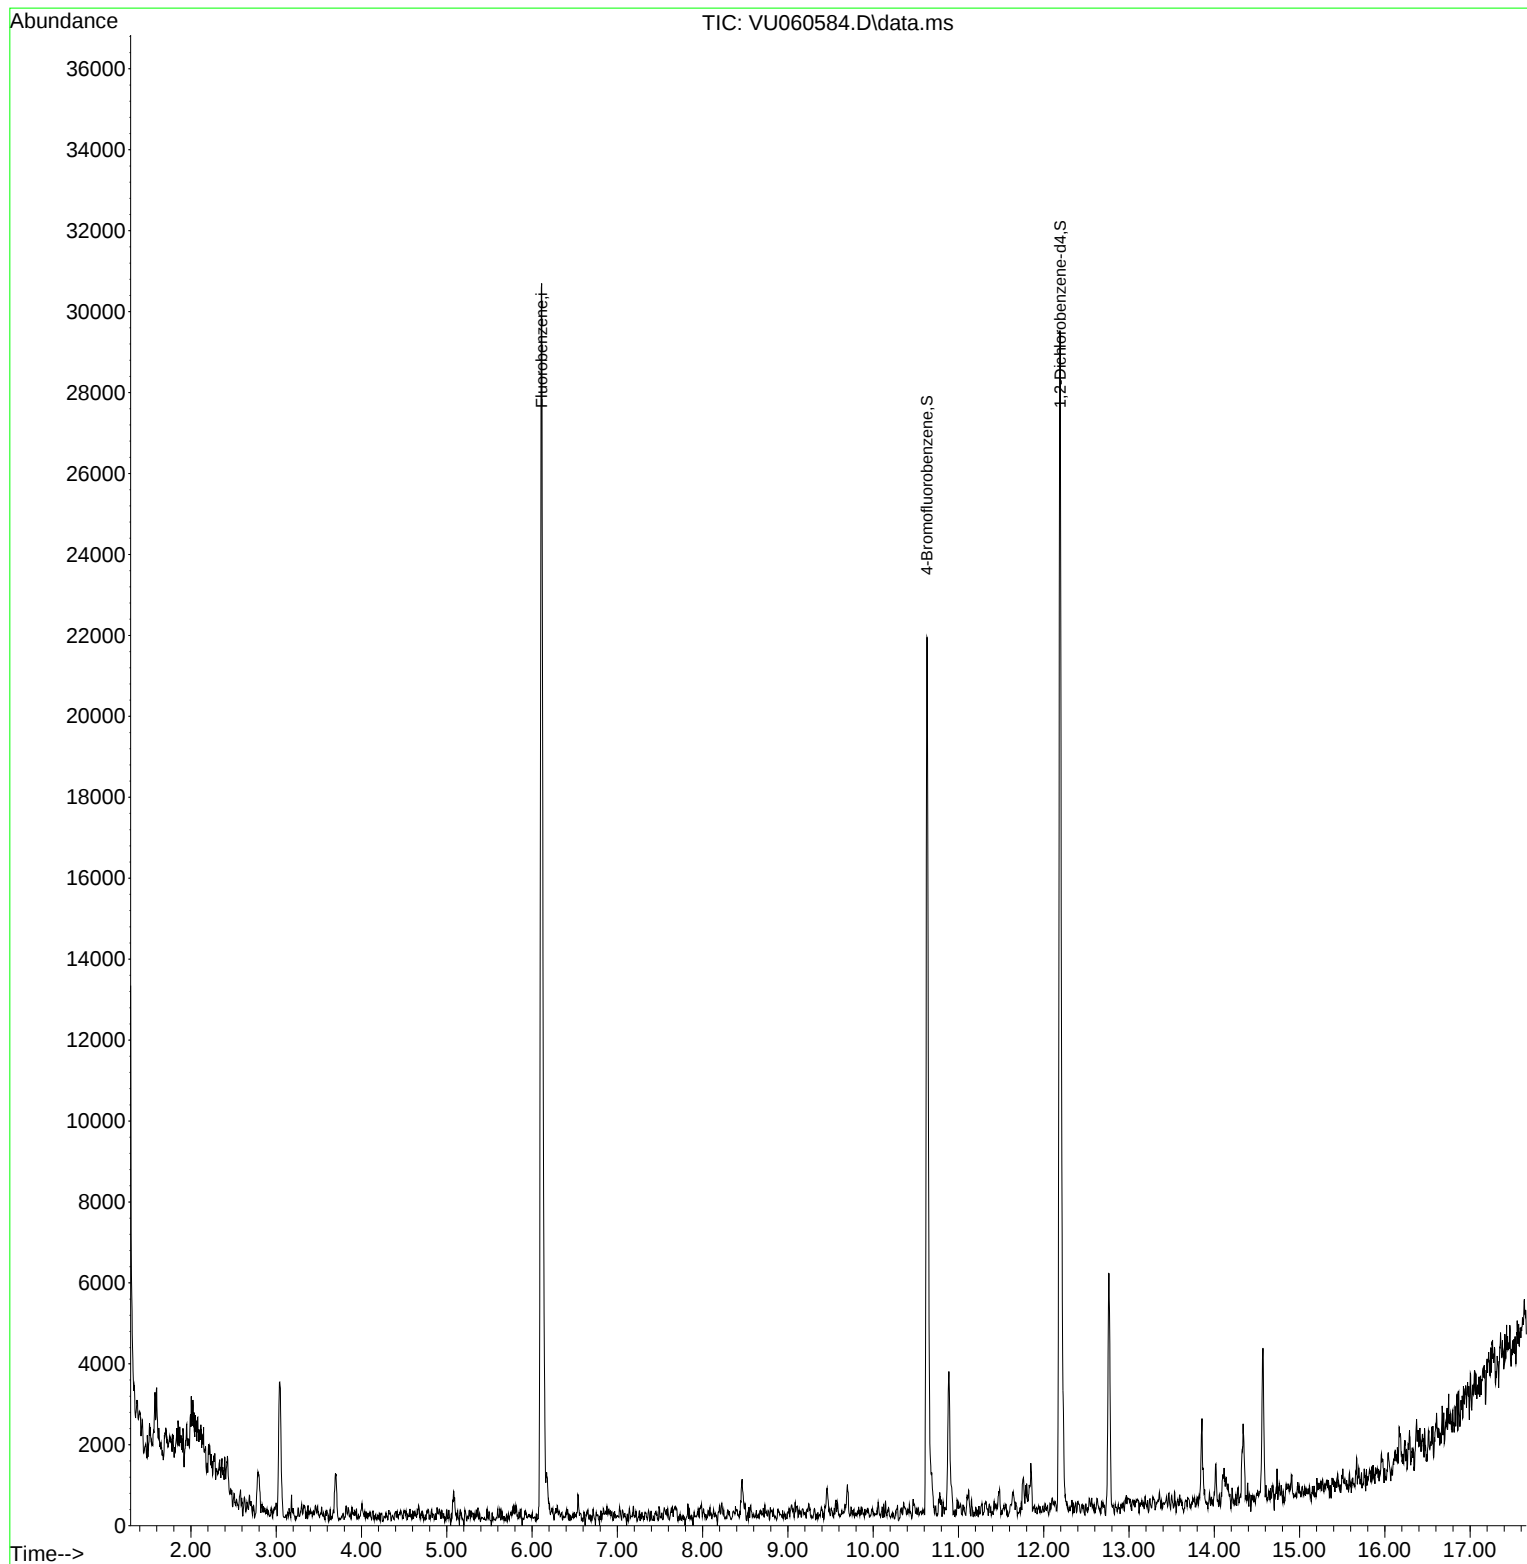




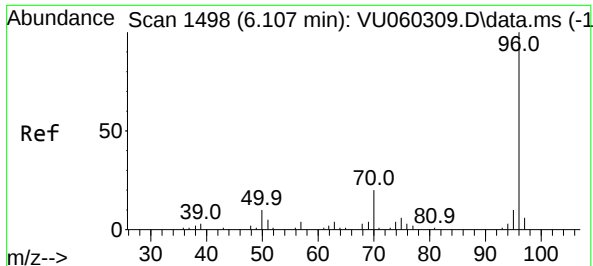


#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.113 min Scan# 1
Delta R.T. 0.006 min
Lab File: VU060584.D
Acq: 03 Sep 2024 14:12

Instrument :
MSVOA_U
ClientSampleId :
VU0903WBL01

Tgt Ion: 96 Resp: 30307




Ion	Ratio	Lower	Upper
96	100		
70	21.4	17.2	25.8
95	8.9	7.9	11.9
97	6.5	0.0	0.0

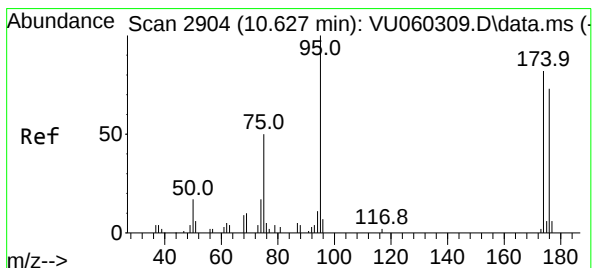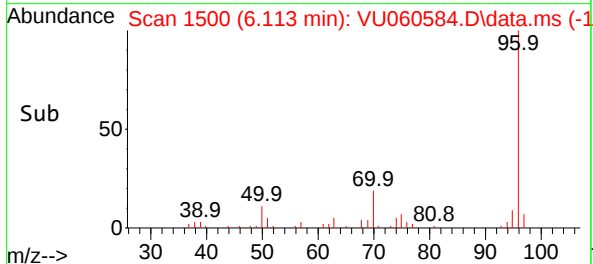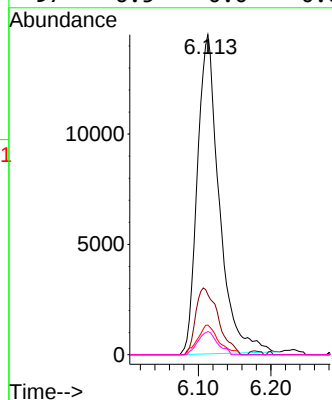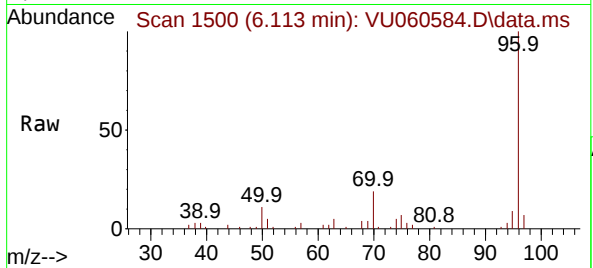


#57
4-Bromofluorobenzene
Concen: 0.871 ug/l
RT: 10.631 min Scan# 2905
Delta R.T. 0.003 min
Lab File: VU060584.D
Acq: 03 Sep 2024 14:12

Tgt Ion: 95 Resp: 8990


Ion	Ratio	Lower	Upper
95	100		
174	85.3	65.6	98.4
176	75.4	60.4	90.6

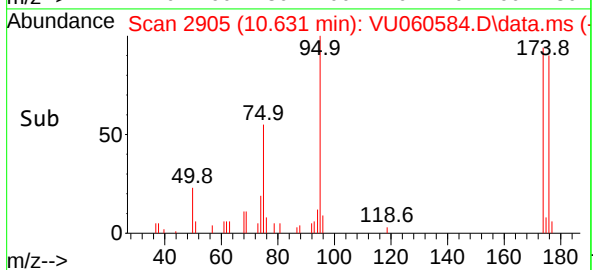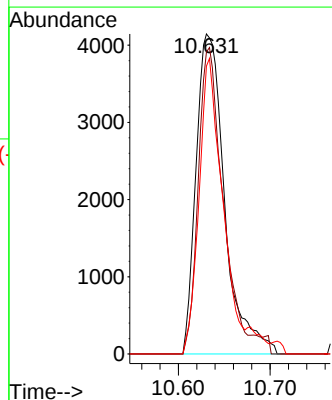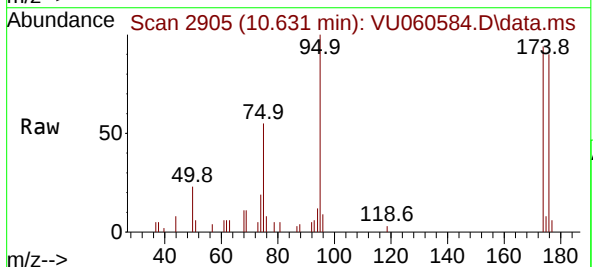

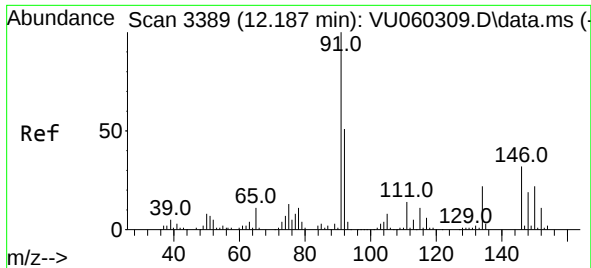

#68
1,2-Dichlorobenzene-d4
Concen: 0.776 ug/l
RT: 12.193 min Scan# 31
Delta R.T. 0.006 min
Lab File: VU060584.D
Acq: 03 Sep 2024 14:12

Instrument :
MSVOA_U
ClientSampleId :
VU0903WBL01

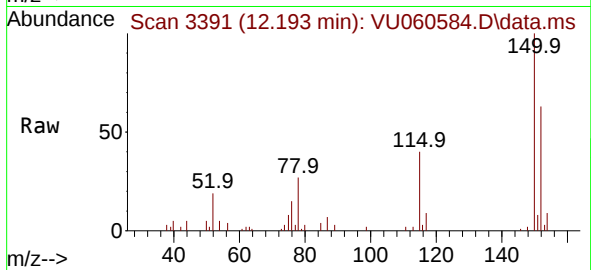

Tgt Ion	Ratio	Lower	Upper
152	100		
115	66.6	0.0	325.2
150	174.1	0.0	684.2

