

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090324\
 Data File : VU060584.D
 Acq On : 03 Sep 2024 14:12
 Operator : MD/SY
 Sample : VU0903WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0903WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU060584.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.428	348	354	363	rVB3	948	1411	2.31%	0.666%
2	2.785	457	465	466	rBV2	1025	1075	1.76%	0.507%
3	3.042	535	545	561	rVB6	3349	6764	11.06%	3.192%
4	3.695	742	748	749	rBV3	981	930	1.52%	0.439%
5	6.113	1487	1500	1515	rBV2	30524	61183	100.00%	28.871%
6	8.463	2221	2231	2240	rBV2	962	1736	2.84%	0.819%
7	9.460	2536	2541	2547	rVB4	577	733	1.20%	0.346%
8	9.698	2610	2615	2623	rVB3	778	987	1.61%	0.466%
9	10.631	2897	2905	2921	rBV	21664	38677	63.22%	18.251%
10	10.888	2976	2985	3000	rVB4	3547	6910	11.29%	3.261%
11	11.119	3055	3057	3065	rVB3	650	615	1.01%	0.290%
12	11.762	3251	3257	3262	rBV4	801	1153	1.88%	0.544%
13	11.849	3281	3284	3290	rVB3	1186	1211	1.98%	0.571%
14	12.190	3379	3390	3412	rBV2	29162	55134	90.11%	26.017%
15	12.762	3557	3568	3579	rBV2	5983	10369	16.95%	4.893%
16	13.856	3900	3908	3911	rBV4	1958	2198	3.59%	1.037%
17	14.020	3954	3959	3965	rVB6	928	982	1.61%	0.463%
18	14.328	4050	4055	4056	rBV3	1185	1017	1.66%	0.480%
19	14.338	4056	4058	4066	rVB4	1867	2150	3.51%	1.015%
20	14.573	4121	4131	4139	rVB2	3680	5874	9.60%	2.772%
21	16.042	4581	4588	4597	rVB8	699	1137	1.86%	0.537%
22	16.290	4662	4665	4670	rVB4	885	763	1.25%	0.360%
23	16.373	4683	4691	4693	rBV4	1273	1530	2.50%	0.722%
24	16.466	4718	4720	4726	rVB7	811	617	1.01%	0.291%
25	16.511	4729	4734	4739	rBV4	768	898	1.47%	0.424%
26	16.608	4754	4764	4767	rBV5	1070	1610	2.63%	0.760%
27	16.672	4780	4784	4787	rBV3	928	641	1.05%	0.302%
28	16.849	4834	4839	4841	rVB4	910	784	1.28%	0.370%
29	16.868	4842	4845	4849	rBV5	954	671	1.10%	0.317%
30	17.003	4883	4887	4892	rBV5	1155	1106	1.81%	0.522%
31	17.199	4943	4948	4950	rBV5	1122	1050	1.72%	0.495%




Sum of corrected areas: 211916

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090324\
Data File : VU060584.D
Acq On : 03 Sep 2024 14:12
Operator : MD/SY
Sample : VU0903WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0903WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

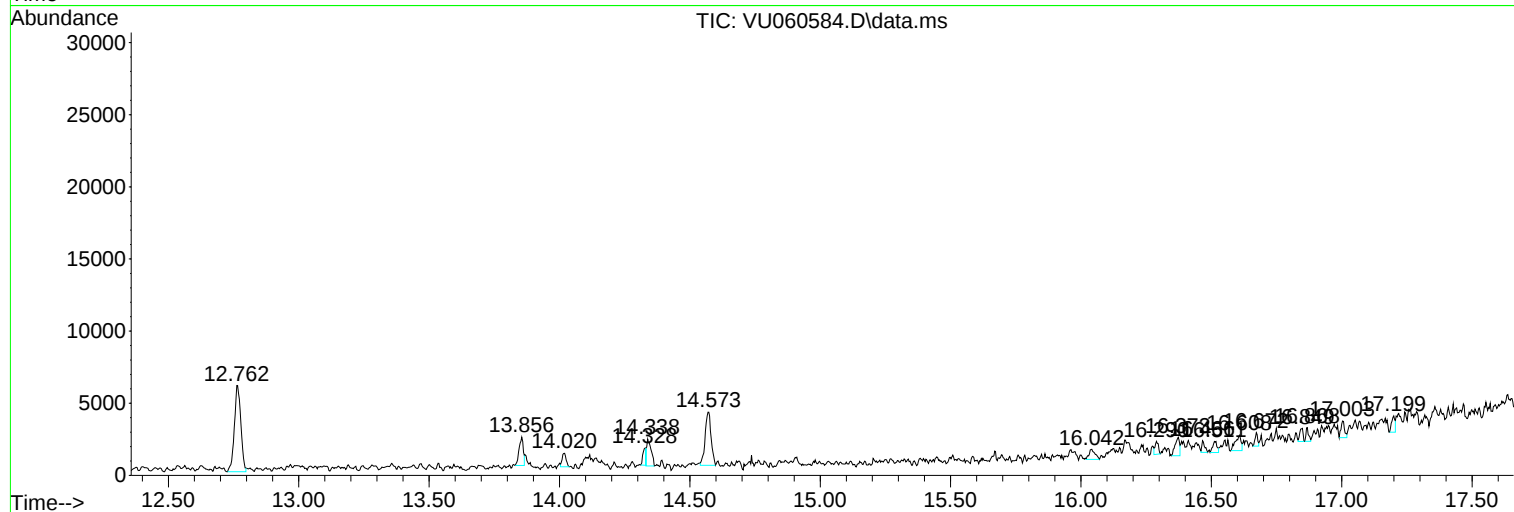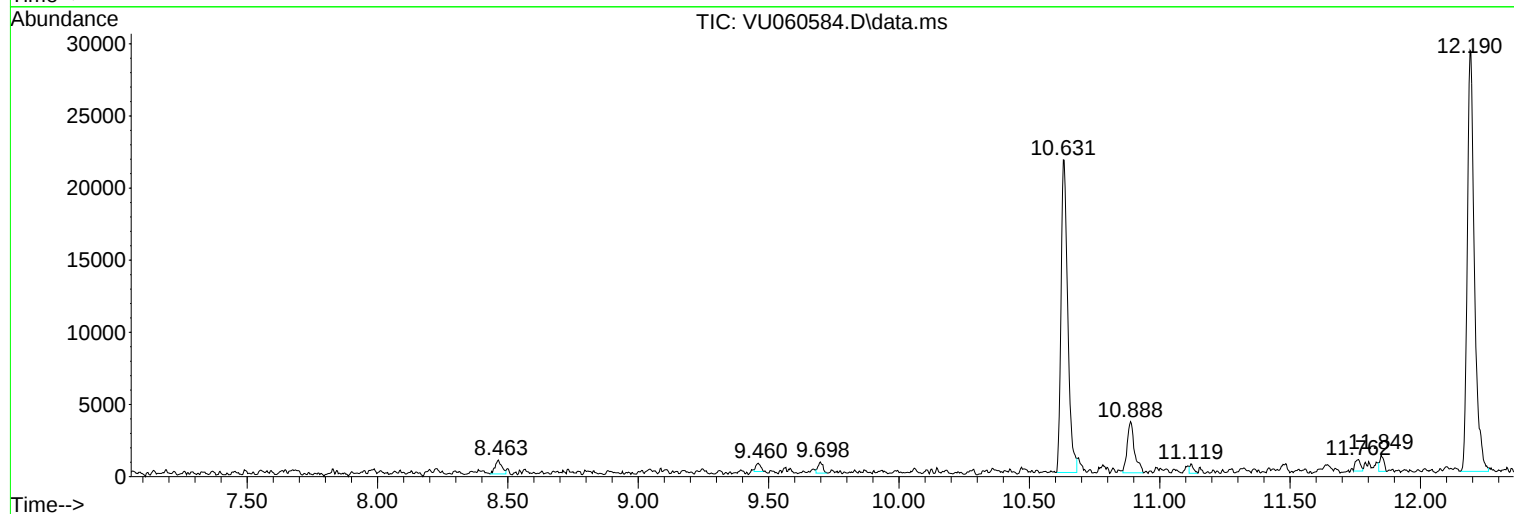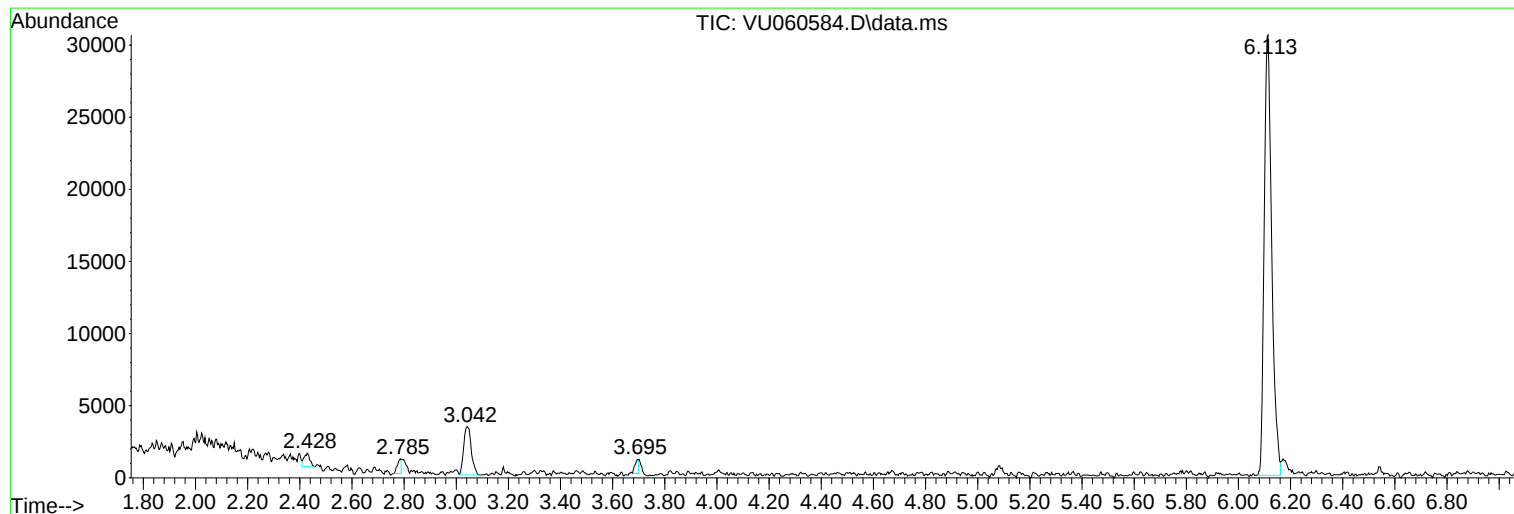

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090324\
Data File : VU060584.D
Acq On : 03 Sep 2024 14:12
Operator : MD/SY
Sample : VU0903WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0903WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090324\
Data File : VU060584.D
Acq On : 03 Sep 2024 14:12
Operator : MD/SY
Sample : VU0903WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0903WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------