

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090324\
 Data File : VU060588.D
 Acq On : 03 Sep 2024 16:29
 Operator : MD/SY
 Sample : P3810-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-UNRVOA-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU060588.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.856	166	176	190	rBV	536441	717396	33.38%	3.027%
2	1.930	190	199	231	rVB	476250	649796	30.24%	2.741%
3	2.132	250	262	277	rBV	725032	1046964	48.72%	4.417%
4	3.039	534	544	559	rBV2	11348	21936	1.02%	0.093%
5	3.354	624	642	677	rBV	524844	1231321	57.30%	5.195%
6	3.859	779	799	826	rBV	266852	638015	29.69%	2.692%
7	4.653	1027	1046	1068	rBV2	359852	900076	41.88%	3.797%
8	4.965	1128	1143	1170	rBV2	236200	542491	25.24%	2.289%
9	5.518	1295	1315	1336	rBV	148947	310858	14.47%	1.312%
10	6.110	1487	1499	1521	rBV	34016	67734	3.15%	0.286%
11	6.537	1623	1632	1650	rVB3	10649	21946	1.02%	0.093%
12	6.914	1737	1749	1778	rBV2	98803	193420	9.00%	0.816%
13	7.598	1946	1962	1996	rBV	295742	541958	25.22%	2.287%
14	8.203	2139	2150	2180	rBV	150340	269734	12.55%	1.138%
15	8.566	2249	2263	2287	rBV	257925	459806	21.40%	1.940%
16	9.524	2548	2561	2587	rBV	669778	1116354	51.95%	4.710%
17	10.476	2840	2857	2883	rBV	905052	1434567	66.75%	6.052%
18	10.630	2893	2905	2926	rVB2	36046	61221	2.85%	0.258%
19	10.775	2936	2950	2957	rBV	270308	443344	20.63%	1.870%
20	10.814	2957	2962	2976	rVB2	111851	170496	7.93%	0.719%
21	10.897	2976	2988	3010	rBV	1044944	1639690	76.30%	6.918%
22	11.081	3032	3045	3069	rBV	1083252	1671799	77.79%	7.053%
23	11.412	3133	3148	3163	rBV	1389208	2149035	100.00%	9.067%
24	11.637	3204	3218	3238	rBV	443716	700367	32.59%	2.955%
25	11.740	3238	3250	3256	rBV	284237	463495	21.57%	1.955%
26	11.785	3256	3264	3277	rVB	1316224	1959443	91.18%	8.267%
27	12.200	3379	3393	3417	rBV	662728	1060171	49.33%	4.473%
28	13.836	3897	3902	3913	rVB4	17389	27370	1.27%	0.115%
29	14.013	3942	3957	3971	rBV	1379470	2136363	99.41%	9.013%
30	14.322	4040	4053	4076	rBV	640572	1055058	49.09%	4.451%




Sum of corrected areas: 23702224

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090324\
Data File : VU060588.D
Acq On : 03 Sep 2024 16:29
Operator : MD/SY
Sample : P3810-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

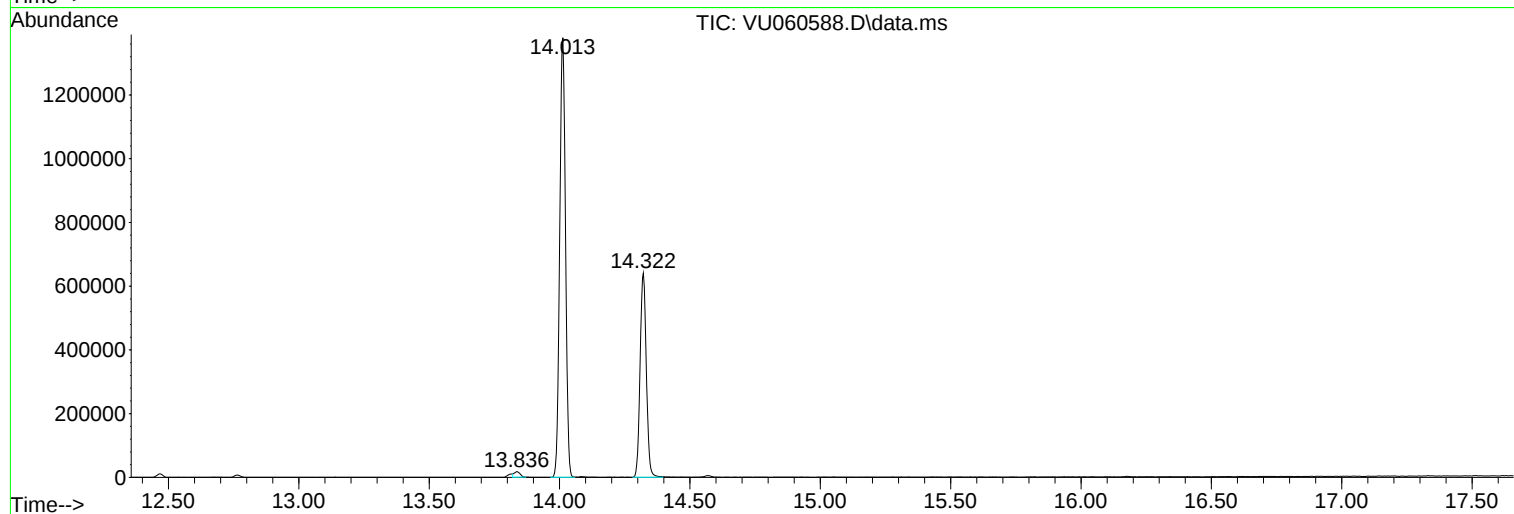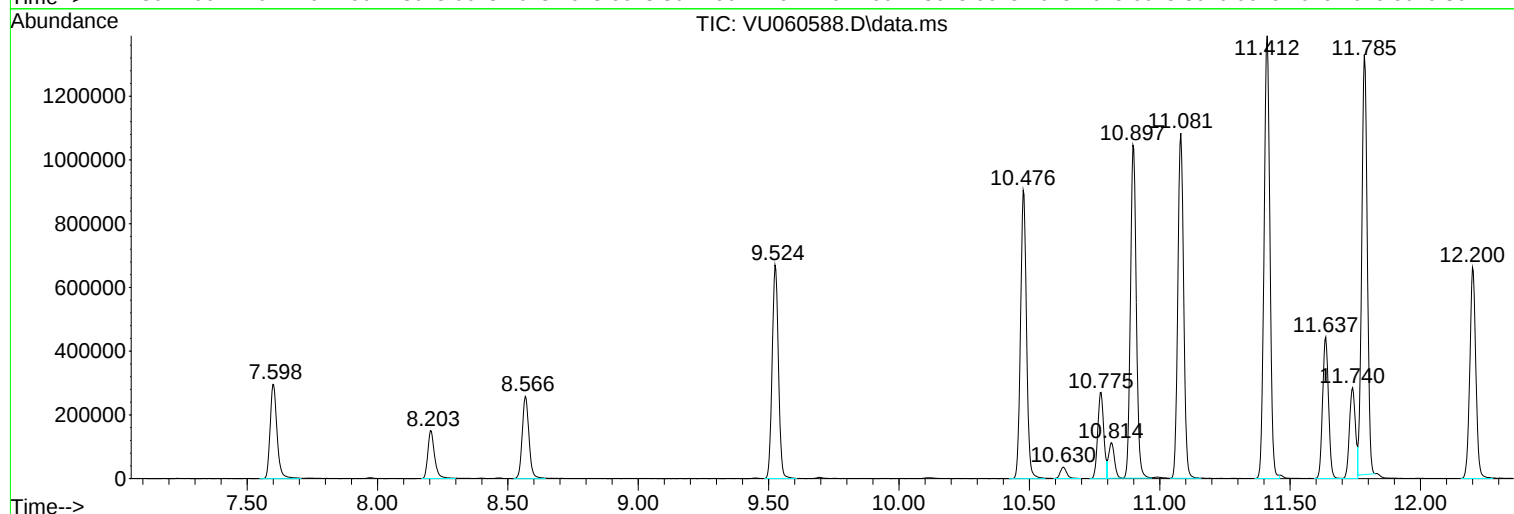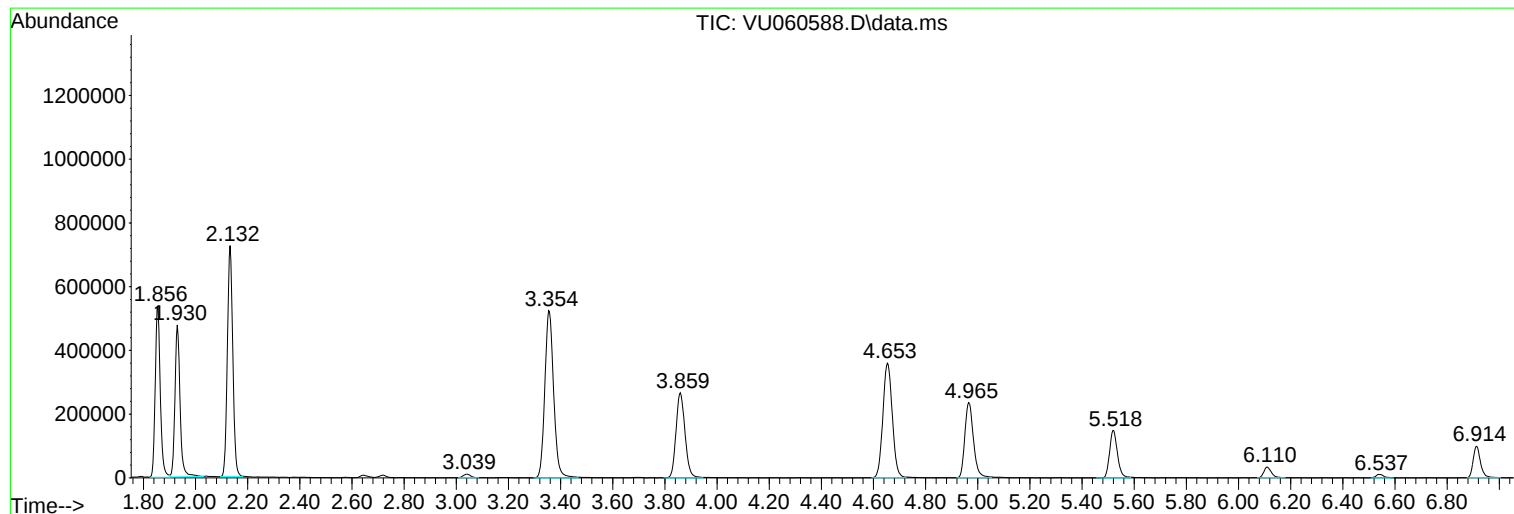

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090324\
Data File : VU060588.D
Acq On : 03 Sep 2024 16:29
Operator : MD/SY
Sample : P3810-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090324\
Data File : VU060588.D
Acq On : 03 Sep 2024 16:29
Operator : MD/SY
Sample : P3810-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------