

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090324\
 Data File : VU060589.D
 Acq On : 03 Sep 2024 16:53
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU060589.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.862	175	178	183	rVB5	1077	996	1.58%	0.361%
2	2.007	220	223	228	rBV5	915	745	1.18%	0.270%
3	2.129	258	261	265	rVB3	886	782	1.24%	0.284%
4	2.470	364	367	373	rVB3	590	642	1.02%	0.233%
5	2.788	459	466	473	rVB3	833	1064	1.68%	0.386%
6	3.039	536	544	557	rBV3	4858	8877	14.06%	3.220%
7	3.695	740	748	757	rBV4	1419	2311	3.66%	0.838%
8	6.113	1488	1500	1517	rBV	27835	59941	94.91%	21.742%
9	6.547	1629	1635	1638	rVB2	849	831	1.32%	0.301%
10	8.460	2223	2230	2240	rVB3	1134	1717	2.72%	0.623%
11	9.451	2533	2538	2542	rBV2	761	768	1.22%	0.279%
12	10.483	2851	2859	2866	rVB3	1362	1746	2.76%	0.633%
13	10.634	2896	2906	2921	rBV2	21168	37085	58.72%	13.452%
14	10.888	2975	2985	2986	rBV4	4260	4552	7.21%	1.651%
15	11.090	3040	3048	3061	rBV3	1643	2437	3.86%	0.884%
16	11.415	3140	3149	3158	rVB4	2471	3418	5.41%	1.240%
17	11.643	3211	3220	3227	rBV3	1225	1794	2.84%	0.651%
18	11.749	3247	3253	3259	rBV4	1767	2485	3.93%	0.901%
19	11.791	3259	3266	3276	rVV3	3933	6216	9.84%	2.255%
20	11.843	3276	3282	3292	rVB4	1406	2051	3.25%	0.744%
21	12.190	3377	3390	3410	rBV3	30608	63157	100.00%	22.908%
22	12.765	3559	3569	3578	rVB2	5155	8291	13.13%	3.007%
23	13.855	3898	3908	3912	rBV5	1312	2013	3.19%	0.730%
24	14.013	3945	3957	3970	rBV4	15785	24440	38.70%	8.865%
25	14.328	4046	4055	4072	rBV3	15813	28066	44.44%	10.180%
26	14.566	4121	4129	4130	rBV3	1972	1736	2.75%	0.630%
27	15.460	4402	4407	4410	rBV3	639	642	1.02%	0.233%
28	15.868	4529	4534	4539	rVB3	1133	1089	1.72%	0.395%
29	16.174	4626	4629	4635	rVB5	890	992	1.57%	0.360%
30	16.441	4708	4712	4715	rBV4	912	703	1.11%	0.255%
31	16.486	4722	4726	4729	rVV4	884	704	1.11%	0.255%
32	16.704	4790	4794	4800	rBV3	706	856	1.36%	0.310%
33	16.769	4811	4814	4817	rVB4	853	665	1.05%	0.241%
34	17.010	4885	4889	4895	rVB7	838	1029	1.63%	0.373%
35	17.357	4993	4997	4999	rBV5	1077	852	1.35%	0.309%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090324\
Data File : VU060589.D
Acq On : 03 Sep 2024 16:53
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER




Sum of corrected areas: 275693

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090324\
Data File : VU060589.D
Acq On : 03 Sep 2024 16:53
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

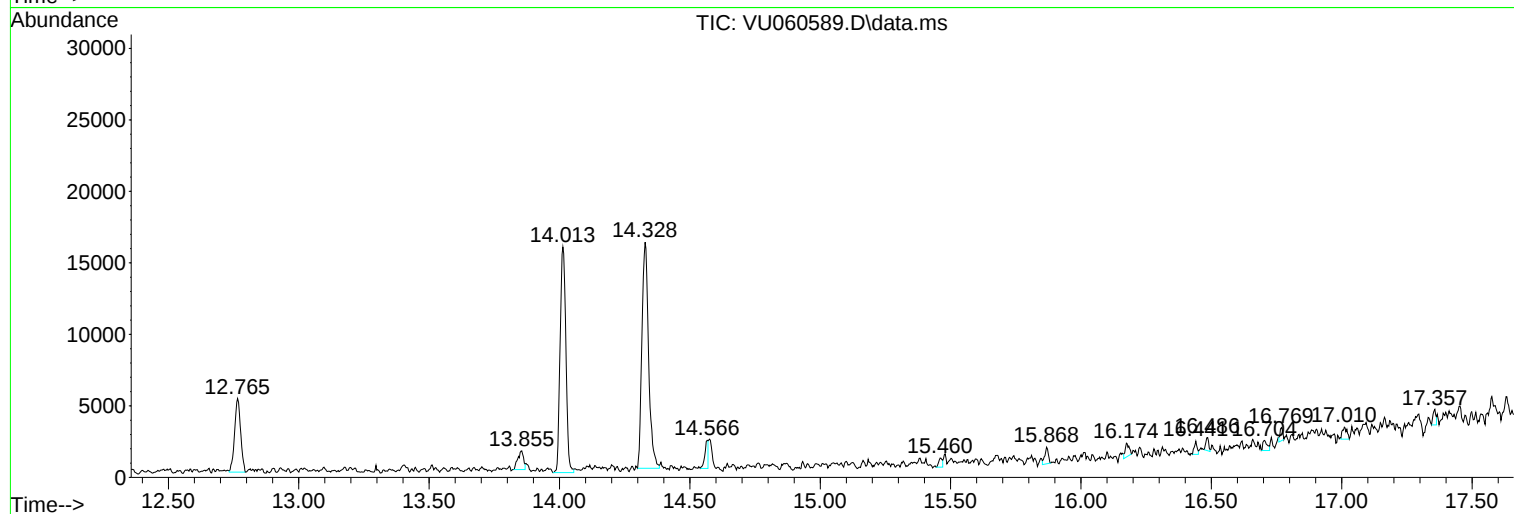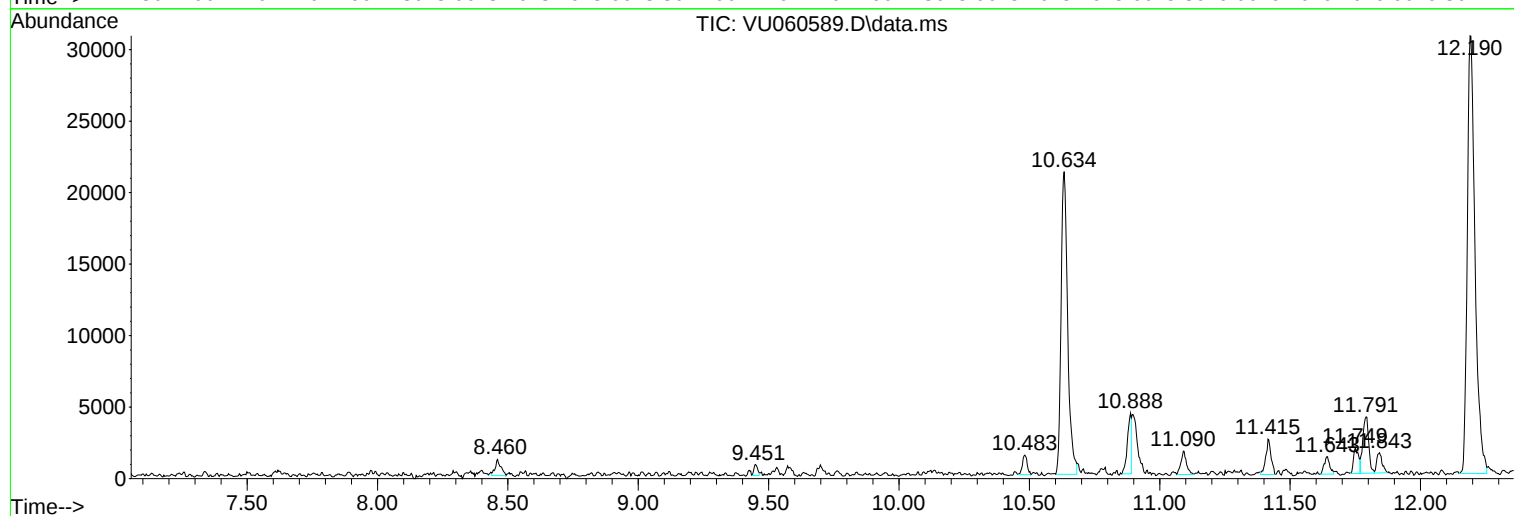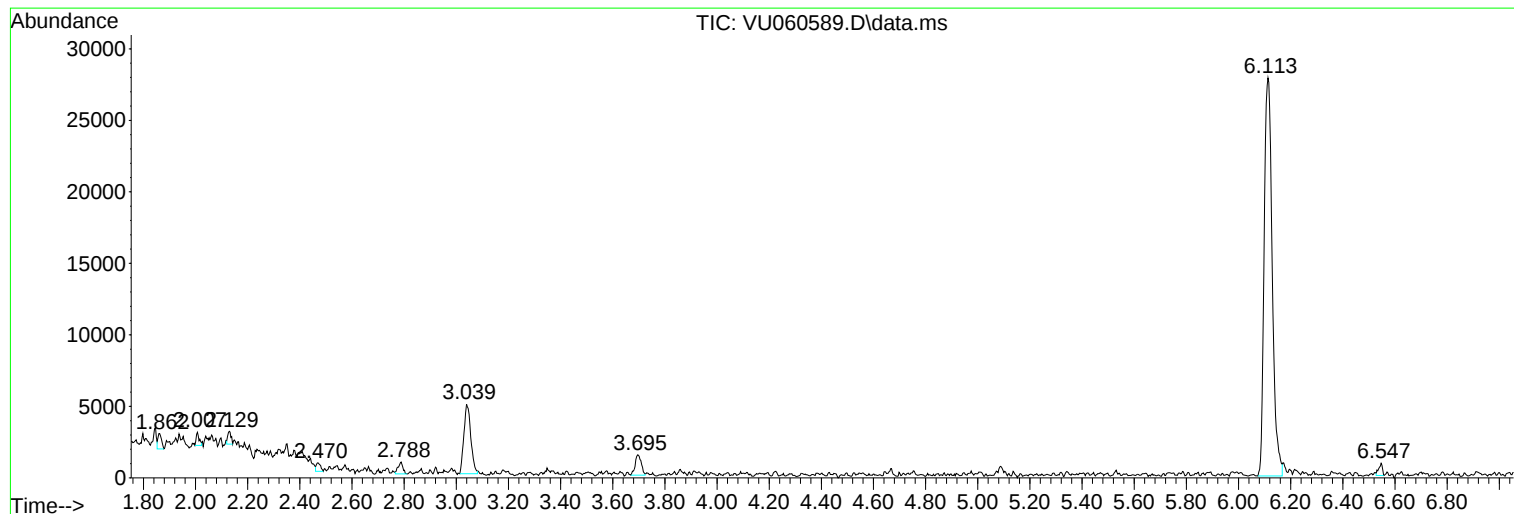

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090324\
Data File : VU060589.D
Acq On : 03 Sep 2024 16:53
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090324\
Data File : VU060589.D
Acq On : 03 Sep 2024 16:53
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------