

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090418\
 Data File : VU026521.D
 Acq On : 04 Sep 2018 13:35
 Operator : MD/SY
 Sample : J4694-06 25X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEE24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.619	7	9	12	rBV	141	119	0.01%	0.002%
2	0.709	33	37	40	rBV	277	204	0.02%	0.004%
3	0.796	62	64	67	rBV	127	110	0.01%	0.002%
4	0.851	76	81	84	rBV	138	187	0.02%	0.003%
5	0.928	102	105	107	rBB	168	107	0.01%	0.002%
6	0.973	113	119	123	rBB	207	274	0.03%	0.005%
7	0.999	123	127	130	rBV	131	163	0.02%	0.003%
8	1.015	130	132	137	rVB	282	213	0.02%	0.004%
9	1.085	138	154	171	rBV	172683	198846	22.45%	3.698%
10	1.397	244	251	263	rBV	82069	82248	9.29%	1.529%
11	1.680	330	339	355	rVB	61386	80376	9.08%	1.495%
12	2.272	511	523	536	rVB	118220	180622	20.40%	3.359%
13	2.442	574	576	579	rVB2	184	117	0.01%	0.002%
14	2.516	597	599	603	rVB	177	93	0.01%	0.002%
15	2.542	603	607	610	rBV	113	102	0.01%	0.002%
16	2.577	616	618	621	rBV2	172	102	0.01%	0.002%
17	2.703	650	657	667	rVB2	861	1214	0.14%	0.023%
18	2.818	691	693	696	rBV	125	100	0.01%	0.002%
19	2.841	696	700	707	rVB2	192	183	0.02%	0.003%
20	2.953	733	735	738	rBV	144	73	0.01%	0.001%
21	2.982	743	744	747	rVB	167	83	0.01%	0.002%
22	3.072	769	772	775	rBV2	151	95	0.01%	0.002%
23	3.301	841	843	847	rVB	196	93	0.01%	0.002%
24	3.330	848	852	854	rVB2	173	121	0.01%	0.002%
25	3.384	867	869	872	rVB	280	100	0.01%	0.002%
26	3.638	945	948	951	rVB	146	84	0.01%	0.002%
27	3.754	980	984	986	rBV	137	104	0.01%	0.002%
28	3.976	1051	1053	1056	rVB2	131	73	0.01%	0.001%
29	4.043	1071	1074	1078	rBV	100	70	0.01%	0.001%
30	4.178	1102	1116	1150	rBV2	45887	151535	17.11%	2.818%
31	4.391	1179	1182	1185	rBV	197	110	0.01%	0.002%
32	4.651	1245	1263	1288	rBV	82924	196089	22.14%	3.646%
33	4.754	1292	1295	1297	rBV	309	276	0.03%	0.005%
34	4.889	1330	1337	1344	rVB2	529	828	0.09%	0.015%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090418\
 Data File : VU026521.D
 Acq On : 04 Sep 2018 13:35
 Operator : MD/SY
 Sample : J4694-06 25X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEE24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

35	5.018	1376	1377	1378	rBV2	228	76	0.01%	0.001%
36	5.236	1440	1445	1451	rBV	186	309	0.03%	0.006%
37	5.342	1455	1478	1503	rVV2	166842	489970	55.33%	9.111%
38	5.616	1558	1563	1571	rBV	206	365	0.04%	0.007%
39	5.889	1632	1648	1667	rBV	204150	391852	44.25%	7.287%
40	6.188	1729	1741	1762	rBV2	62339	120249	13.58%	2.236%
41	6.333	1772	1786	1807	rBV	115271	228446	25.80%	4.248%
42	6.458	1822	1825	1827	rBV	153	67	0.01%	0.001%
43	6.561	1854	1857	1861	rVB	114	81	0.01%	0.002%
44	6.587	1862	1865	1870	rBV	75	76	0.01%	0.001%
45	6.709	1898	1903	1906	rBV	91	95	0.01%	0.002%
46	6.860	1947	1950	1956	rVB3	411	416	0.05%	0.008%
47	6.950	1976	1978	1983	rVB	166	69	0.01%	0.001%
48	6.979	1983	1987	1993	rBV	124	130	0.01%	0.002%
49	7.230	2054	2065	2081	rBV	61796	107091	12.09%	1.991%
50	7.464	2135	2138	2144	rBV	106	111	0.01%	0.002%
51	7.567	2156	2170	2187	rBV	221190	378732	42.77%	7.043%
52	7.715	2213	2216	2219	rVB2	154	116	0.01%	0.002%
53	7.854	2247	2259	2273	rBV	42639	72505	8.19%	1.348%
54	7.940	2282	2286	2288	rBV2	205	190	0.02%	0.004%
55	8.030	2311	2314	2316	rBV2	152	98	0.01%	0.002%
56	8.043	2316	2318	2320	rVB2	181	95	0.01%	0.002%
57	8.059	2320	2323	2328	rVB2	191	132	0.01%	0.002%
58	8.133	2339	2346	2349	rBV	148	165	0.02%	0.003%
59	8.185	2349	2362	2365	rBV	29036	47250	5.34%	0.879%
60	8.230	2366	2376	2392	rVV	514225	885546	100.00%	16.467%
61	8.313	2393	2402	2435	rVB	155371	268067	30.27%	4.985%
62	8.497	2456	2459	2465	rVB2	196	136	0.02%	0.003%
63	8.526	2465	2468	2470	rBV	322	198	0.02%	0.004%
64	8.564	2478	2480	2483	rVB2	213	117	0.01%	0.002%
65	8.606	2491	2493	2497	rVB	179	89	0.01%	0.002%
66	8.628	2497	2500	2505	rBV2	178	132	0.01%	0.002%
67	8.680	2513	2516	2521	rVB2	140	105	0.01%	0.002%
68	8.780	2544	2547	2551	rBV2	204	185	0.02%	0.003%
69	9.024	2620	2623	2626	rBV	132	85	0.01%	0.002%
70	9.091	2632	2644	2666	rBV	289709	469265	52.99%	8.726%
71	9.699	2832	2833	2838	rVB	207	93	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090418\
 Data File : VU026521.D
 Acq On : 04 Sep 2018 13:35
 Operator : MD/SY
 Sample : J4694-06 25X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEE24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

72	9.770	2853	2855	2858	rBV	162	71	0.01%	0.001%
73	10.178	2980	2982	2986	rBV	198	94	0.01%	0.002%
74	10.333	3028	3030	3035	rVB2	144	112	0.01%	0.002%
75	10.432	3049	3061	3078	rBV	158532	250566	28.30%	4.659%
76	10.516	3085	3087	3088	rBV	152	66	0.01%	0.001%
77	10.612	3106	3117	3135	rBV2	8780	16814	1.90%	0.313%
78	10.699	3141	3144	3145	rBV2	168	82	0.01%	0.002%
79	10.734	3153	3155	3158	rBV	98	71	0.01%	0.001%
80	10.783	3167	3170	3175	rBV	92	91	0.01%	0.002%
81	10.869	3193	3197	3199	rBV2	452	286	0.03%	0.005%
82	11.111	3270	3272	3276	rVB	169	89	0.01%	0.002%
83	11.484	3376	3388	3408	rBV	260934	403555	45.57%	7.504%
84	11.603	3423	3425	3432	rVB2	276	208	0.02%	0.004%
85	11.860	3494	3505	3525	rBV	216302	340146	38.41%	6.325%
86	11.988	3543	3545	3548	rVB	196	93	0.01%	0.002%
87	12.004	3548	3550	3554	rBV2	283	176	0.02%	0.003%
88	12.271	3630	3633	3639	rVB2	309	257	0.03%	0.005%
89	12.477	3687	3697	3708	rBV2	2040	3390	0.38%	0.063%
90	12.657	3751	3753	3758	rVB	205	101	0.01%	0.002%
91	12.927	3836	3837	3841	rBV	132	83	0.01%	0.002%
92	13.159	3907	3909	3911	rBV	167	80	0.01%	0.001%
93	13.265	3940	3942	3945	rBV	195	126	0.01%	0.002%
94	13.291	3946	3950	3954	rVB2	258	216	0.02%	0.004%
95	13.345	3965	3967	3968	rBV2	168	74	0.01%	0.001%
96	13.455	3998	4001	4004	rBV	214	132	0.01%	0.002%
97	13.487	4008	4011	4014	rBV2	236	175	0.02%	0.003%
98	13.625	4050	4054	4056	rBV	280	249	0.03%	0.005%
99	13.709	4078	4080	4085	rBV	205	80	0.01%	0.001%
100	14.278	4250	4257	4267	rBV2	1401	2240	0.25%	0.042%


Sum of corrected areas: 5377541

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU090418\
Data File : VU026521.D
Acq On : 04 Sep 2018 13:35
Operator : MD/SY
Sample : J4694-06 25X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEE24

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

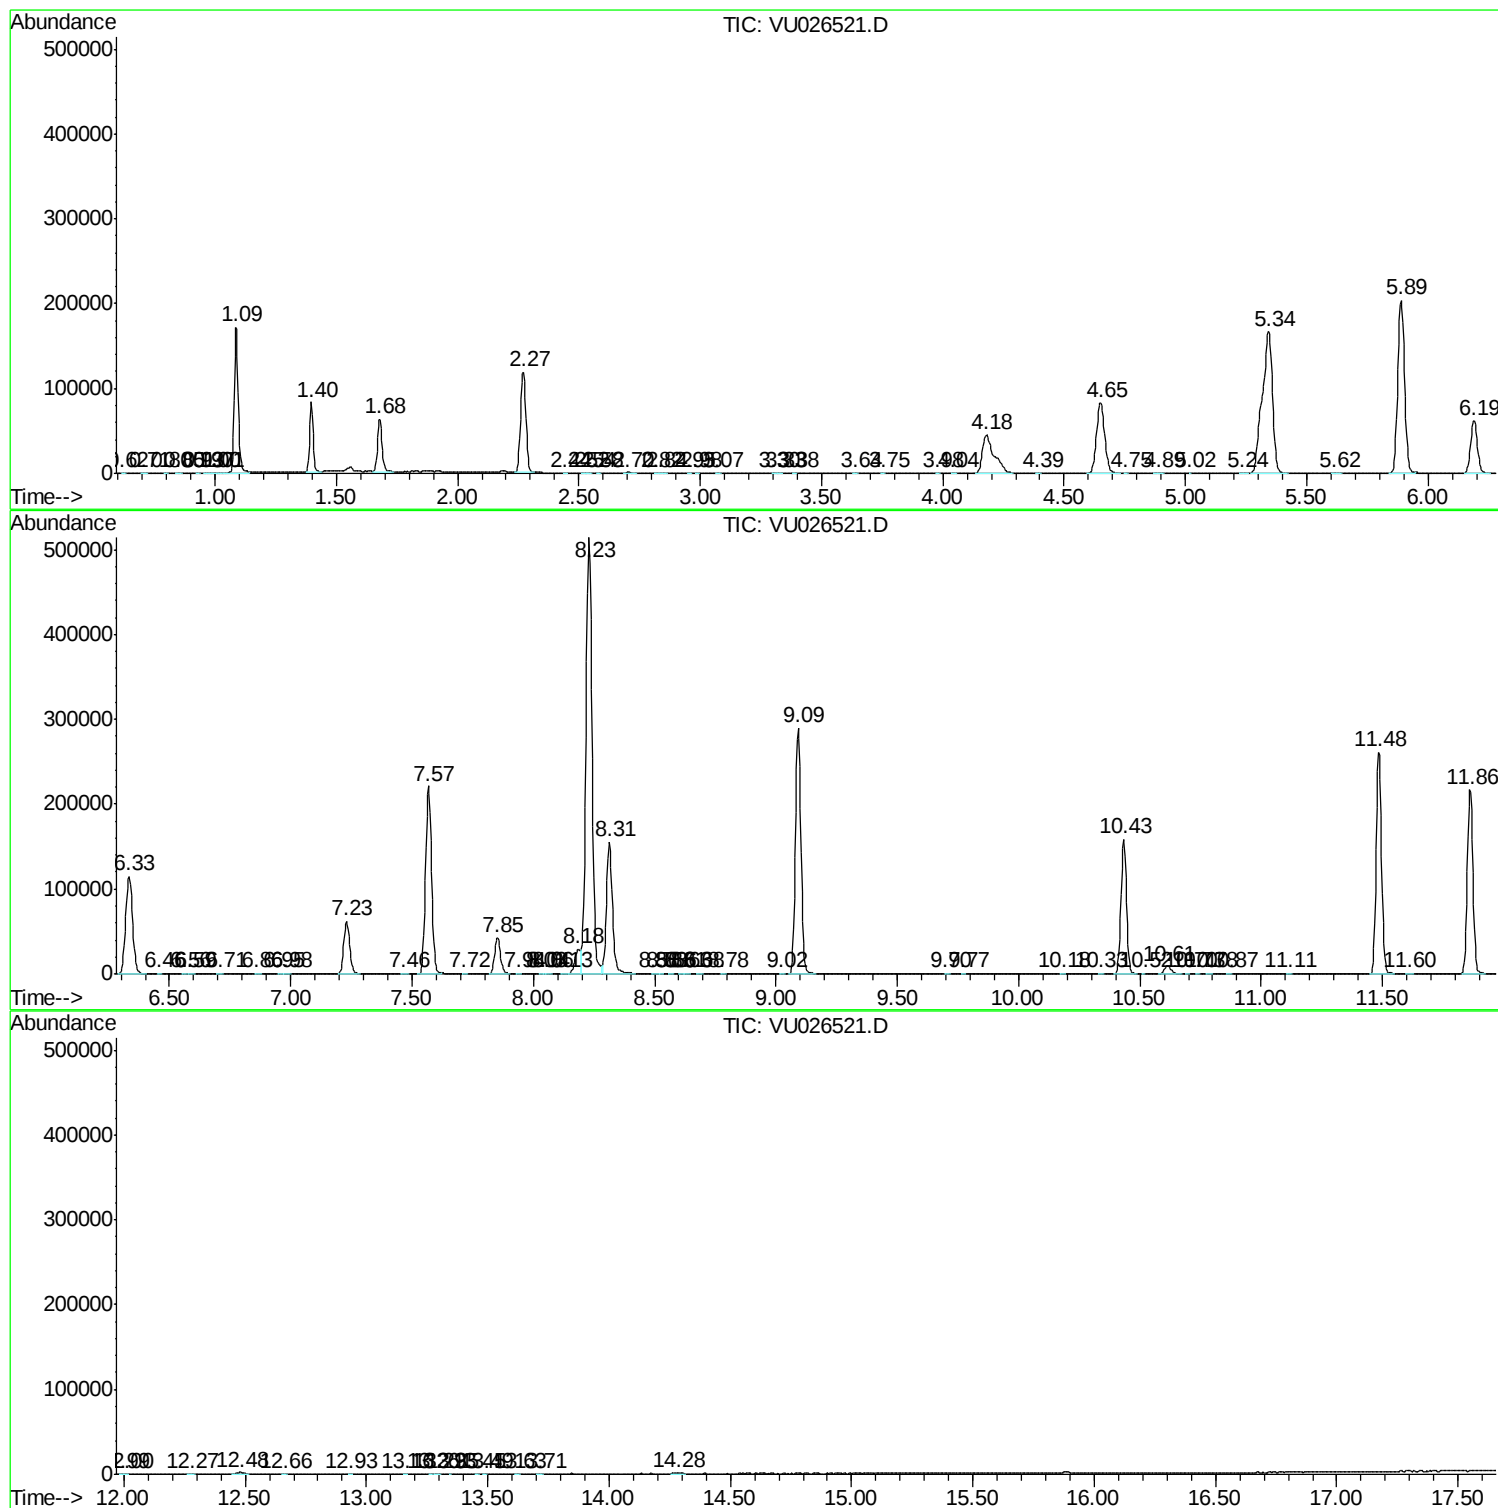

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU090418\
Data File : VU026521.D
Acq On : 04 Sep 2018 13:35
Operator : MD/SY
Sample : J4694-06 25X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEE24

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU090418\
Data File : VU026521.D
Acq On : 04 Sep 2018 13:35
Operator : MD/SY
Sample : J4694-06 25X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEE24

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc