

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090418\
 Data File : VU026523.D
 Acq On : 04 Sep 2018 14:21
 Operator : MD/SY
 Sample : J4694-05 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEE23

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.670	20	25	28	rBV	170	206	0.00%	0.000%
2	0.924	101	104	109	rBB	154	177	0.00%	0.000%
3	0.957	112	114	118	rBV	165	165	0.00%	0.000%
4	1.008	127	130	132	rBV	186	80	0.00%	0.000%
5	1.085	138	154	173	rBV	163820	191542	0.08%	0.081%
6	1.397	244	251	264	rVB	54113	54289	0.02%	0.023%
7	1.471	269	274	282	rVV	7291	7791	0.00%	0.003%
8	1.677	330	338	351	rVB	46019	58848	0.03%	0.025%
9	2.272	512	523	533	rBV	72512	110686	0.05%	0.047%
10	2.323	534	539	552	rVB3	4050	6391	0.00%	0.003%
11	2.394	558	561	562	rBV3	145	63	0.00%	0.000%
12	2.474	582	586	591	rVB	436	452	0.00%	0.000%
13	2.619	627	631	636	rVB2	302	352	0.00%	0.000%
14	2.703	651	657	663	rVB2	850	1125	0.00%	0.000%
15	2.831	686	697	711	rVB4	1973	4216	0.00%	0.002%
16	2.985	737	745	754	rBV2	2609	4247	0.00%	0.002%
17	3.069	768	771	775	rVB	116	78	0.00%	0.000%
18	3.101	777	781	787	rBV	305	413	0.00%	0.000%
19	3.188	804	808	811	rBV	191	173	0.00%	0.000%
20	3.220	815	818	823	rVB	204	164	0.00%	0.000%
21	3.278	833	836	840	rVB2	163	128	0.00%	0.000%
22	3.323	847	850	853	rBV	171	153	0.00%	0.000%
23	3.889	1022	1026	1030	rBV	101	99	0.00%	0.000%
24	3.960	1046	1048	1054	rBV	68	68	0.00%	0.000%
25	4.075	1081	1084	1088	rVB	101	75	0.00%	0.000%
26	4.182	1101	1117	1121	rBV	55976	112727	0.05%	0.048%
27	4.403	1182	1186	1188	rBV2	163	130	0.00%	0.000%
28	4.436	1192	1196	1200	rBV	173	110	0.00%	0.000%
29	4.461	1200	1204	1209	rBV	82	98	0.00%	0.000%
30	4.651	1246	1263	1285	rBV	77952	182723	0.08%	0.077%
31	4.767	1297	1299	1302	rVB2	166	66	0.00%	0.000%
32	4.821	1310	1316	1321	rBV2	180	252	0.00%	0.000%
33	4.886	1332	1336	1340	rBV2	278	270	0.00%	0.000%
34	4.915	1342	1345	1353	rVB4	443	544	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090418\
 Data File : VU026523.D
 Acq On : 04 Sep 2018 14:21
 Operator : MD/SY
 Sample : J4694-05 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEE23

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

35	4.985	1365	1367	1373	rVB2	173	145	0.00%	0.000%
36	5.082	1395	1397	1398	rBV2	208	83	0.00%	0.000%
37	5.095	1398	1401	1402	rVV	93	67	0.00%	0.000%
38	5.127	1409	1411	1415	rVB2	170	124	0.00%	0.000%
39	5.233	1442	1444	1447	rBV2	172	100	0.00%	0.000%
40	5.342	1455	1478	1504	rBV2	139023	433932	0.19%	0.184%
41	5.635	1567	1569	1574	rBV	74	62	0.00%	0.000%
42	5.796	1616	1619	1623	rVB	92	65	0.00%	0.000%
43	5.889	1634	1648	1671	rBV	150000	291084	0.13%	0.123%
44	6.188	1725	1741	1764	rBV	2181206	4098933	1.79%	1.735%
45	6.333	1773	1786	1803	rVB	109056	216531	0.09%	0.092%
46	6.413	1809	1811	1814	rVV3	162	103	0.00%	0.000%
47	6.429	1814	1816	1818	rVB3	199	71	0.00%	0.000%
48	6.490	1832	1835	1837	rBV2	134	71	0.00%	0.000%
49	6.786	1923	1927	1931	rBV2	247	233	0.00%	0.000%
50	6.863	1947	1951	1952	rBV2	176	116	0.00%	0.000%
51	7.005	1993	1995	1997	rBV	136	97	0.00%	0.000%
52	7.230	2054	2065	2083	rBV	44091	76386	0.03%	0.032%
53	7.310	2088	2090	2093	rVB	173	73	0.00%	0.000%
54	7.570	2157	2171	2188	rBV	171616	296481	0.13%	0.125%
55	7.693	2206	2209	2211	rBV	161	72	0.00%	0.000%
56	7.812	2244	2246	2249	rVB	193	72	0.00%	0.000%
57	7.853	2249	2259	2279	rBV	31911	52756	0.02%	0.022%
58	8.040	2315	2317	2321	rVB2	201	126	0.00%	0.000%
59	8.069	2324	2326	2332	rVB	178	92	0.00%	0.000%
60	8.271	2349	2389	2400	rBV4	88828922	228718477	100.00%	96.811%
61	9.091	2632	2644	2665	rBV	222355	356023	0.16%	0.151%
62	9.252	2688	2694	2703	rBV4	628	1080	0.00%	0.000%
63	9.377	2726	2733	2739	rBV2	4145	5538	0.00%	0.002%
64	9.471	2760	2762	2765	rBV2	314	188	0.00%	0.000%
65	9.722	2837	2840	2843	rVB	214	122	0.00%	0.000%
66	9.783	2852	2859	2868	rBV	3048	4064	0.00%	0.002%
67	9.821	2869	2871	2873	rBV	199	120	0.00%	0.000%
68	9.956	2910	2913	2916	rVB2	478	298	0.00%	0.000%
69	10.172	2976	2980	2989	rVB3	781	816	0.00%	0.000%
70	10.281	3011	3014	3017	rBV2	254	137	0.00%	0.000%
71	10.432	3049	3061	3078	rBV	169515	270915	0.12%	0.115%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090418\
 Data File : VU026523.D
 Acq On : 04 Sep 2018 14:21
 Operator : MD/SY
 Sample : J4694-05 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEE23

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

72	10.612	3106	3117	3131	rVB2	8120	15921	0.001%	0.0007%
73	10.683	3132	3139	3156	rVB	3617	6493	0.000%	0.0003%
74	10.773	3161	3167	3177	rBV3	1598	2079	0.000%	0.0001%
75	10.866	3194	3196	3200	rBV3	303	213	0.000%	0.0000%
76	10.976	3222	3230	3237	rBV4	1174	1727	0.000%	0.0001%
77	11.085	3261	3264	3265	rBV2	210	96	0.000%	0.0000%
78	11.152	3277	3285	3295	rVB3	3800	4930	0.000%	0.0002%
79	11.233	3307	3310	3312	rBV	431	301	0.000%	0.0000%
80	11.316	3334	3336	3339	rVB2	204	115	0.000%	0.0000%
81	11.484	3377	3388	3404	rBV	210211	327510	0.14%	0.139%
82	11.574	3410	3416	3422	rVB2	1524	1824	0.000%	0.0001%
83	11.863	3494	3506	3522	rBV	196937	316833	0.14%	0.134%
84	11.950	3531	3533	3534	rBV	260	91	0.000%	0.0000%
85	12.165	3598	3600	3603	rBV2	265	163	0.000%	0.0000%
86	12.220	3613	3617	3619	rVB	279	162	0.000%	0.0000%
87	12.390	3668	3670	3674	rBV2	307	183	0.000%	0.0000%
88	12.480	3688	3698	3707	rBV3	2006	3751	0.000%	0.0002%
89	12.567	3723	3725	3728	rBV2	270	205	0.000%	0.0000%
90	13.110	3891	3894	3895	rBV	291	148	0.000%	0.0000%
91	13.159	3907	3909	3912	rVB2	362	196	0.000%	0.0000%
92	13.307	3952	3955	3956	rBV	254	131	0.000%	0.0000%
93	13.416	3986	3989	3990	rBV2	263	166	0.000%	0.0000%
94	13.474	4004	4007	4009	rBV2	201	112	0.000%	0.0000%
95	14.027	4177	4179	4180	rBV2	238	105	0.000%	0.0000%
96	14.088	4196	4198	4200	rBV2	219	107	0.000%	0.0000%
97	14.175	4223	4225	4226	rBV	413	150	0.000%	0.0000%
98	14.278	4251	4257	4265	rBV2	1427	2076	0.000%	0.0001%
99	15.654	4682	4685	4688	rBV2	489	274	0.000%	0.0000%
100	15.885	4748	4757	4765	rBV2	1780	2967	0.000%	0.0001%


Sum of corrected areas: 236253583

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU090418\
Data File : VU026523.D
Acq On : 04 Sep 2018 14:21
Operator : MD/SY
Sample : J4694-05 5X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEE23

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

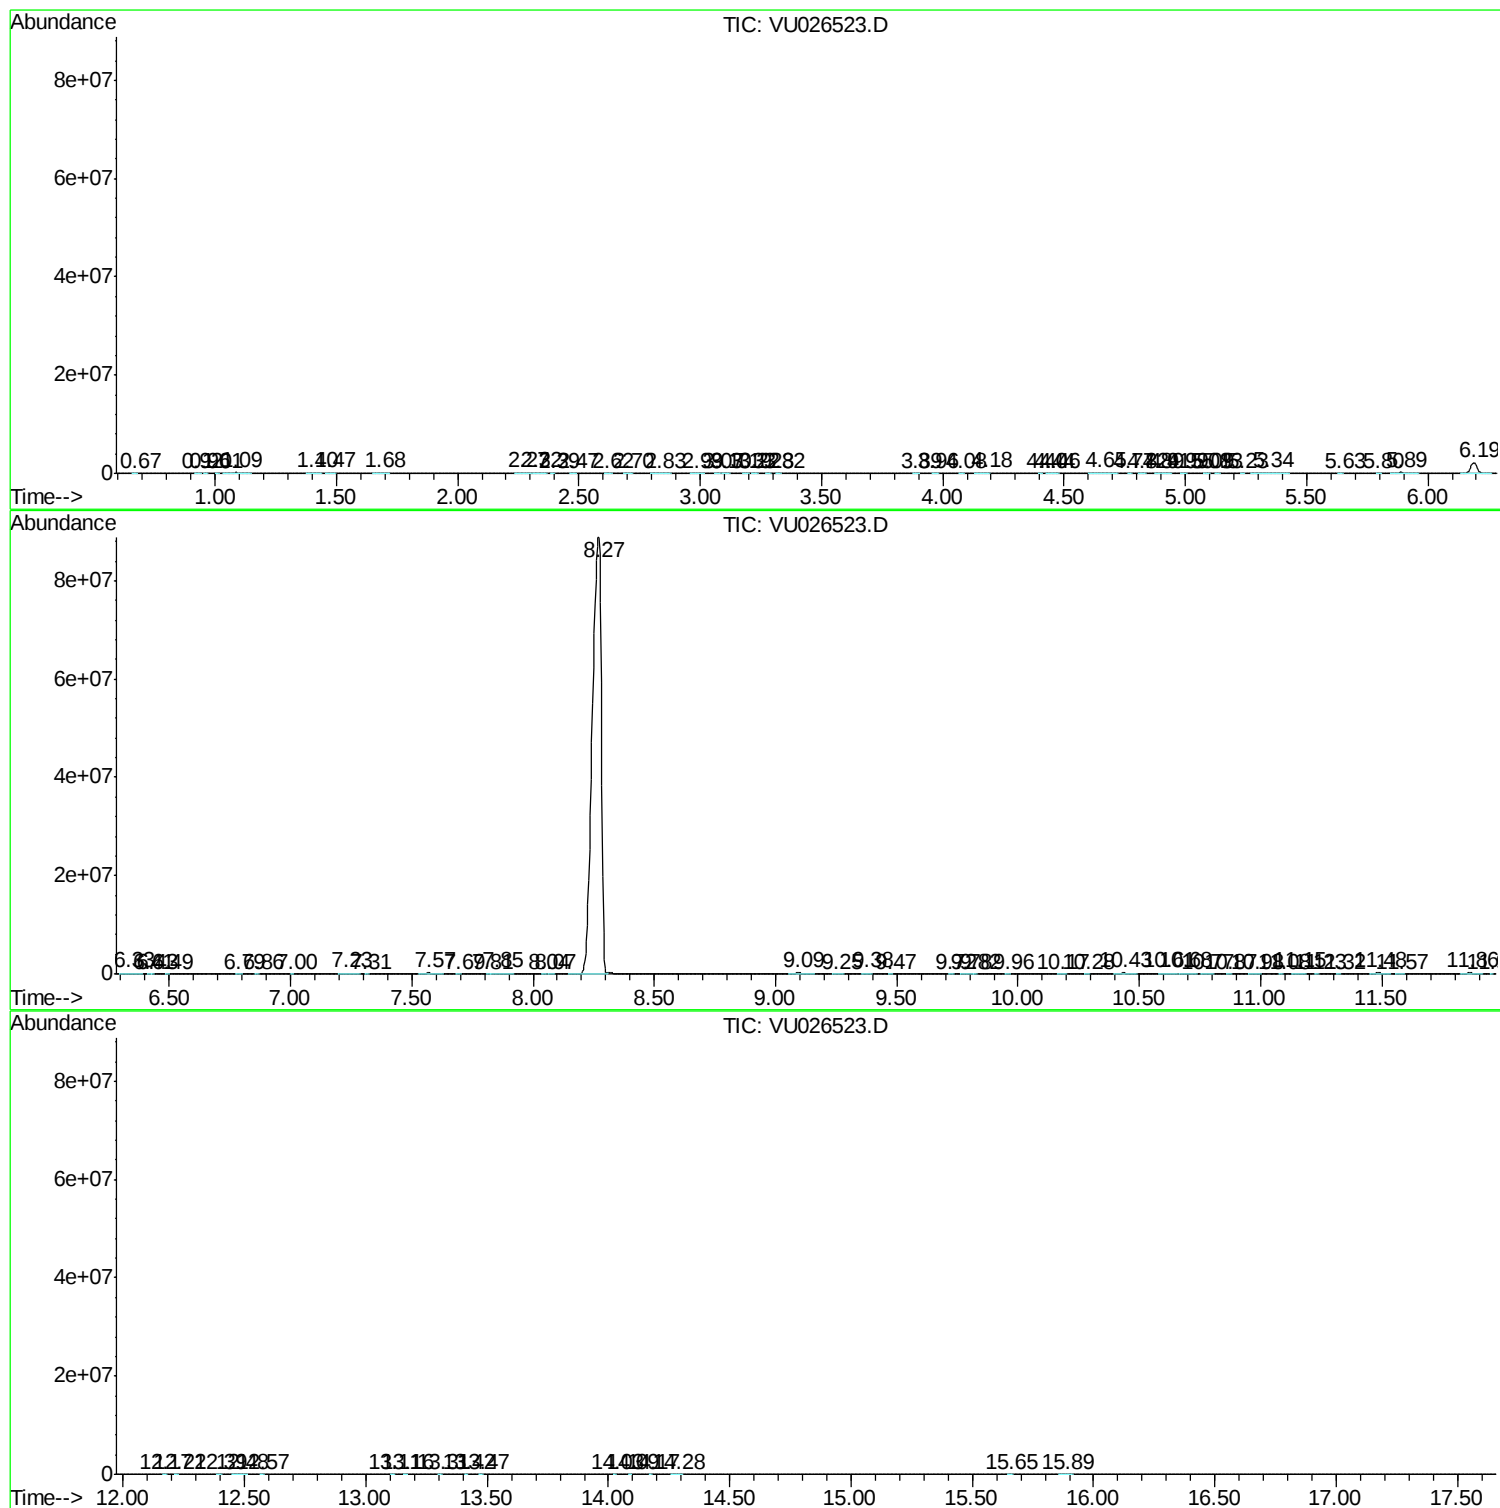

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU090418\
Data File : VU026523.D
Acq On : 04 Sep 2018 14:21
Operator : MD/SY
Sample : J4694-05 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEE23

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU090418\
Data File : VU026523.D
Acq On : 04 Sep 2018 14:21
Operator : MD/SY
Sample : J4694-05 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEE23

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc