

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090418\
 Data File : VU026525.D
 Acq On : 04 Sep 2018 16:54
 Operator : MD/SY
 Sample : VIBLK48
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK48

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.658	19	21	30	rVB2	208	188	0.03%	0.004%
2	0.703	31	35	39	rBV	95	97	0.02%	0.002%
3	0.928	101	105	110	rBB	175	224	0.04%	0.005%
4	0.963	111	116	119	rBV	179	207	0.03%	0.004%
5	0.995	124	126	127	rBV	137	55	0.01%	0.001%
6	1.089	137	155	178	rBV	547371	633834	100.00%	13.216%
7	1.397	244	251	263	rBV	70391	74274	11.72%	1.549%
8	1.677	331	338	353	rVB	58644	75216	11.87%	1.568%
9	2.272	512	523	534	rBV	130687	194207	30.64%	4.050%
10	2.507	594	596	600	rBV	133	61	0.01%	0.001%
11	2.584	617	620	622	rBV	102	55	0.01%	0.001%
12	2.613	622	629	637	rVB2	331	553	0.09%	0.012%
13	2.700	648	656	665	rBV3	1362	2026	0.32%	0.042%
14	2.835	690	698	699	rBV2	1234	1511	0.24%	0.032%
15	3.555	917	922	924	rBV	89	95	0.01%	0.002%
16	4.011	1060	1064	1069	rBV	190	261	0.04%	0.005%
17	4.047	1072	1075	1078	rVB	91	77	0.01%	0.002%
18	4.182	1102	1117	1144	rBV3	28549	85310	13.46%	1.779%
19	4.507	1212	1218	1221	rBV2	288	286	0.05%	0.006%
20	4.548	1228	1231	1235	rBV	81	57	0.01%	0.001%
21	4.571	1235	1238	1244	rBV	68	81	0.01%	0.002%
22	4.648	1244	1262	1285	rBV	86173	209225	33.01%	4.363%
23	4.770	1298	1300	1307	rBV2	179	229	0.04%	0.005%
24	4.799	1307	1309	1313	rBV2	164	152	0.02%	0.003%
25	4.841	1318	1322	1323	rBV	113	93	0.01%	0.002%
26	4.876	1329	1333	1336	rBV2	307	242	0.04%	0.005%
27	4.892	1336	1338	1340	rVB	291	135	0.02%	0.003%
28	4.953	1354	1357	1362	rBV2	314	353	0.06%	0.007%
29	5.011	1373	1375	1379	rVB	192	71	0.01%	0.001%
30	5.034	1379	1382	1385	rBV	104	79	0.01%	0.002%
31	5.053	1386	1388	1390	rVV	150	72	0.01%	0.002%
32	5.072	1392	1394	1396	rVB	163	71	0.01%	0.001%
33	5.092	1396	1400	1403	rBV	181	86	0.01%	0.002%
34	5.121	1406	1409	1415	rVB	153	78	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090418\
 Data File : VU026525.D
 Acq On : 04 Sep 2018 16:54
 Operator : MD/SY
 Sample : VIBLK48
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK48

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

35	5.179	1425	1427	1429	rBV	130	59	0.01%	0.001%
36	5.343	1445	1478	1497	rBV2	177701	519488	81.96%	10.832%
37	5.458	1511	1514	1517	rVB2	262	171	0.03%	0.004%
38	5.609	1559	1561	1566	rVB	144	75	0.01%	0.002%
39	5.683	1581	1584	1589	rBV	69	60	0.01%	0.001%
40	5.725	1595	1597	1601	rVB	147	69	0.01%	0.001%
41	5.822	1625	1627	1632	rVB	166	100	0.02%	0.002%
42	5.886	1632	1647	1670	rBV	194018	378533	59.72%	7.893%
43	6.008	1682	1685	1689	rBV2	155	114	0.02%	0.002%
44	6.079	1703	1707	1710	rBV	75	62	0.01%	0.001%
45	6.179	1731	1738	1742	rVV4	713	957	0.15%	0.020%
46	6.333	1772	1786	1810	rVB	122632	242878	38.32%	5.064%
47	6.423	1811	1814	1817	rBV	83	57	0.01%	0.001%
48	6.535	1847	1849	1851	rVB	107	60	0.01%	0.001%
49	6.625	1871	1877	1879	rBV	202	265	0.04%	0.006%
50	6.780	1922	1925	1926	rBV	152	66	0.01%	0.001%
51	6.793	1927	1929	1932	rVB	129	67	0.01%	0.001%
52	6.867	1949	1952	1954	rBV2	284	144	0.02%	0.003%
53	7.021	1997	2000	2003	rBV	101	84	0.01%	0.002%
54	7.043	2004	2007	2009	rVV	185	98	0.02%	0.002%
55	7.230	2053	2065	2084	rVB	46537	80603	12.72%	1.681%
56	7.301	2085	2087	2091	rVB	107	60	0.01%	0.001%
57	7.333	2094	2097	2101	rVB	117	77	0.01%	0.002%
58	7.355	2101	2104	2108	rBV	104	78	0.01%	0.002%
59	7.503	2147	2150	2152	rBV	88	64	0.01%	0.001%
60	7.568	2157	2170	2190	rBV	241118	405978	64.05%	8.465%
61	7.674	2201	2203	2208	rVB2	214	143	0.02%	0.003%
62	7.696	2208	2210	2213	rBV	111	76	0.01%	0.002%
63	7.738	2221	2223	2226	rVB	174	92	0.01%	0.002%
64	7.757	2227	2229	2235	rVB	178	88	0.01%	0.002%
65	7.850	2247	2258	2273	rBV	33732	55125	8.70%	1.149%
66	7.924	2279	2281	2283	rBV	219	144	0.02%	0.003%
67	7.995	2299	2303	2304	rBV	182	148	0.02%	0.003%
68	8.185	2347	2362	2372	rBV	27674	66368	10.47%	1.384%
69	8.313	2392	2402	2431	rVB	153036	265919	41.95%	5.545%
70	8.484	2449	2455	2458	rBV2	266	274	0.04%	0.006%
71	8.555	2474	2477	2485	rVB	100	88	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090418\
 Data File : VU026525.D
 Acq On : 04 Sep 2018 16:54
 Operator : MD/SY
 Sample : VIBLK48
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK48

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

72	8.622	2491	2498	2504	rBV	821	1109	0.17%	0.023%
73	8.735	2530	2533	2535	rBV	84	59	0.01%	0.001%
74	8.902	2582	2585	2589	rBV	114	89	0.01%	0.002%
75	9.092	2631	2644	2672	rBV	280056	450748	71.11%	9.399%
76	9.220	2679	2684	2687	rBV	134	136	0.02%	0.003%
77	9.686	2826	2829	2835	rBV	116	127	0.02%	0.003%
78	9.767	2851	2854	2856	rBV	88	59	0.01%	0.001%
79	9.825	2869	2872	2875	rBV	118	89	0.01%	0.002%
80	9.899	2893	2895	2901	rBV	77	80	0.01%	0.002%
81	10.043	2937	2940	2944	rBV	179	118	0.02%	0.002%
82	10.291	3014	3017	3020	rVB	150	70	0.01%	0.001%
83	10.432	3049	3061	3080	rBV	171657	271937	42.90%	5.670%
84	10.548	3095	3097	3100	rVB	207	96	0.02%	0.002%
85	10.616	3107	3118	3132	rBV2	8684	16626	2.62%	0.347%
86	10.876	3195	3199	3202	rBV2	181	213	0.03%	0.004%
87	10.998	3234	3237	3239	rBV	151	100	0.02%	0.002%
88	11.487	3377	3389	3406	rBV	245756	382321	60.32%	7.972%
89	11.812	3487	3490	3492	rVB	158	69	0.01%	0.001%
90	11.863	3492	3506	3526	rBV	230884	368204	58.09%	7.678%
91	11.979	3540	3542	3546	rVB2	334	192	0.03%	0.004%
92	12.108	3580	3582	3584	rBV2	143	66	0.01%	0.001%
93	12.378	3664	3666	3668	rBV	185	89	0.01%	0.002%
94	12.413	3675	3677	3681	rVB2	231	138	0.02%	0.003%
95	12.484	3687	3699	3707	rBV3	2296	3511	0.55%	0.073%
96	12.519	3708	3710	3715	rVB	187	105	0.02%	0.002%
97	13.095	3886	3889	3891	rBV	210	125	0.02%	0.003%
98	13.780	4100	4102	4103	rBV	137	56	0.01%	0.001%
99	13.815	4107	4113	4118	rVV2	554	747	0.12%	0.016%
100	14.336	4272	4275	4278	rBV2	301	208	0.03%	0.004%


Sum of corrected areas: 4795780

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU090418\
Data File : VU026525.D
Acq On : 04 Sep 2018 16:54
Operator : MD/SY
Sample : VIBLK48
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK48

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

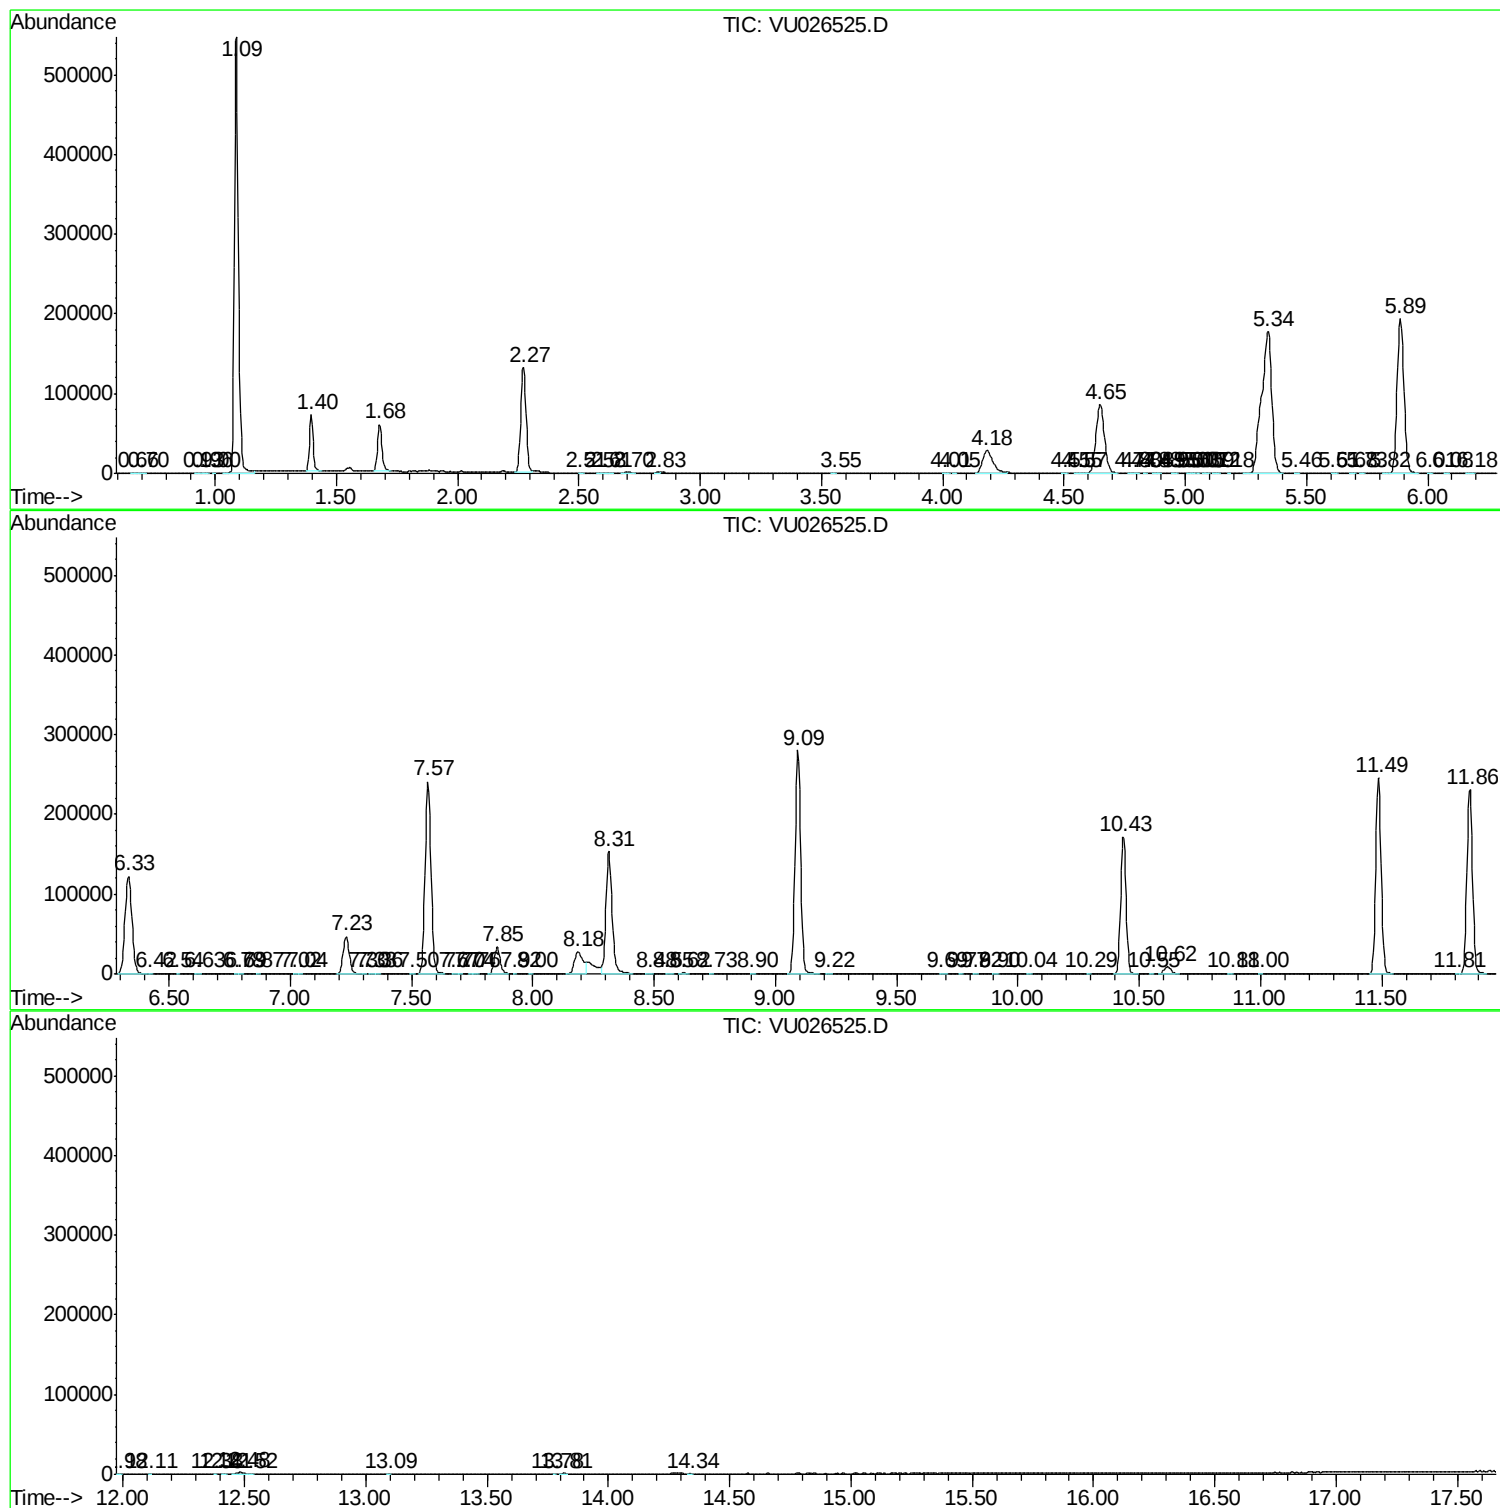

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU090418\
Data File : VU026525.D
Acq On : 04 Sep 2018 16:54
Operator : MD/SY
Sample : VIBLK48
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK48

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU090418\
Data File : VU026525.D
Acq On : 04 Sep 2018 16:54
Operator : MD/SY
Sample : VIBLK48
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK48

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc