


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090418\
 Data File : VU026514.D
 Acq On : 04 Sep 2018 08:15
 Operator : MD/SY
 Sample : BFB48
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB48

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis
 Last Update : Thu Sep 06 05:59:28 2018

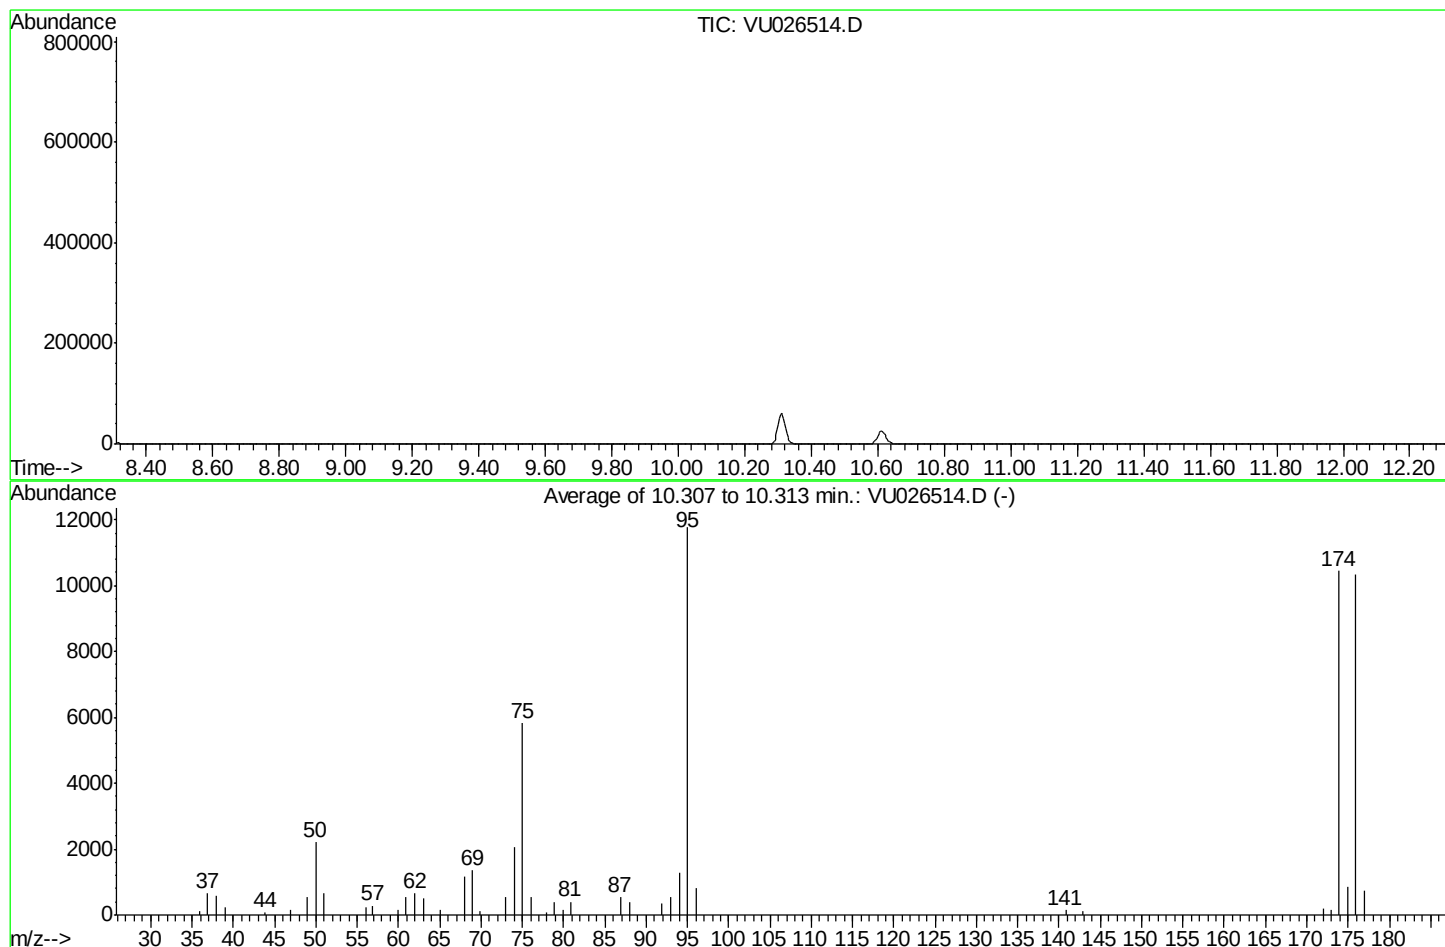

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	2202	PASS
75	95	30	80	49.4	5820	PASS
95	95	100	100	100.0	11770	PASS
96	95	5	9	7.0	822	PASS
173	174	0.00	2	1.6	164	PASS
174	95	50	120	88.7	10438	PASS
175	174	5	9	8.3	864	PASS
176	174	95	101	99.2	10356	PASS
177	176	5	9	7.0	725	PASS

m/z	Abundance
43.90	166.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
35.90	129.0
36.90	653.0
38.00	598.0
39.00	234.0
43.90	230.0
47.00	128.0
49.00	531.0
50.00	2227.0
51.00	689.0
56.00	229.0
56.90	292.0
60.00	155.0
60.90	572.0
62.00	586.0
63.00	468.0
65.00	166.0
68.00	1213.0
69.00	1290.0
69.90	107.0
72.90	519.0
74.00	1998.0
75.00	5818.0
76.00	504.0
77.90	127.0
78.90	378.0
79.90	129.0
80.90	414.0
86.90	466.0
87.90	419.0
91.90	320.0
92.90	529.0
94.00	1226.0
95.00	11736.0
96.00	832.0
140.80	159.0
142.90	116.0
172.00	207.0
172.90	159.0
173.90	10191.0
174.90	838.0
175.90	9913.0
176.90	722.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
35.90	121.0
36.90	671.0
38.00	624.0
39.00	239.0
44.00	249.0
47.00	150.0
49.00	555.0
50.00	2266.0
51.00	688.0
56.00	235.0
56.90	287.0
60.00	166.0
60.90	564.0
62.00	674.0
63.00	521.0
65.00	189.0
68.00	1209.0
69.00	1408.0
69.90	114.0
72.90	562.0
74.00	2148.0
75.00	5929.0
76.00	537.0
77.90	134.0
78.90	406.0
79.90	156.0
80.90	410.0
86.90	536.0
88.00	409.0
91.80	365.0
93.00	568.0
94.00	1259.0
95.00	12157.0
96.00	855.0
140.90	162.0
142.90	115.0
171.90	214.0
172.90	175.0
173.90	10741.0
174.90	899.0
175.90	10770.0
176.90	739.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
35.90	100.0
36.90	648.0
38.00	574.0
39.00	252.0
43.90	241.0
47.00	163.0
49.00	505.0
50.00	2113.0
51.00	610.0
56.00	196.0
56.90	282.0
59.90	153.0
60.90	515.0
62.00	669.0
63.00	529.0
65.00	164.0
68.00	1119.0
69.00	1345.0
69.80	102.0
73.00	574.0
74.00	2085.0
75.00	5715.0
76.00	567.0
78.80	388.0
79.90	152.0
80.80	380.0
86.90	599.0
88.00	366.0
91.80	353.0
93.00	581.0
94.00	1310.0
95.00	11417.0
96.00	779.0
140.90	146.0
142.90	113.0
171.90	206.0
172.90	160.0
173.90	10384.0
174.90	856.0
175.90	10385.0
176.90	715.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48