


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU090419\
Data File : VU034212.D
Acq On : 03 Sep 2019 09:00
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
Title : SW846 8260
Last Update : Thu Aug 29 04:11:12 2019

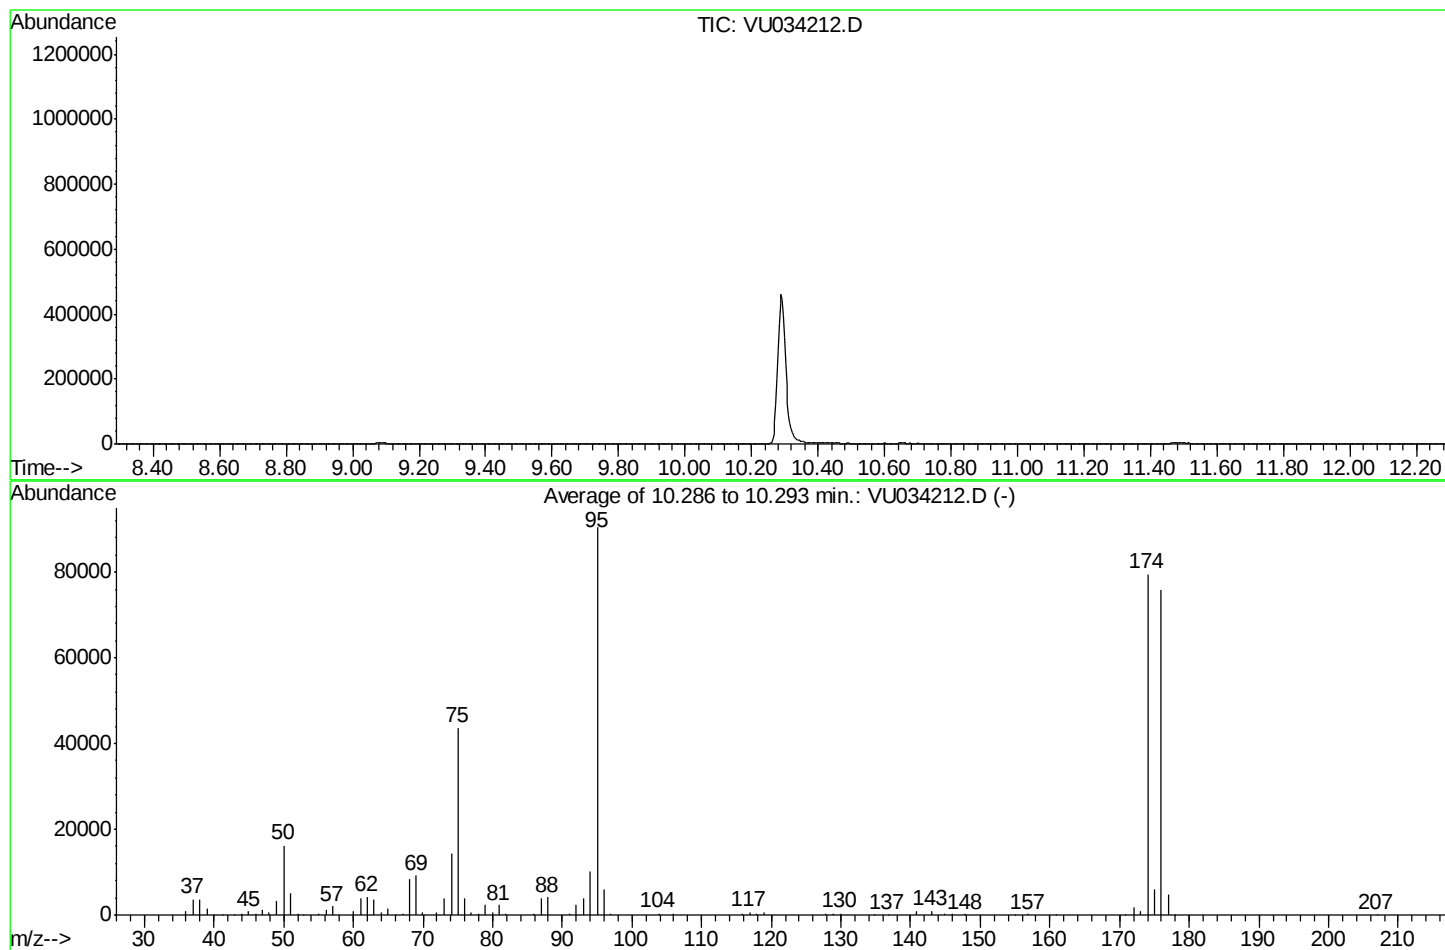

AutoFind: Scans 2860, 2861, 2862; Background Corrected with Scan 2847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	16197	PASS
75	95	30	60	48.3	43650	PASS
95	95	100	100	100.0	90434	PASS
96	95	5	9	6.7	6047	PASS
173	174	0.00	2	1.3	1033	PASS
174	95	50	100	87.9	79512	PASS
175	174	5	9	7.5	5999	PASS
176	174	95	101	95.4	75832	PASS
177	176	5	9	6.2	4739	PASS