




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090424\
Data File : VU060597.D
Acq On : 04 Sep 2024 14:15
Operator : MD/SY
Sample : P3809-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YE3F4

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/06/2024
Supervised By :Semsettin Yesilyurt 09/06/2024

Quant Time: Sep 05 03:56:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 05 03:55:13 2024
Response via : Initial Calibration

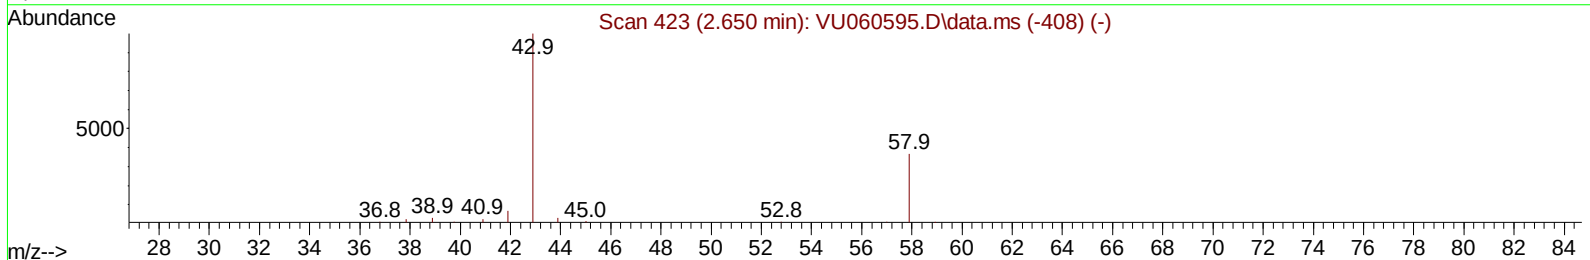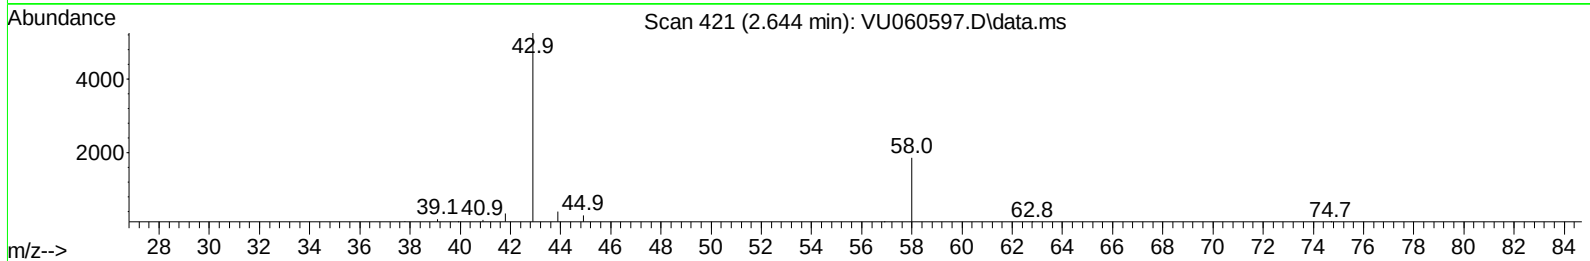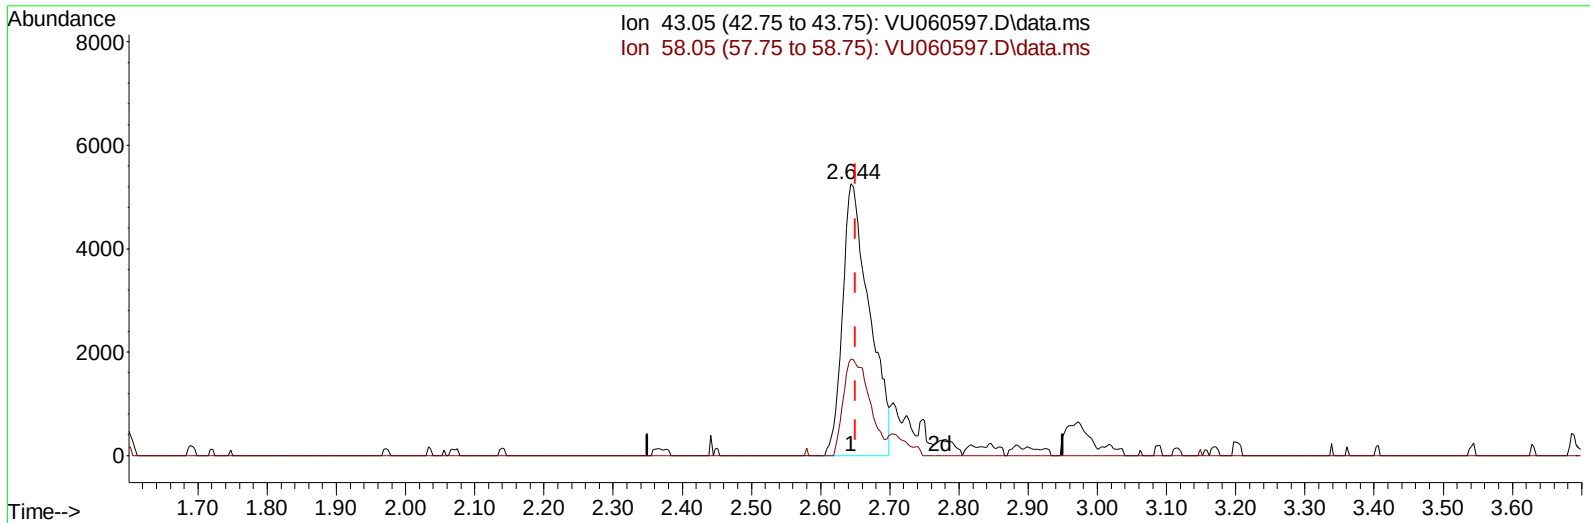

TIC: VU060597.D\data.ms

(13) Acetone (T)

2.644min (-0.006) 8.44 ug/L

response 14120

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.40	34.40
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090424\
Data File : VU060597.D
Acq On : 04 Sep 2024 14:15
Operator : MD/SY
Sample : P3809-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YE3F4

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/06/2024
Supervised By :Semsettin Yesilyurt 09/06/2024

Quant Time: Sep 05 03:56:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 05 03:55:13 2024
Response via : Initial Calibration

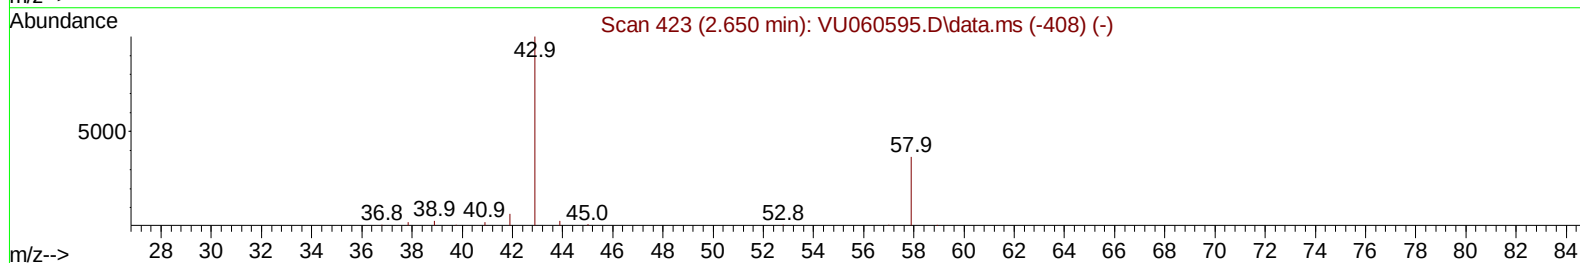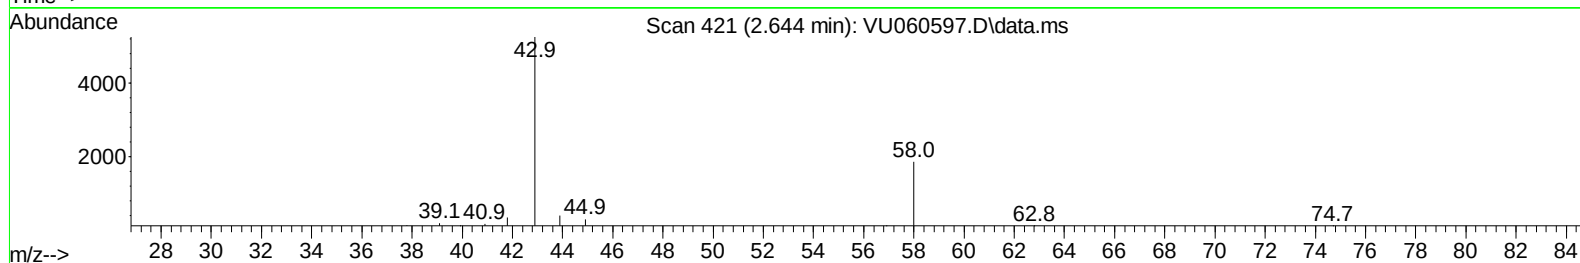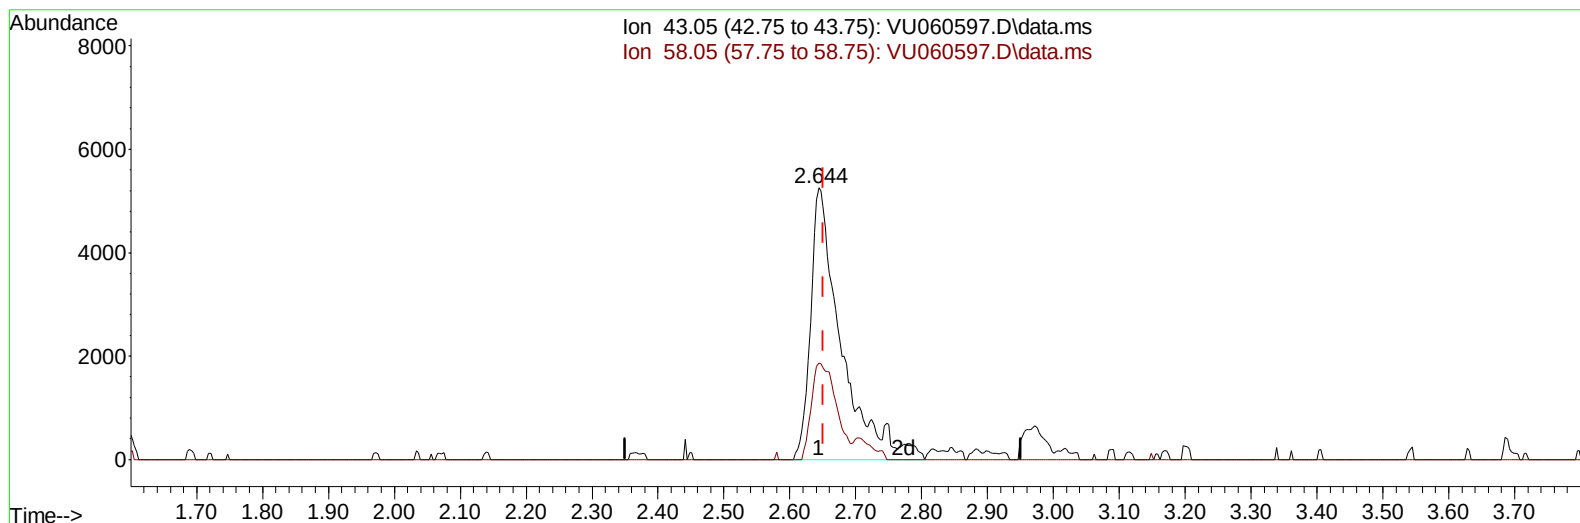

TIC: VU060597.D\data.ms

(13) Acetone (T)

2.644min (-0.006) 10.12 ug/L m

response 16941

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.40	28.67
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090424\
 Data File : VU060597.D
 Acq On : 04 Sep 2024 14:15
 Operator : MD/SY
 Sample : P3809-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YE3F4

Manual IntegrationsAPPROVED

Quant Time: Sep 05 03:56:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 05 03:55:13 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/06/2024
 Supervised By :Semsettin Yesilyurt 09/06/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		131712	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		139052	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.808	152		56535	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		37938	6.521	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	130.400%#	
7) Chloroethane-d5	1.911	69		36785	4.173	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	83.400%	
11) 1,1-Dichloroethene-d2	2.564	65		17731	5.171	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	103.400%	
20) 2-Butanone-d5	4.634	46		93991	46.984	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	93.960%	
24) Chloroform-d	5.056	84		84832	5.115	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	102.200%	
26) 1,2-Dichloroethane-d4	5.699	65		41929	4.845	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	96.800%	
32) Benzene-d6	5.721	84		155153	5.103	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	102.000%	
36) 1,2-Dichloropropane-d6	6.682	67		52524	5.354	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	107.000%	
41) Toluene-d8	7.891	98		124823	4.376	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	87.600%	
43) trans-1,3-Dichloroprop...	8.178	79		14814	4.220	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	84.400%	
46) 2-Hexanone-d5	8.631	63		61558	36.623	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	73.240%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84		38658	4.428	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	88.600%	
66) 1,2-Dichlorobenzene-d4	12.187	152		44361	5.322	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	106.400%	
Target Compounds							Qvalue
13) Acetone	2.644	43		16941m	10.120	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090424\
Data File : VU060597.D
Acq On : 04 Sep 2024 14:15
Operator : MD/SY
Sample : P3809-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YE3F4

Manual IntegrationsAPPROVED

Quant Time: Sep 05 03:56:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 05 03:55:13 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/06/2024
Supervised By :Semsettin Yesilyurt 09/06/2024

