

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090424\
 Data File : VU060601.D
 Acq On : 04 Sep 2024 15:52
 Operator : MD/SY
 Sample : VIBLK130
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK130

Quant Time: Sep 05 03:57:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 05 03:55:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	136607	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	145760	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	57573	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	38001	6.298	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	126.000%
7) Chloroethane-d5	1.911	69	36730	4.018	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	80.400%
11) 1,1-Dichloroethene-d2	2.560	65	17387	4.889	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	97.800%
20) 2-Butanone-d5	4.634	46	95083	45.827	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.660%
24) Chloroform-d	5.058	84	82055	4.770	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.400%
26) 1,2-Dichloroethane-d4	5.698	65	42488	4.733	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.600%
32) Benzene-d6	5.721	84	160870	5.047	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.000%
36) 1,2-Dichloropropane-d6	6.682	67	52601	5.115	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.200%
41) Toluene-d8	7.894	98	129334	4.325	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.600%
43) trans-1,3-Dichloroprop...	8.177	79	14701	3.995	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.800%
46) 2-Hexanone-d5	8.631	63	63554	36.071	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	72.140%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	38772	4.237	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.800%
66) 1,2-Dichlorobenzene-d4	12.190	152	44764	5.273	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.400%
Target Compounds						
					Qvalue	
16) Methylene chloride	3.042	84	5238	0.482	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090424\
Data File : VU060601.D
Acq On : 04 Sep 2024 15:52
Operator : MD/SY
Sample : VIBLK130
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK130


Quant Time: Sep 05 03:57:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 05 03:55:13 2024
Response via : Initial Calibration

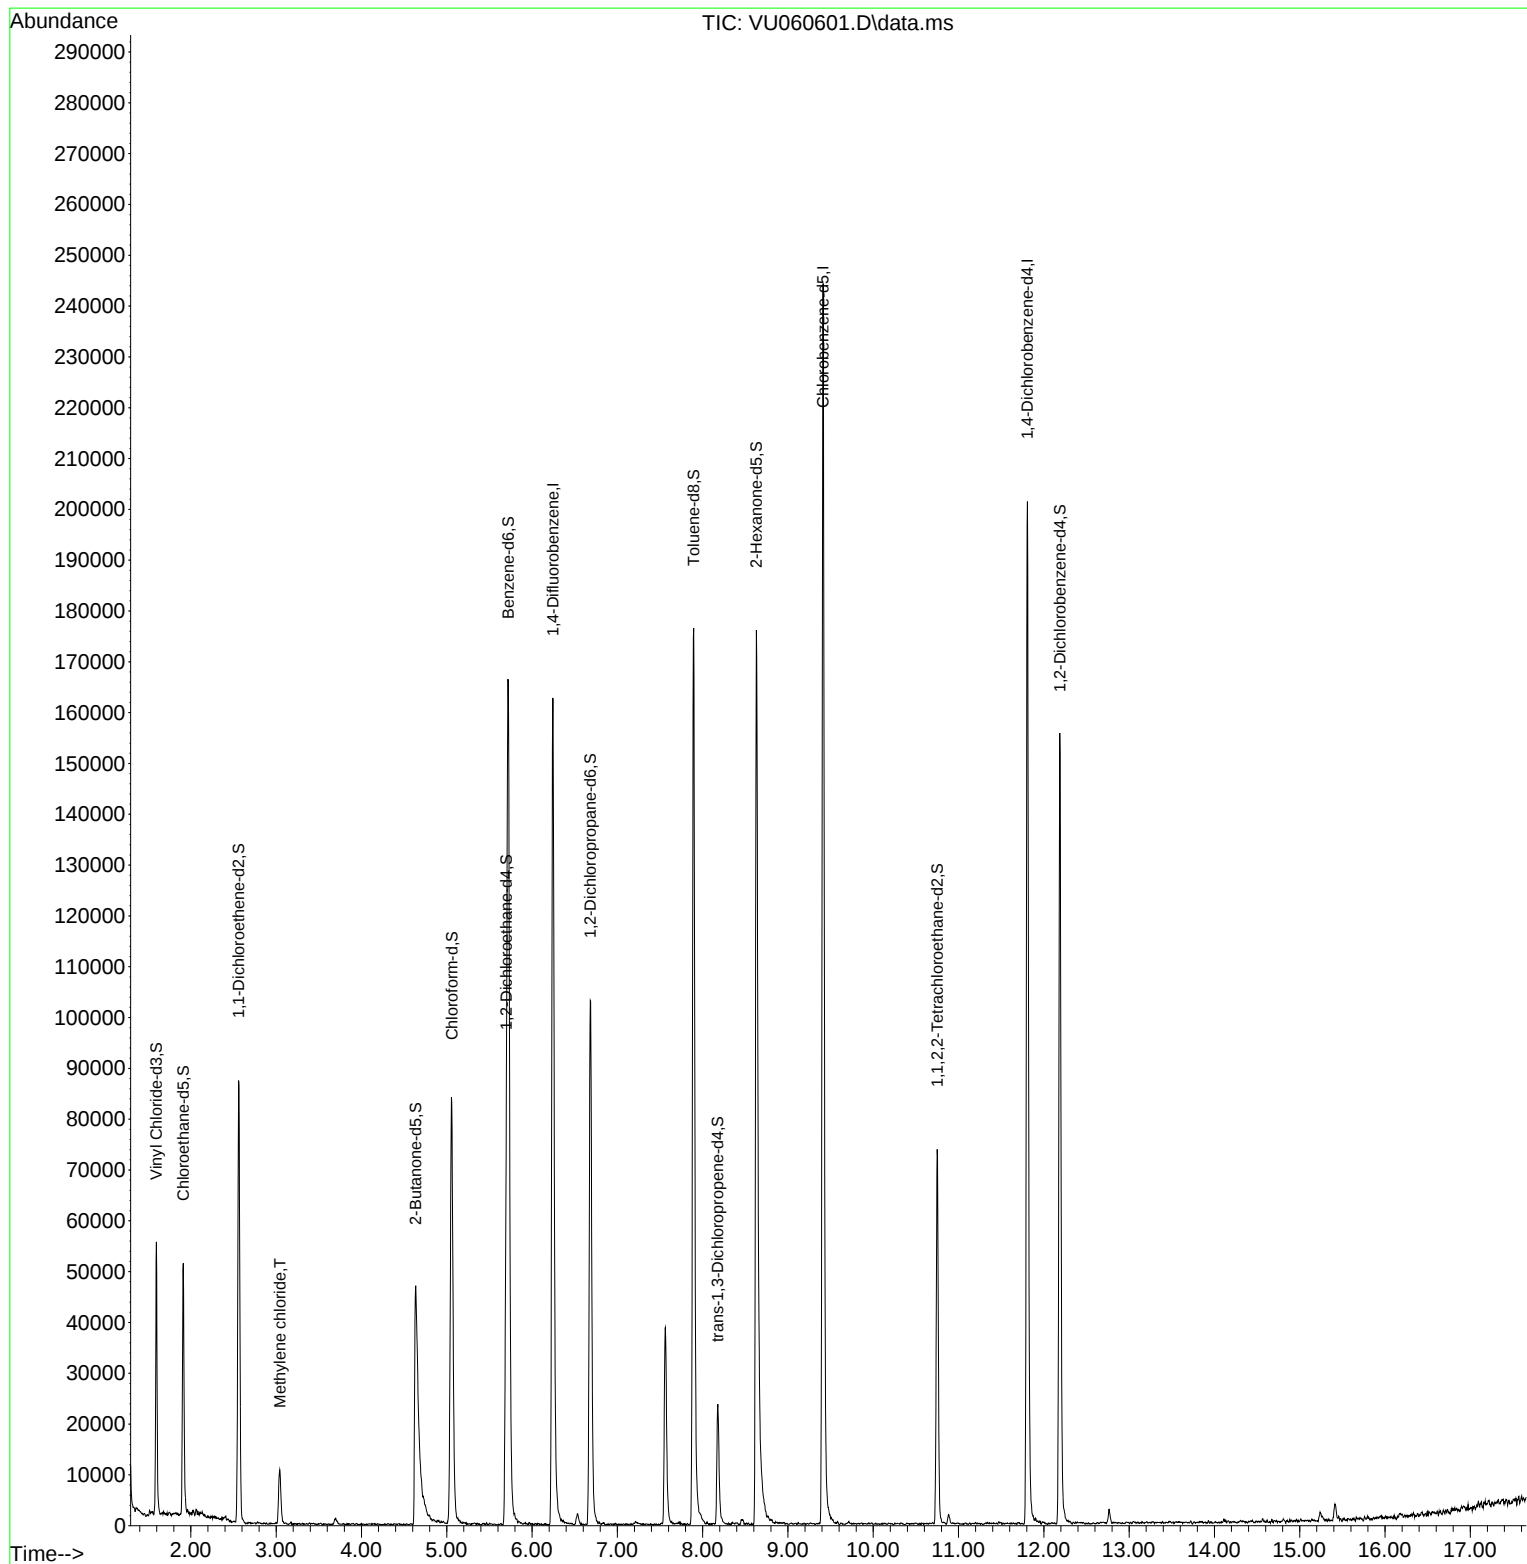

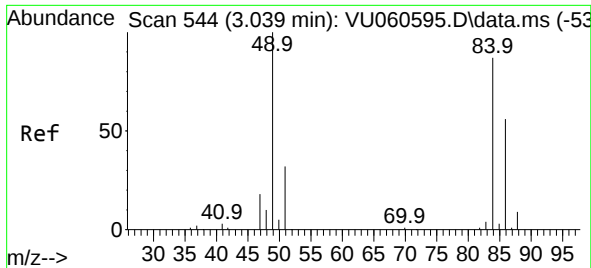

#16
Methylene chloride
Concen: 0.482 ug/L
RT: 3.042 min Scan# 54
Delta R.T. 0.003 min
Lab File: VU060601.D
Acq: 04 Sep 2024 15:52

Instrument :
MSVOA_U
ClientSampleId :
VIBLK130

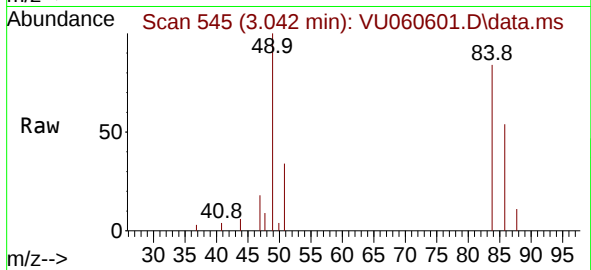

Tgt Ion: 84 Resp: 5238
Ion Ratio Lower Upper
84 100
86 63.7 47.5 88.3
49 118.6 94.4 175.2

