


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090424\
Data File : VU060594.D
Acq On : 04 Sep 2024 10:04
Operator : MD/SY
Sample : BFB193
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB193

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Sep 06 02:03:06 2024

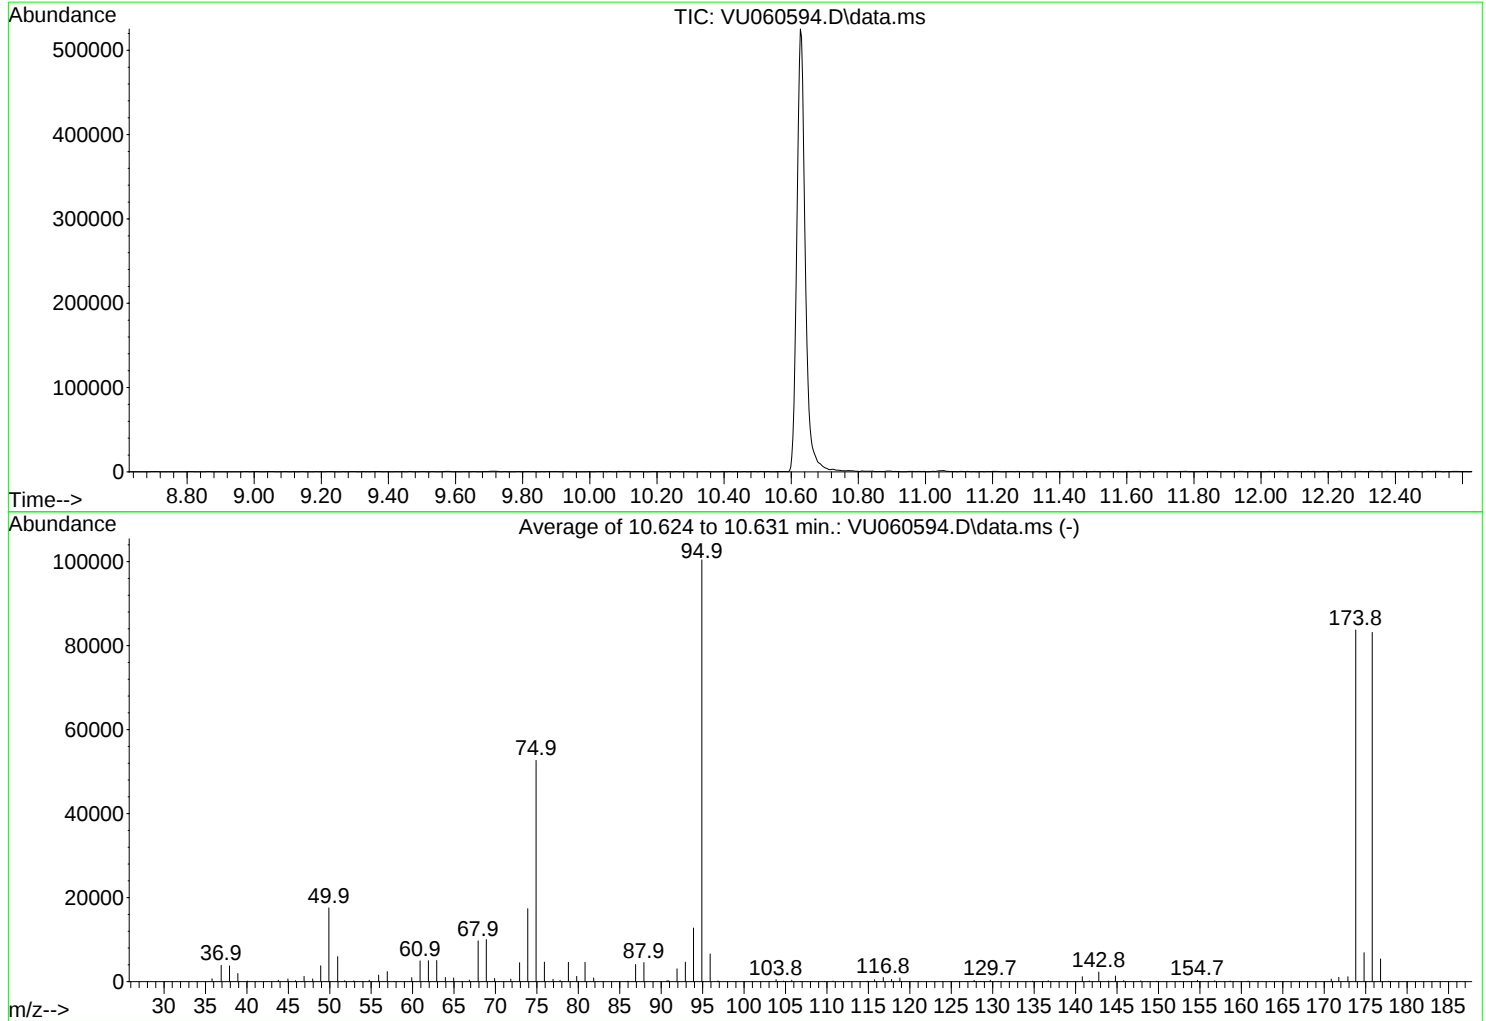

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	17576	PASS
75	95	30	80	52.5	52696	PASS
95	95	100	100	100.0	100421	PASS
96	95	5	9	6.6	6610	PASS
173	174	0.00	2	1.4	1196	PASS
174	95	50	120	83.4	83736	PASS
175	174	5	9	8.2	6889	PASS
176	174	95	101	99.3	83165	PASS
177	176	5	9	6.5	5426	PASS

m/z	Abundance
39.80	128.0
43.70	323.0

Instrument :
MSVOA_U
ClientSampleId :
BFB193

m/z	Abundance
35.80	648.0
36.90	4001.0
37.90	3565.0
38.90	1896.0
40.20	143.0
43.80	711.0
44.90	641.0
45.80	249.0
46.90	1285.0
48.00	533.0
48.90	3689.0
49.90	17304.0
50.90	5897.0
51.80	197.0
52.90	190.0
53.90	104.0
54.80	366.0
55.90	1345.0
57.00	2282.0
59.90	945.0
60.90	4652.0
61.90	4731.0
62.90	4875.0
64.00	970.0
64.90	858.0
66.90	369.0
67.90	9586.0
68.90	9889.0
69.90	792.0
71.90	583.0
72.90	4376.0
73.90	16600.0
74.90	50352.0
75.90	4589.0
77.00	488.0
77.70	260.0
78.80	4539.0
79.80	1196.0
80.80	4417.0
81.80	905.0
85.90	220.0
86.90	4103.0
87.90	4352.0
90.70	396.0
91.90	2936.0
92.90	4438.0
93.90	11843.0
94.90	96136.0
95.90	6277.0
96.80	132.0
103.80	516.0
104.80	136.0
105.70	414.0
110.70	166.0
114.90	124.0
115.80	469.0
116.80	980.0
117.80	507.0
118.80	816.0
127.80	275.0
128.50	115.0
129.70	383.0
134.80	198.0
136.70	215.0
140.80	1083.0
141.80	198.0
142.80	2178.0
144.00	190.0
144.80	1304.0
145.80	293.0
147.90	155.0
149.70	103.0
154.70	327.0
156.80	155.0
158.60	122.0
160.80	105.0
170.80	680.0
171.70	926.0
173.80	78848.0
174.80	6327.0
175.80	79000.0
176.80	5461.0
177.80	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB193

m/z	Abundance
35.80	758.0
36.90	3961.0
37.90	3838.0
38.90	1971.0
40.20	162.0
43.80	668.0
44.90	635.0
45.80	217.0
46.90	1325.0
48.00	706.0
48.90	3904.0
49.90	18088.0
50.90	6177.0
51.80	243.0
52.90	215.0
53.90	102.0
54.80	379.0
55.90	1631.0
57.00	2460.0
57.70	136.0
59.90	977.0
60.90	5139.0
61.90	5048.0
62.90	5217.0
64.00	1018.0
65.00	901.0
66.80	405.0
67.90	9932.0
68.90	10367.0
69.90	794.0
71.90	616.0
72.90	4678.0
73.90	17888.0
74.90	54400.0
75.90	4859.0
77.00	588.0
77.80	329.0
78.80	4673.0
79.80	1301.0
80.80	4796.0
81.90	893.0
86.00	177.0
86.90	4251.0
87.90	4729.0
90.70	373.0
90.90	374.0
91.90	3126.0
92.90	4756.0
93.90	13257.0
94.90	103400.0
95.90	6774.0
96.90	181.0
103.80	530.0
104.70	192.0
105.80	335.0
109.70	104.0
110.70	151.0
112.70	125.0
114.80	112.0
115.80	454.0
116.80	1014.0
117.80	549.0
118.80	905.0
127.80	317.0
128.60	118.0
128.80	116.0
129.70	370.0
130.70	108.0
134.80	122.0
136.70	217.0
140.80	1188.0
141.60	193.0
142.80	2438.0
144.00	181.0
144.80	1411.0
145.80	273.0
147.80	200.0
148.70	104.0
149.80	116.0
152.60	102.0
154.70	331.0
156.80	230.0
158.70	139.0
160.80	143.0
170.80	648.0
171.80	1069.0
172.90	1888.0
173.80	86248.0
174.80	7096.0
175.80	85904.0
176.80	5559.0
177.80	129.0

Instrument :
MSVOA_U
ClientSampleId :
BFB193

m/z	Abundance
35.80	702.0
36.90	3734.0
37.90	3853.0
38.90	1940.0
40.00	185.0
43.90	609.0
45.00	658.0
45.90	207.0
46.90	1206.0
47.90	696.0
48.90	3774.0
49.90	17336.0
51.00	5809.0
51.80	285.0
52.90	199.0
54.70	332.0
55.90	1692.0
56.90	2525.0
57.80	155.0
59.90	908.0
60.90	5058.0
61.90	5234.0
62.90	4977.0
63.90	961.0
65.00	849.0
65.90	135.0
66.80	360.0
67.90	9650.0
68.90	9835.0
69.90	756.0
71.80	580.0
72.90	4487.0
73.90	17584.0
74.90	53336.0
75.90	4470.0
76.90	596.0
77.90	385.0
78.80	4651.0
79.80	1256.0
80.80	4642.0
81.80	881.0
82.90	110.0
86.90	3942.0
87.90	4519.0
90.90	377.0
91.90	3107.0
92.90	4713.0
93.90	13187.0
94.90	101728.0
95.90	6780.0
96.90	230.0
103.90	477.0
104.80	193.0
105.70	329.0
106.80	101.0
107.70	111.0
109.70	117.0
110.80	118.0
112.60	144.0
114.80	112.0
115.70	438.0
116.80	973.0
117.80	536.0
118.80	973.0
127.70	356.0
128.90	155.0
129.70	315.0
130.70	158.0
136.70	212.0
140.80	1276.0
141.60	147.0
142.80	2256.0
143.90	146.0
144.80	1333.0
145.80	211.0
147.80	267.0
149.90	145.0
152.60	100.0
154.70	294.0
156.80	299.0
158.70	157.0
160.80	179.0
170.90	551.0
171.80	1159.0
172.80	1701.0
173.80	86112.0
174.80	7244.0
175.80	84592.0
176.80	5259.0
177.80	127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB193