


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU090518\
 Data File : VU026527.D
 Acq On : 05 Sep 2018 07:17
 Operator : MD/SY
 Sample : BFB49
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB49

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis
 Last Update : Thu Sep 06 05:59:28 2018

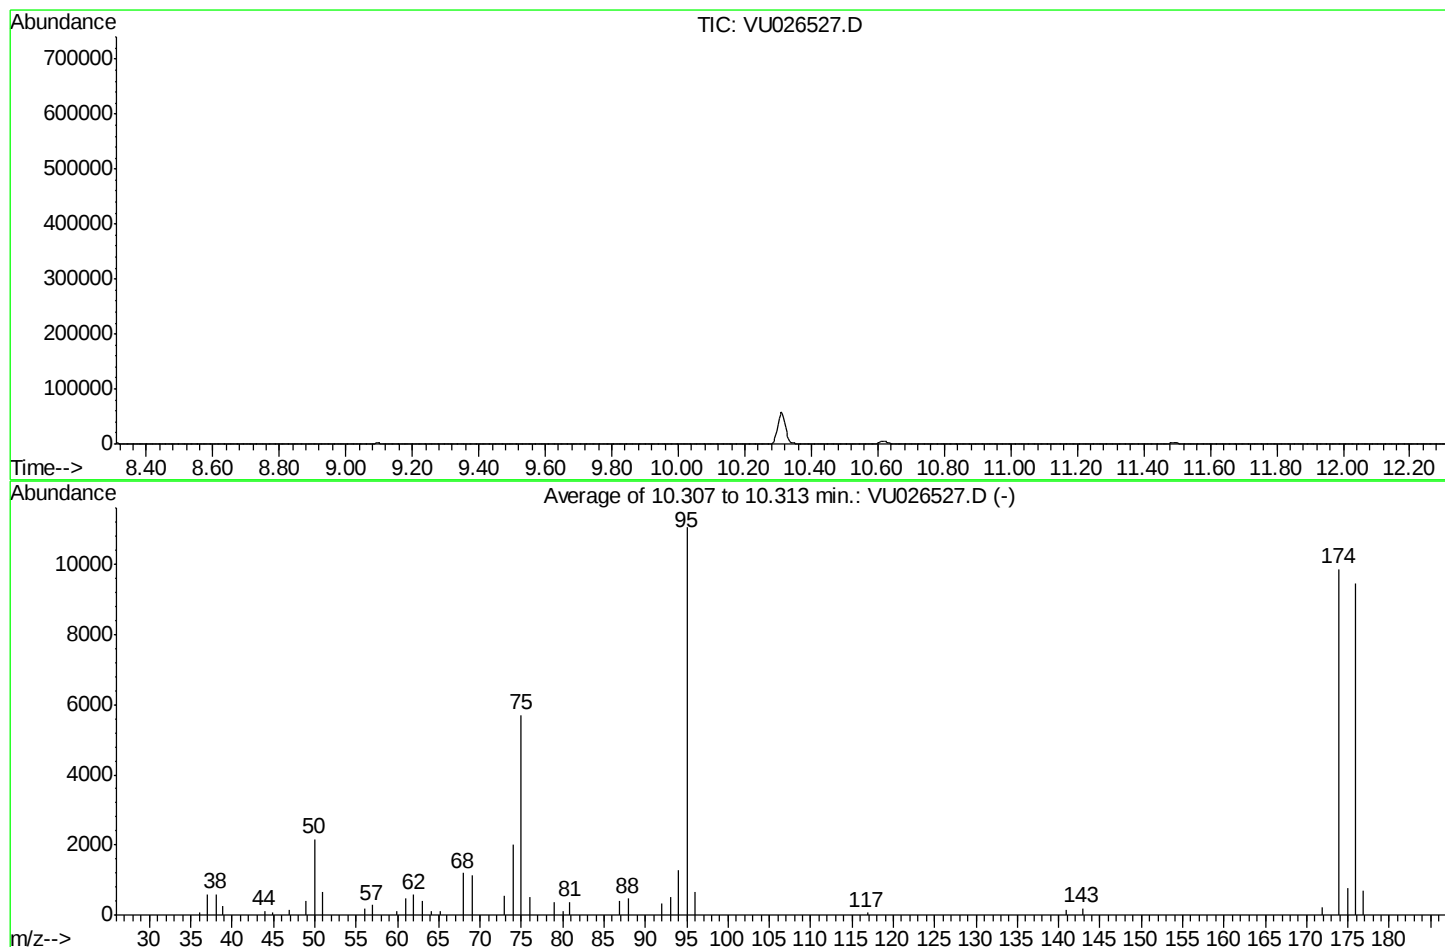

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3012

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	2156	PASS
75	95	30	80	51.5	5699	PASS
95	95	100	100	100.0	11061	PASS
96	95	5	9	6.0	662	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	89.2	9864	PASS
175	174	5	9	7.8	771	PASS
176	174	95	101	95.9	9458	PASS
177	176	5	9	7.2	682	PASS

m/z	Abundance
43.90	153.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
37.00	561.0
38.00	603.0
38.90	234.0
43.90	286.0
47.00	114.0
49.00	393.0
50.00	2161.0
51.00	664.0
56.00	159.0
57.00	266.0
59.90	103.0
61.00	482.0
62.00	570.0
63.00	393.0
64.10	105.0
65.10	120.0
68.00	1193.0
69.00	1159.0
72.90	506.0
74.00	2053.0
75.00	5675.0
76.00	538.0
78.90	386.0
80.00	115.0
80.80	392.0
86.90	391.0
87.90	432.0
92.00	320.0
93.00	494.0
94.00	1227.0
95.00	10787.0
96.00	620.0
140.90	132.0
142.80	179.0
171.90	216.0
173.90	9545.0
175.00	775.0
175.90	8920.0
176.90	658.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
36.00	103.0
37.00	619.0
38.00	603.0
38.90	274.0
43.90	257.0
44.80	101.0
46.90	142.0
48.90	393.0
50.00	2218.0
51.00	652.0
56.00	193.0
57.00	298.0
60.00	114.0
61.00	492.0
62.00	593.0
63.00	415.0
64.00	122.0
65.10	123.0
68.00	1194.0
69.00	1156.0
73.00	555.0
74.00	2065.0
75.00	5942.0
76.00	555.0
78.90	365.0
80.00	128.0
80.90	389.0
86.90	427.0
87.90	491.0
92.00	326.0
93.00	523.0
94.00	1302.0
95.00	11374.0
96.00	676.0
116.90	115.0
140.90	159.0
142.90	199.0
171.90	220.0
173.90	10229.0
175.00	798.0
175.90	9701.0
176.90	704.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
36.00	114.0
37.00	569.0
38.00	559.0
38.90	255.0
43.90	251.0
44.90	100.0
46.90	135.0
49.00	417.0
50.00	2089.0
51.00	608.0
56.00	205.0
56.90	306.0
59.90	111.0
61.00	483.0
62.00	562.0
63.00	422.0
64.00	124.0
65.10	124.0
67.90	1196.0
69.00	1088.0
73.00	539.0
74.00	1864.0
75.00	5481.0
76.00	487.0
78.90	347.0
80.00	115.0
80.90	370.0
86.90	436.0
87.90	492.0
92.00	331.0
93.00	531.0
94.00	1268.0
95.00	11024.0
96.00	692.0
116.90	103.0
140.90	155.0
142.90	189.0
171.90	230.0
173.90	9820.0
175.00	740.0
175.90	9753.0
176.90	685.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49