

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090519\
 Data File : VU034253.D
 Acq On : 04 Sep 2019 13:24
 Operator : JC/SP
 Sample : K4546-40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 T3-S-B4-(2.5)

Quant Time: Sep 05 04:48:11 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 29 04:11:12 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.96	168	425964	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.87	114	677395	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.07	117	676496	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.46	152	326112	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.29	65	258638	47.39	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.78%	
35) Dibromofluoromethane	4.86	113	222759	47.41	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.82%	
50) Toluene-d8	7.55	98	875010	49.74	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.48%	
62) 4-Bromofluorobenzene	10.29	95	307558	44.94	ug/l	0.00
Spiked Amount 50.000			Recovery	=	89.88%	
Target Compounds						
20) Methylene Chloride	2.69	84	5262	0.998	ug/l	96
43) Isopropyl Acetate	5.53	43	42037	3.851	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU090519\
Data File : VU034253.D
Acq On : 04 Sep 2019 13:24
Operator : JC/SP
Sample : K4546-40
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
T3-S-B4-(2.5)

Quant Time: Sep 05 04:48:11 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 29 04:11:12 2019
Response via : Initial Calibration

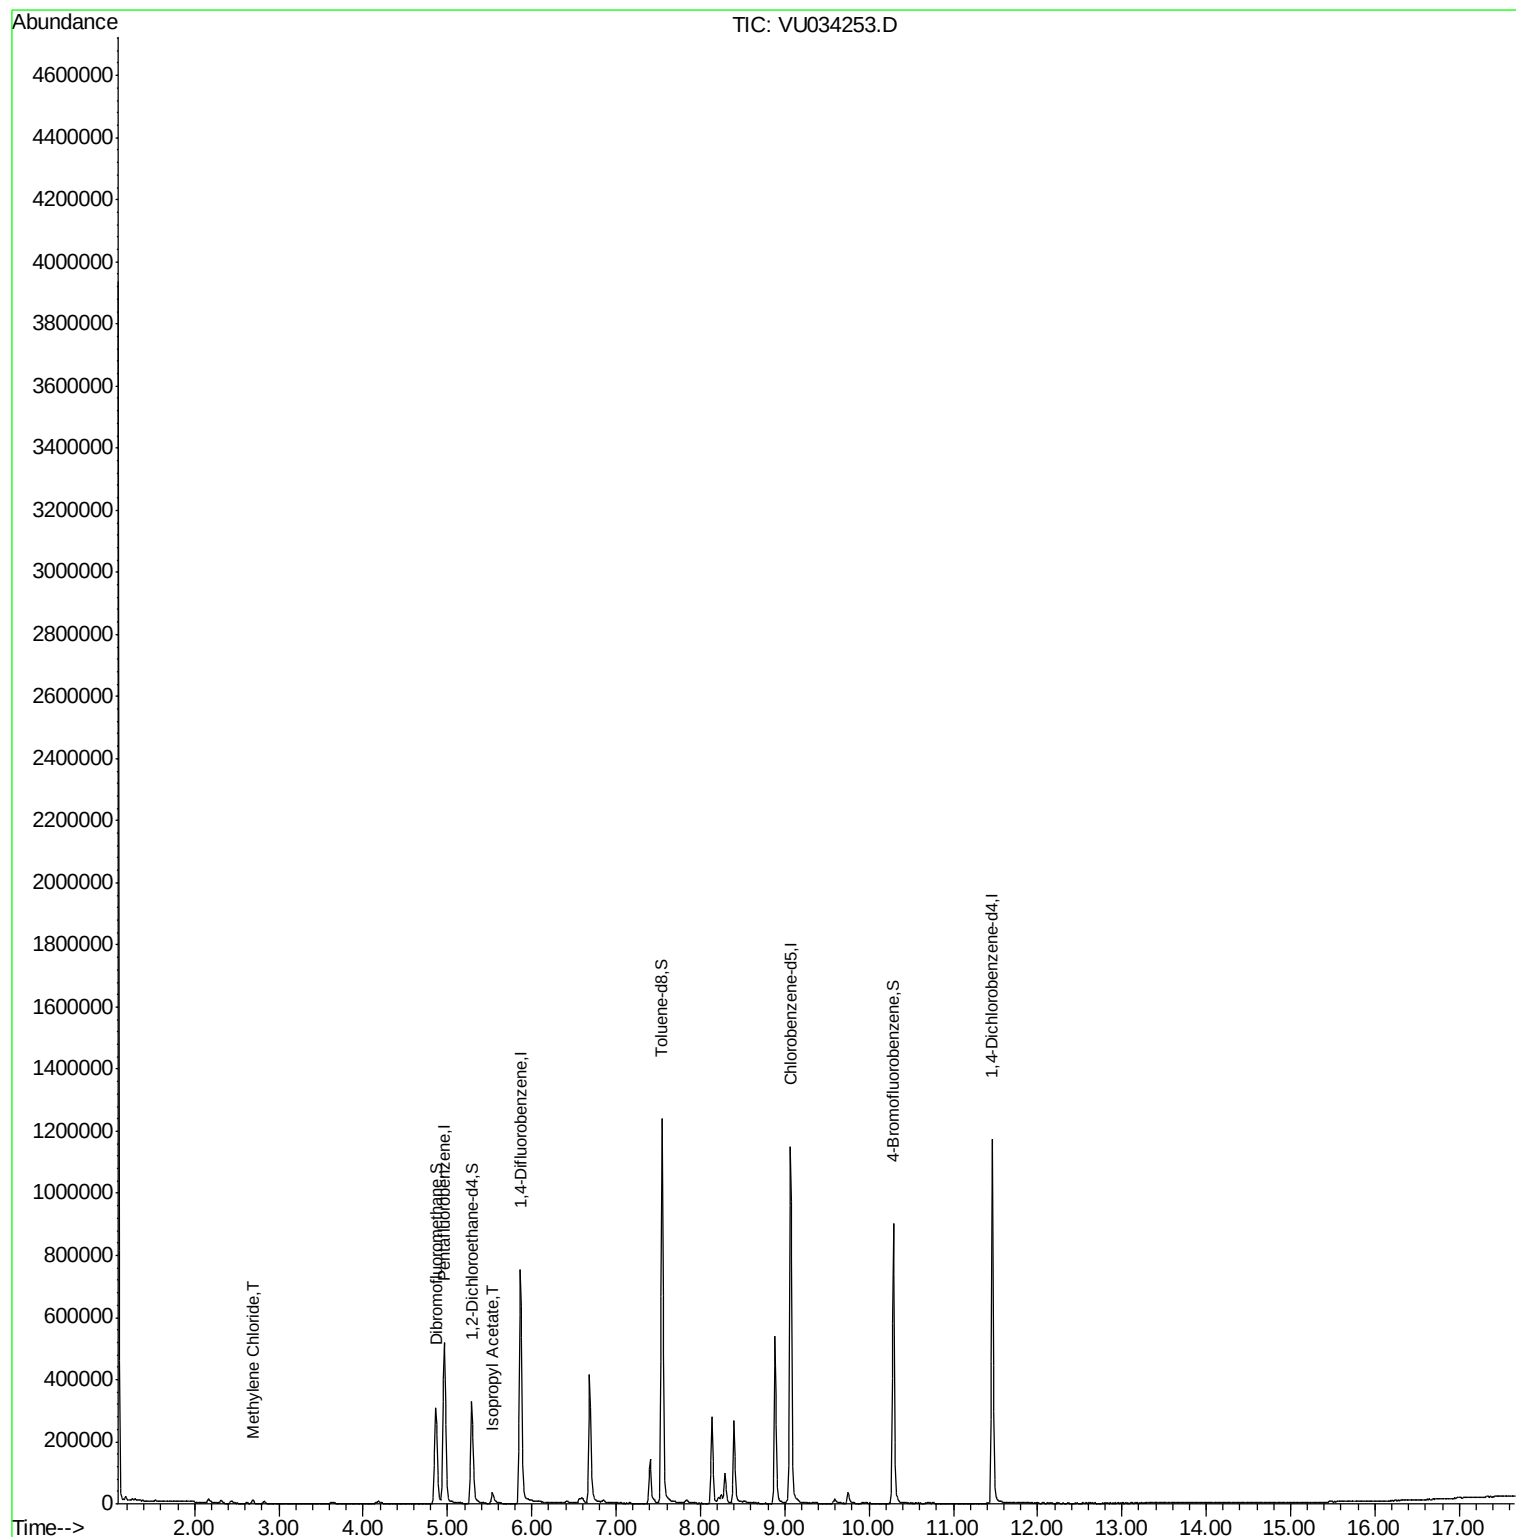

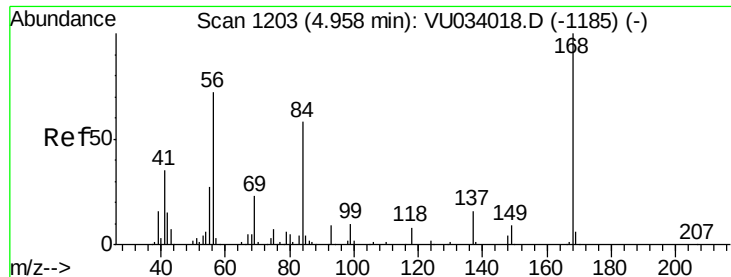

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.96 min Scan# 1204

Delta R.T. 0.00 min

Lab File: VU034253.D

Acq: 04 Sep 2019 13:24

Instrument :

MSVOA_U

ClientSampleId :


T3-S-B4-(2.5)

Tot Ion:168 Resp: 425964

Ion Ratio Lower Upper

168 100

99 52.9 42.3 63.5

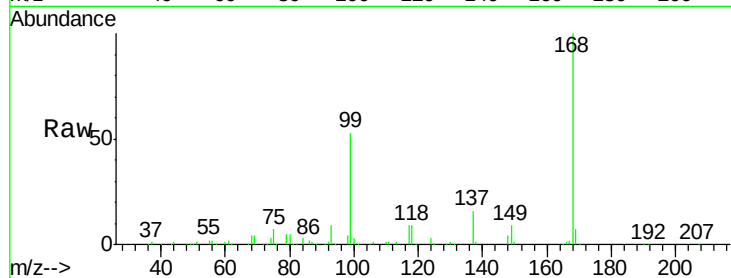

Abundance Ion 167.90 (167.60 to 168.60): VU034018.D (-1185) (-)

Ion 98.90 (98.60 to 99.60): VU034018.D (-1185) (-)

4.96

200000



150000

100000

50000

0

Time-->

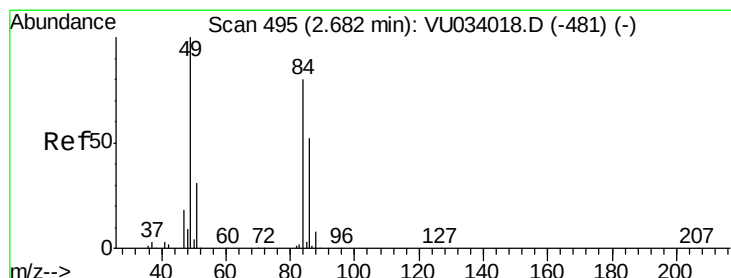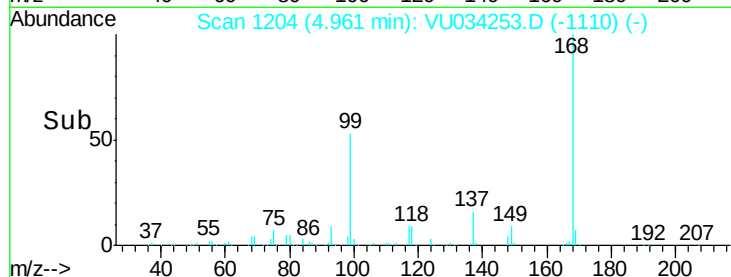

#20

Methylene Chloride

Concen: 0.998 ug/l

RT: 2.69 min Scan# 498

Delta R.T. 0.01 min

Lab File: VU034253.D

Acq: 04 Sep 2019 13:24

Tgt Ion: 84 Resp: 5262


Ion Ratio Lower Upper

84 100

49 122.8 100.2 150.4

51 41.2 30.8 46.2

86 61.1 52.5 78.7

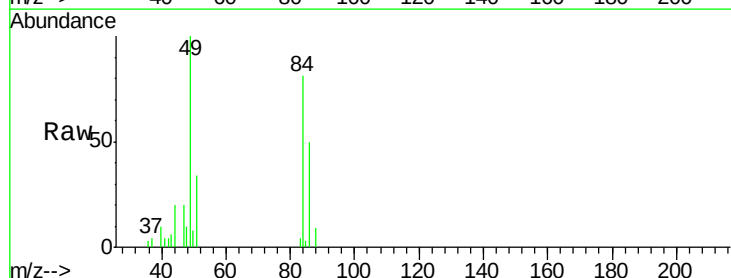

Abundance Ion 83.90 (83.60 to 84.60): VU034018.D (-481) (-)

Ion 48.90 (48.60 to 49.60): VU034018.D (-481) (-)

Ion 50.90 (50.60 to 51.60): VU034018.D (-481) (-)

Ion 85.90 (85.60 to 86.60): VU034018.D (-481) (-)

5000

4000


3000


2000

1000

0

Time-->

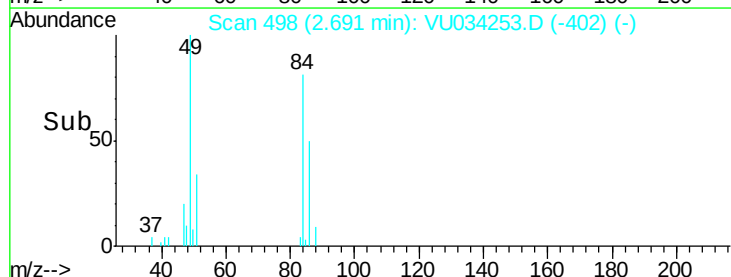

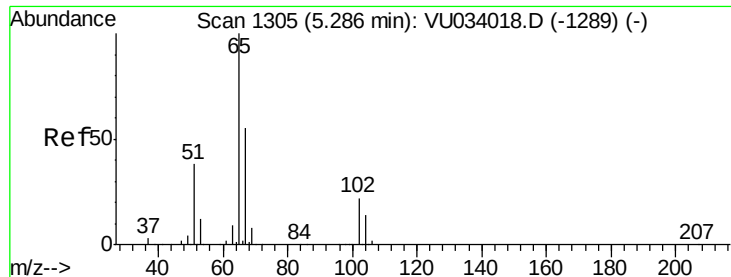

#33

1,2-Dichloroethane-d4

Concen: 47.387 ug/l

RT: 5.29 min Scan# 1306

Delta R.T. 0.00 min

Lab File: VU034253.D

Acq: 04 Sep 2019 13:24

Instrument :

MSVOA_U

ClientSampleId :


T3-S-B4-(2.5)

Tot Ion: 65 Resp: 258638

Ion Ratio Lower Upper




65 100

67 56.0 0.0 110.6

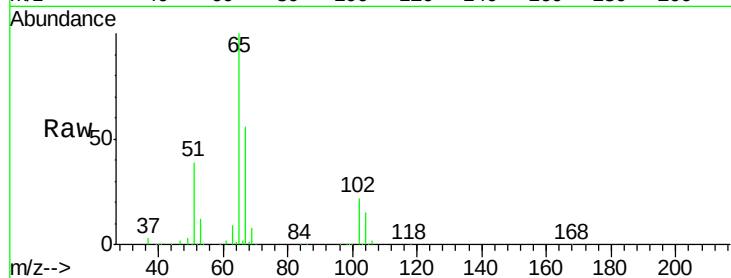

Abundance Ion 64.90 (64.60 to 65.60): VU034018.D (-1289) (-)

Ion 66.90 (66.60 to 67.60): VU034018.D (-1289) (-)

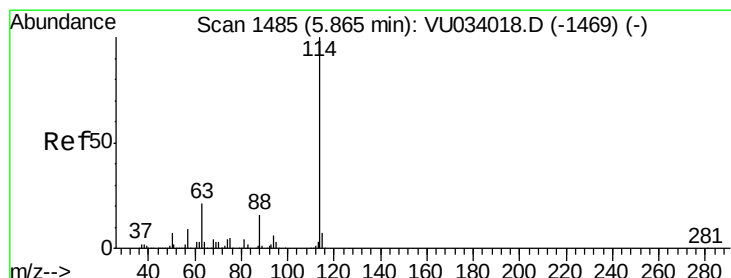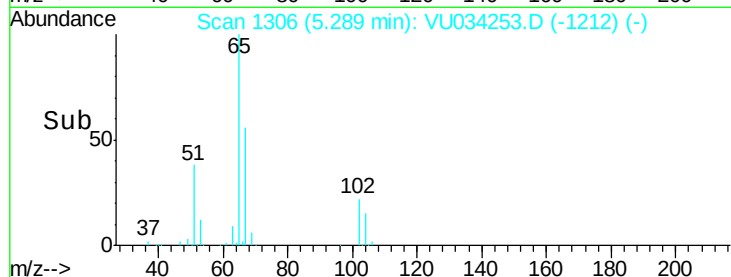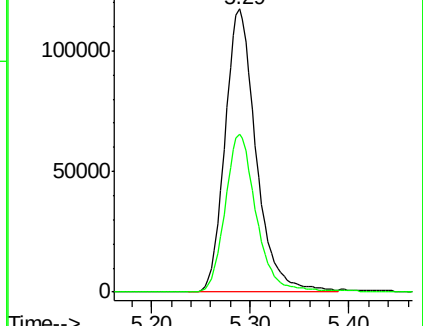

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.87 min Scan# 1486

Delta R.T. 0.00 min

Lab File: VU034253.D

Acq: 04 Sep 2019 13:24


Tgt Ion: 114 Resp: 677395

Ion Ratio Lower Upper

114 100

63 21.2 0.0 42.0



88 15.9 0.0 32.0

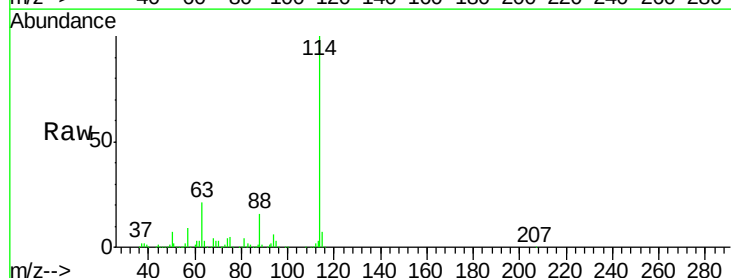


Abundance Ion 113.90 (113.60 to 114.60): VU034018.D (-1469) (-)

Ion 63.00 (62.70 to 63.70): VU034018.D (-1469) (-)

Ion 87.90 (87.60 to 88.60): VU034018.D (-1469) (-)



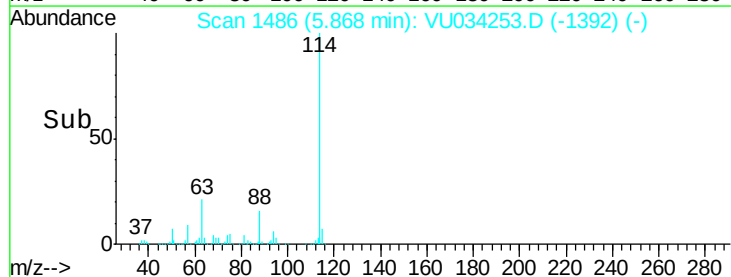
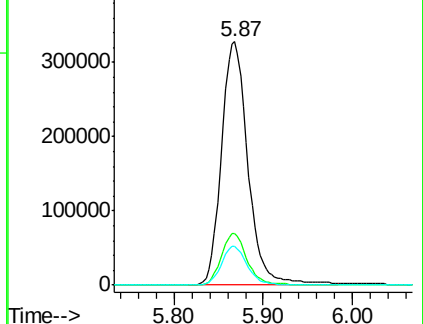


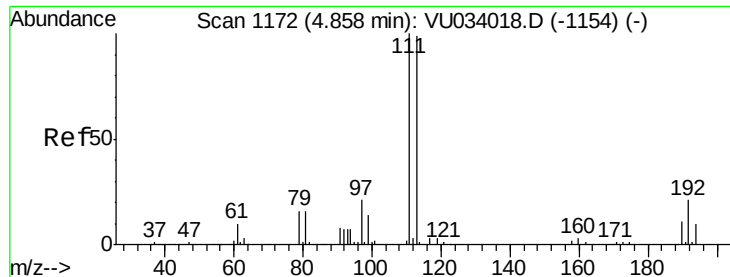

#35
 Dibromofluoromethane
 Concen: 47.412 ug/l
 RT: 4.86 min Scan# 1173
 Delta R.T. 0.00 min
 Lab File: VU034253.D
 Acq: 04 Sep 2019 13:24




Instrument :
 MSVOA_U
 ClientSampleId :
 T3-S-B4-(2.5)


Tot Ion	Ratio	Lower	Upper
113	100		
111	102.3	81.7	122.5
192	21.5	17.1	25.7

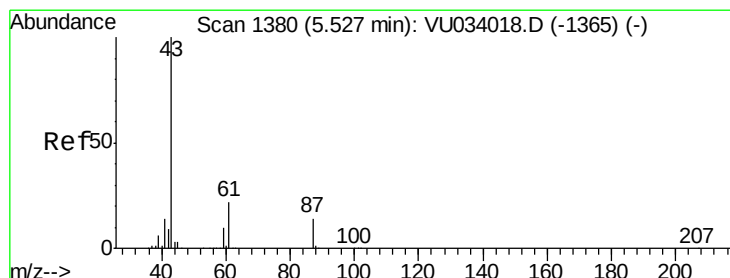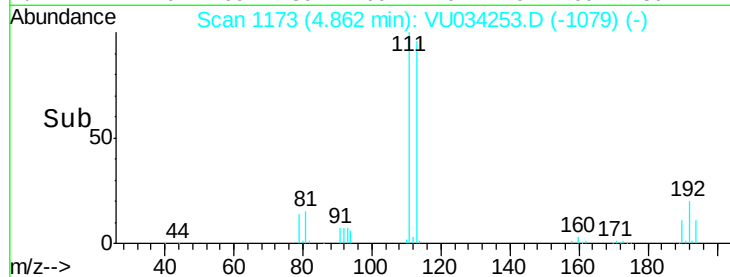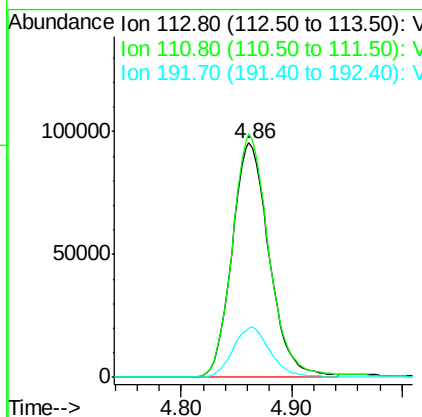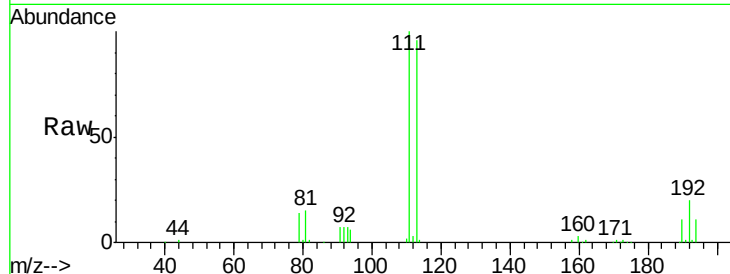

#43
 Isopropyl Acetate
 Concen: 3.851 ug/l
 RT: 5.53 min Scan# 1382
 Delta R.T. 0.01 min
 Lab File: VU034253.D
 Acq: 04 Sep 2019 13:24

Tgt Ion	Ratio	Lower	Upper
43	100		
61	20.4	17.2	25.8
87	13.1	10.8	16.2

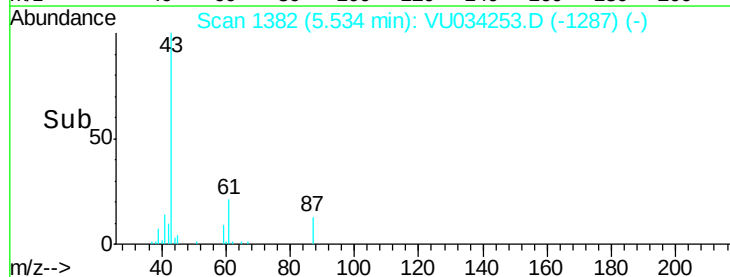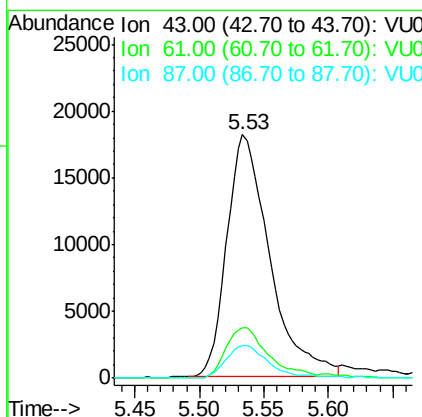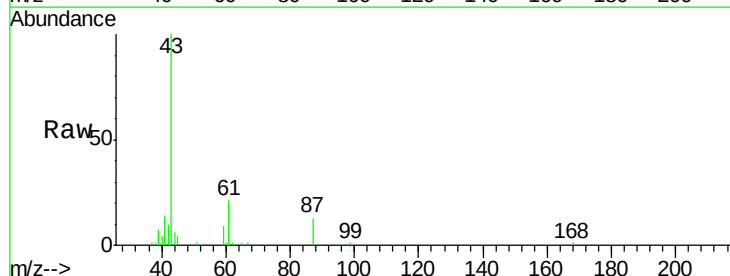

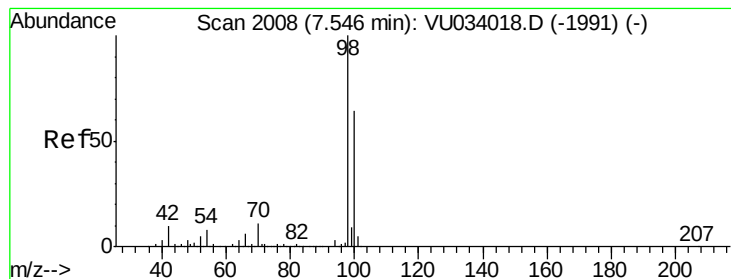

#50

Toluene-d8

Concen: 49.738 ug/l

RT: 7.55 min Scan# 2008

Delta R.T. -0.00 min

Lab File: VU034253.D

Acq: 04 Sep 2019 13:24

Instrument :

MSVOA_U

ClientSampleId :


T3-S-B4-(2.5)

Tot Ion: 98 Resp: 875010

Ion Ratio Lower Upper

98 100

100 64.7 50.3 75.5

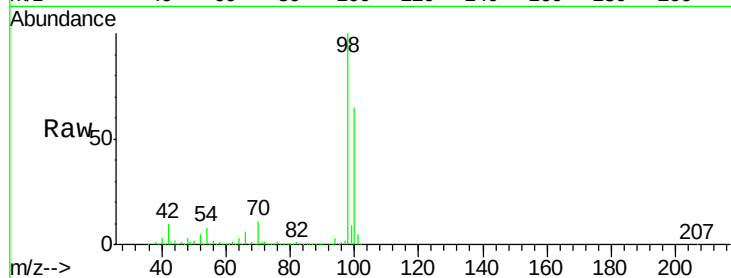

Abundance Ion 98.00 (97.70 to 98.70): VU034018.D (-1991) (-)

Ion 100.00 (99.70 to 100.70): VU034018.D (-1991) (-)

7.55

500000

400000

300000



200000

100000

0

7.50 7.55 7.60 7.70

Time-->

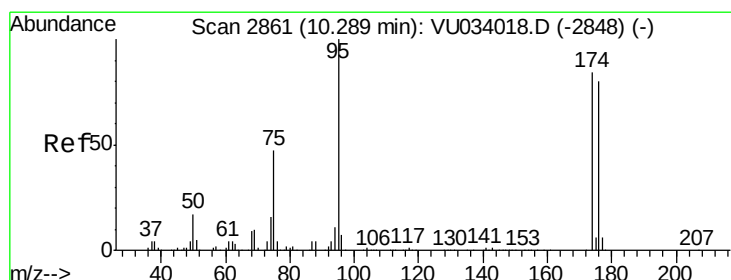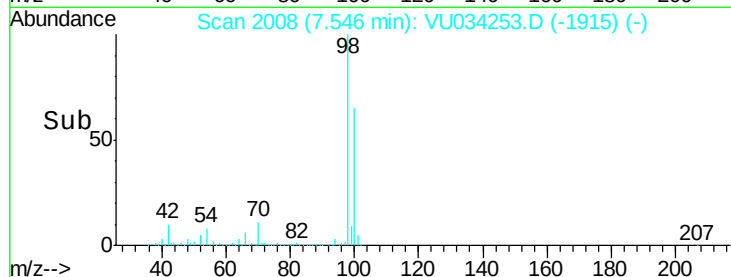

#62

4-Bromofluorobenzene

Concen: 44.943 ug/l

RT: 10.29 min Scan# 2861

Delta R.T. -0.00 min

Lab File: VU034253.D

Acq: 04 Sep 2019 13:24


Tgt Ion: 95 Resp: 307558

Ion Ratio Lower Upper

95 100

174 86.1 0.0 168.8

176 83.0 0.0 161.8

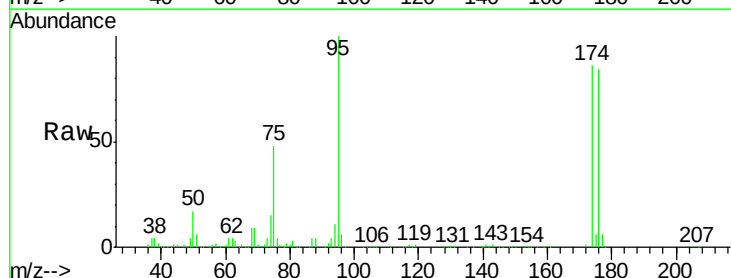

Abundance Ion 94.90 (94.60 to 95.60): VU034018.D (-2848) (-)

Ion 173.80 (173.50 to 174.50): VU034018.D (-2848) (-)

Ion 175.80 (175.50 to 176.50): VU034018.D (-2848) (-)

250000

200000

150000


100000


50000

0

10.20 10.25 10.30 10.35 10.40

Time-->




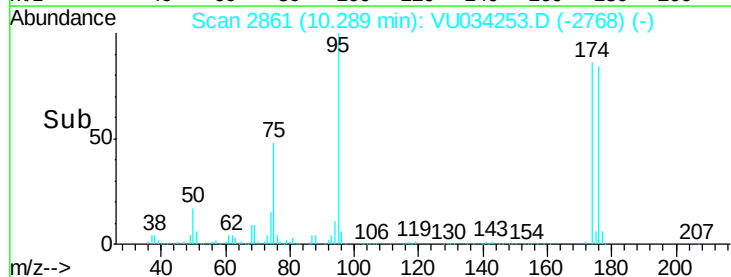


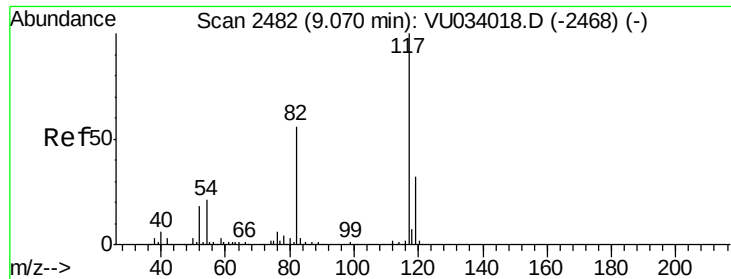

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.07 min Scan# 2482
Delta R.T. -0.00 min
Lab File: VU034253.D
Acq: 04 Sep 2019 13:24

Instrument :
MSVOA_U
ClientSampleId :
T3-S-B4-(2.5)

Tot Ion:117 Resp: 676496
Ion Ratio Lower Upper
117 100
82 56.4 45.1 67.7
119 32.4 25.4 38.0

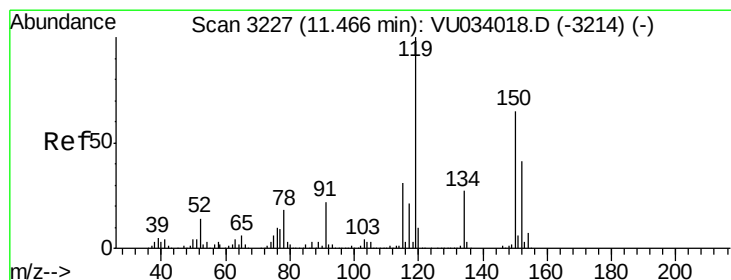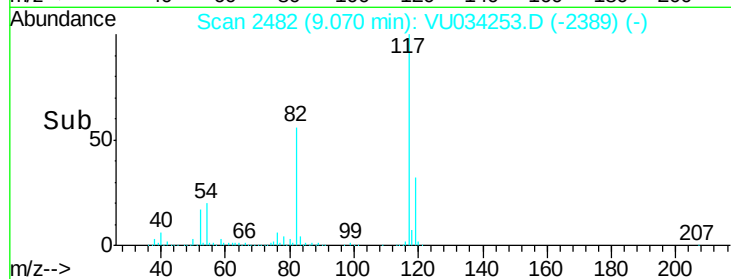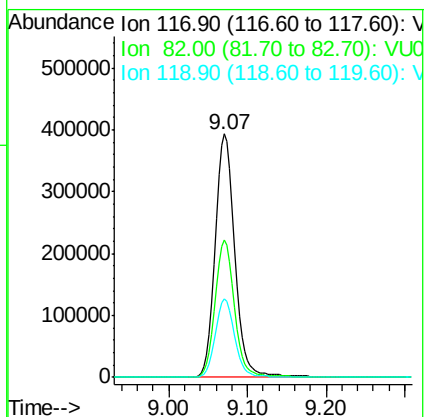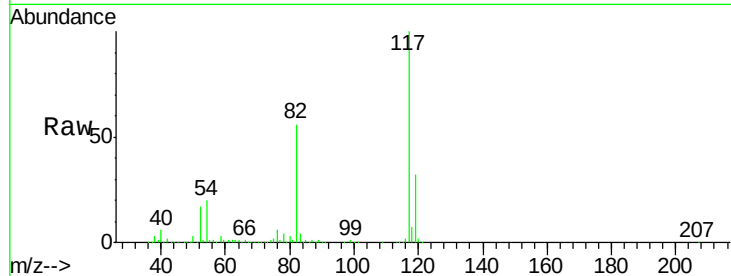

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.46 min Scan# 3226
Delta R.T. -0.00 min
Lab File: VU034253.D
Acq: 04 Sep 2019 13:24

Tgt Ion:152 Resp: 326112
Ion Ratio Lower Upper
152 100
115 57.8 41.1 123.3
150 157.4 0.0 348.8

